


Data Path : Z:\HPCHEM1\BNA F\Data\BF102617\
 Data File : BF099855.D
 Acq On : 26 Oct 2017 11:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

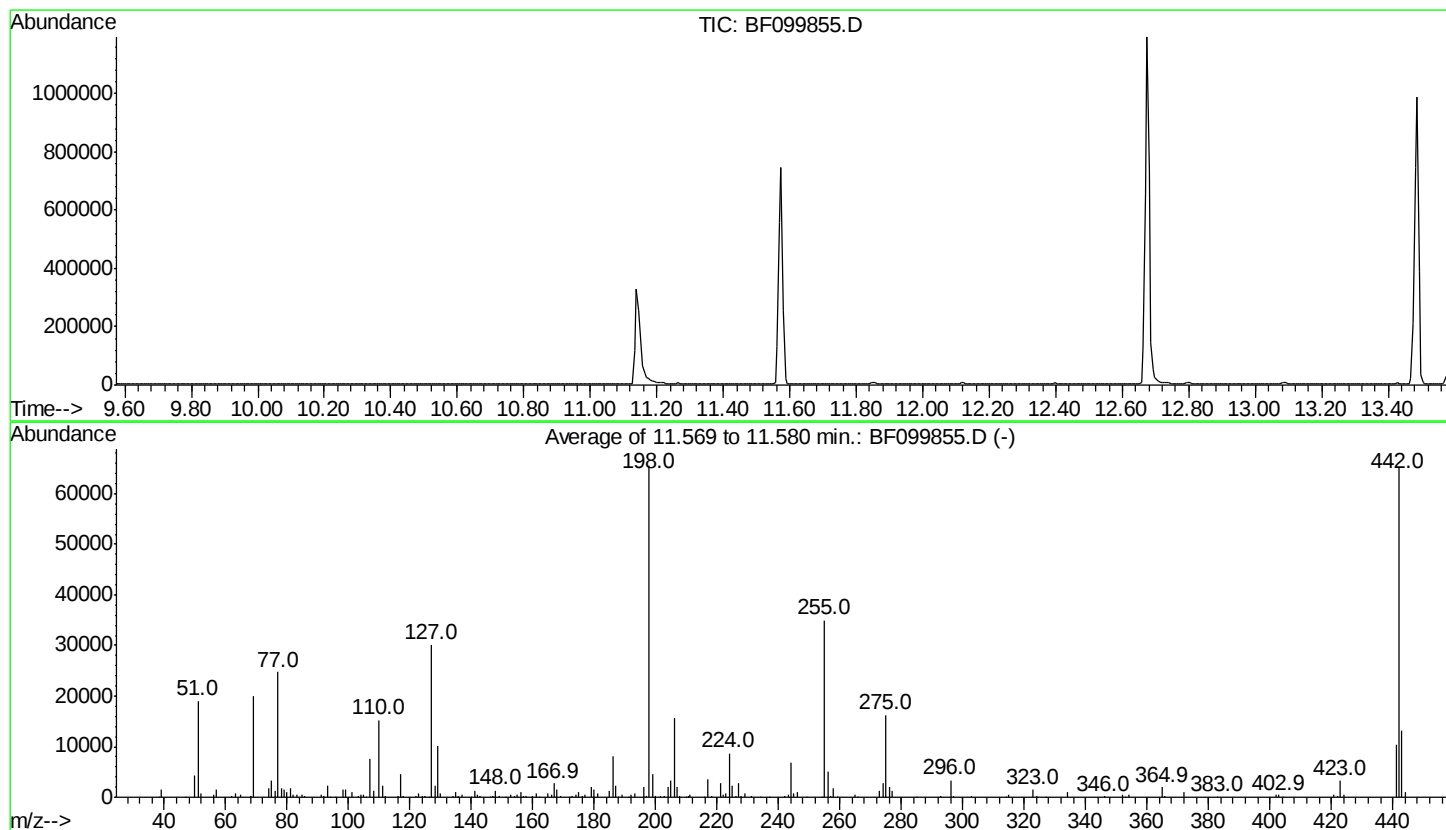

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	19082	PASS
68	69	0.00	2	0.9	182	PASS
69	198	0.00	100	30.3	19892	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	30206	PASS
197	198	0.00	2	0.5	328	PASS
198	198	100	100	100.0	65552	PASS
199	198	5	9	6.9	4516	PASS
275	198	10	60	24.7	16199	PASS
365	198	1	100	3.0	1951	PASS
441	442	0.01	24	16.0	10424	PASS
442	198	50	100	99.5	65226	PASS
443	442	15	24	20.1	13109	PASS