


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
Data File : BF125934.D
Acq On : 26 Oct 2021 15:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 15:59:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 18:49:16 2021
Response via : Initial Calibration

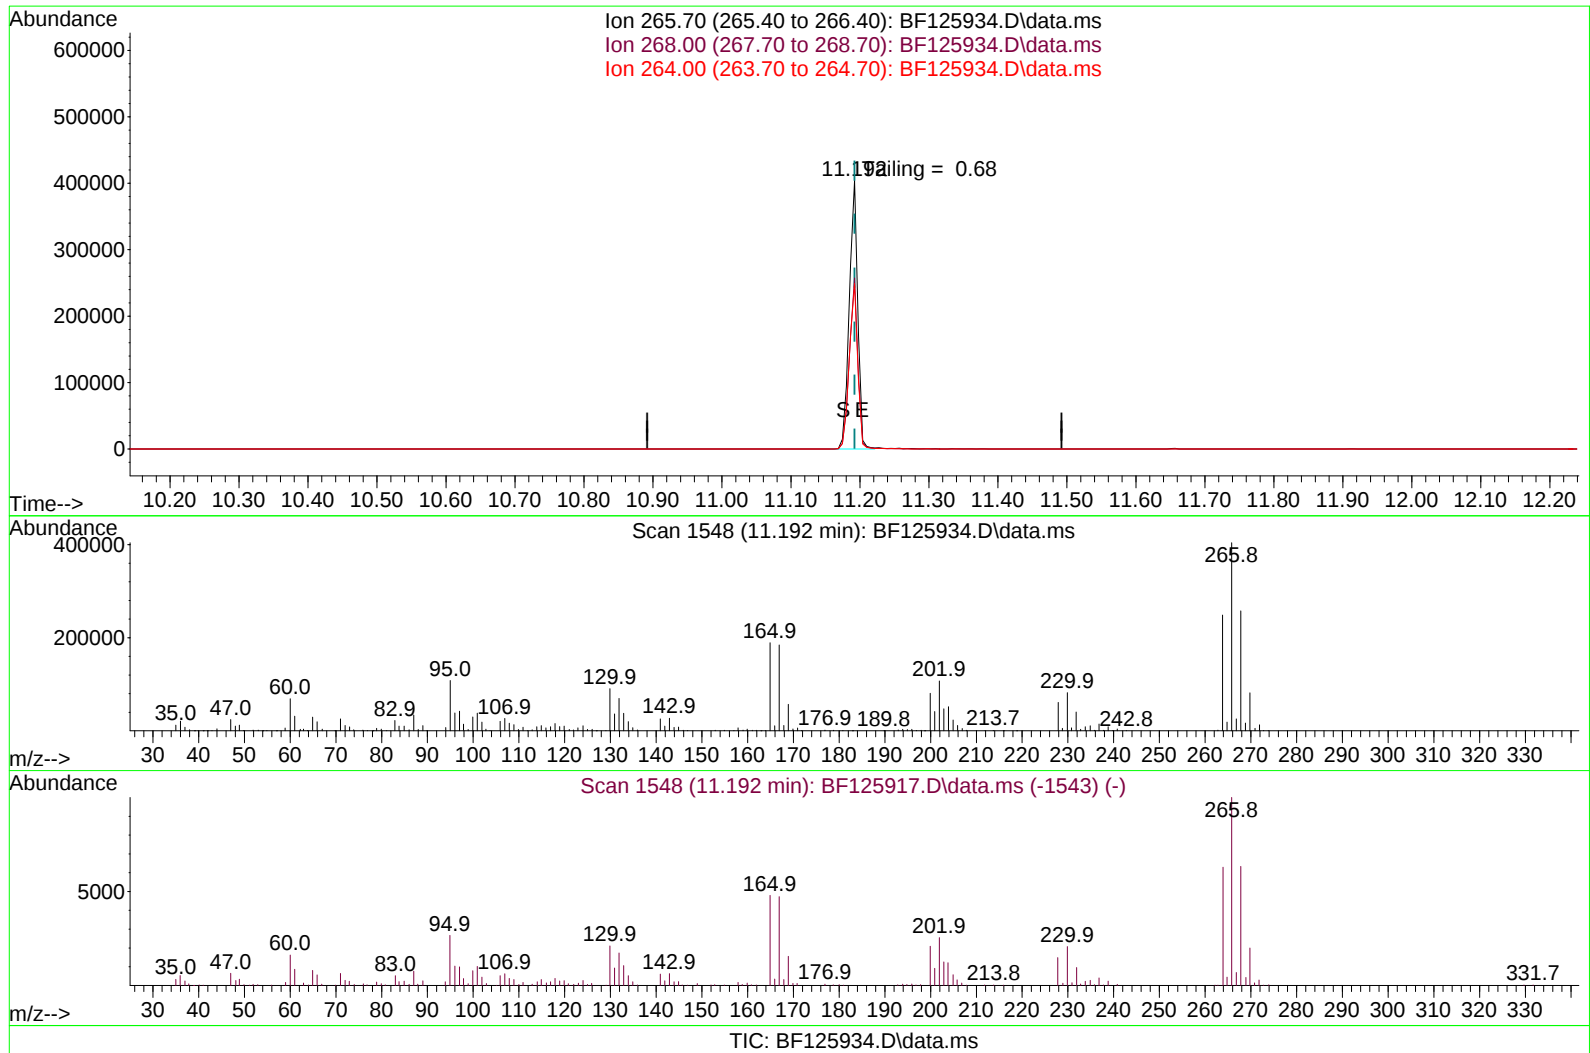

(70) Pentachlorophenol (C)




11.192min (+ 0.000) 35278.80 ng

response 347667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.77
264.00	69.90	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
Data File : BF125934.D
Acq On : 26 Oct 2021 15:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 15:59:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 18:49:16 2021
Response via : Initial Calibration

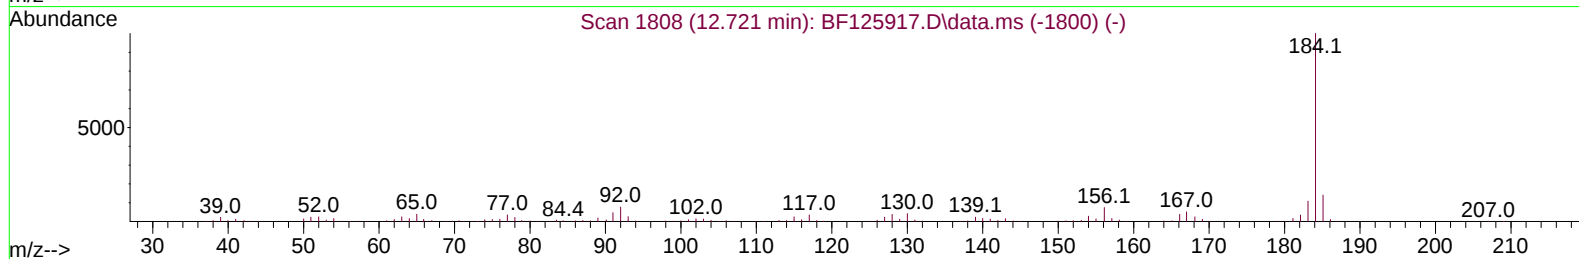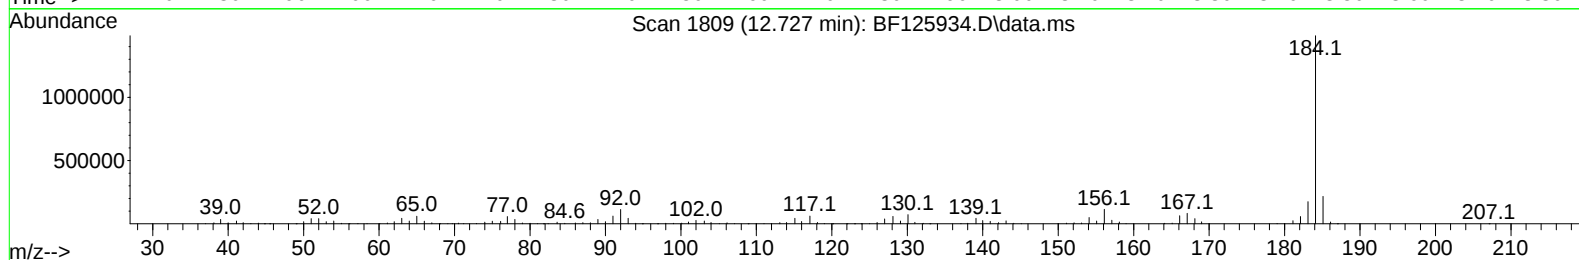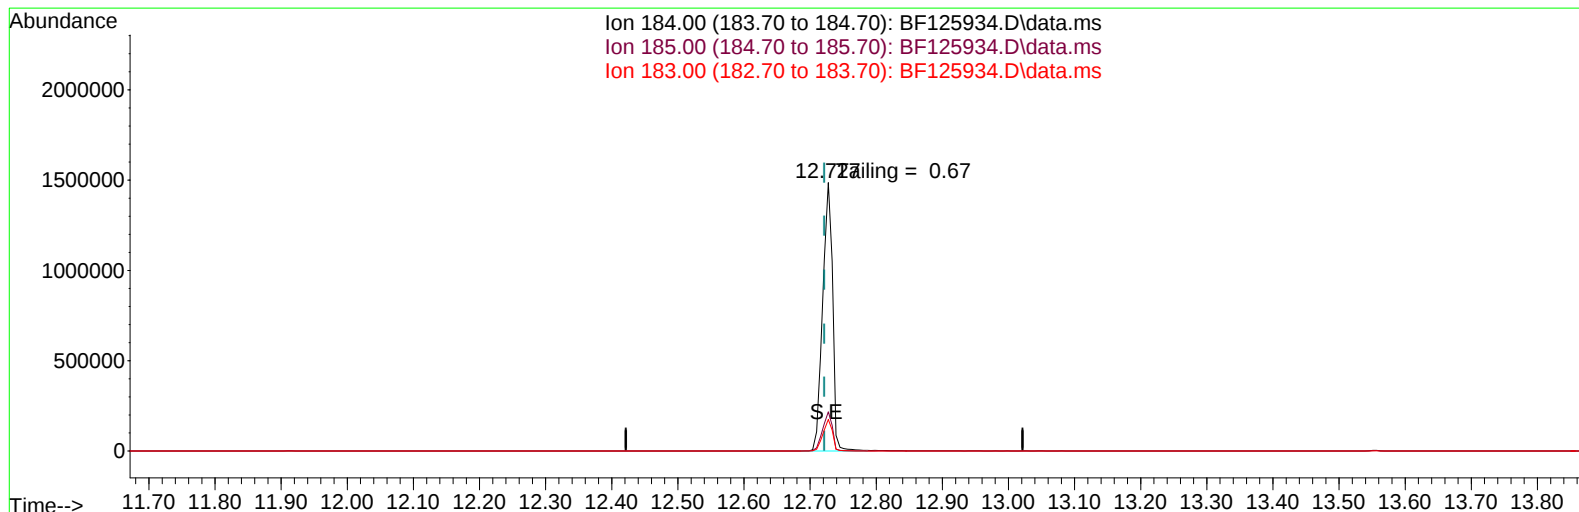

TIC: BF125934.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 1561530

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.61
183.00	10.10	11.74
0.00	0.00	0.00