


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
 Data File : BF125923.D
 Acq On : 26 Oct 2021 8:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 25 18:49:16 2021

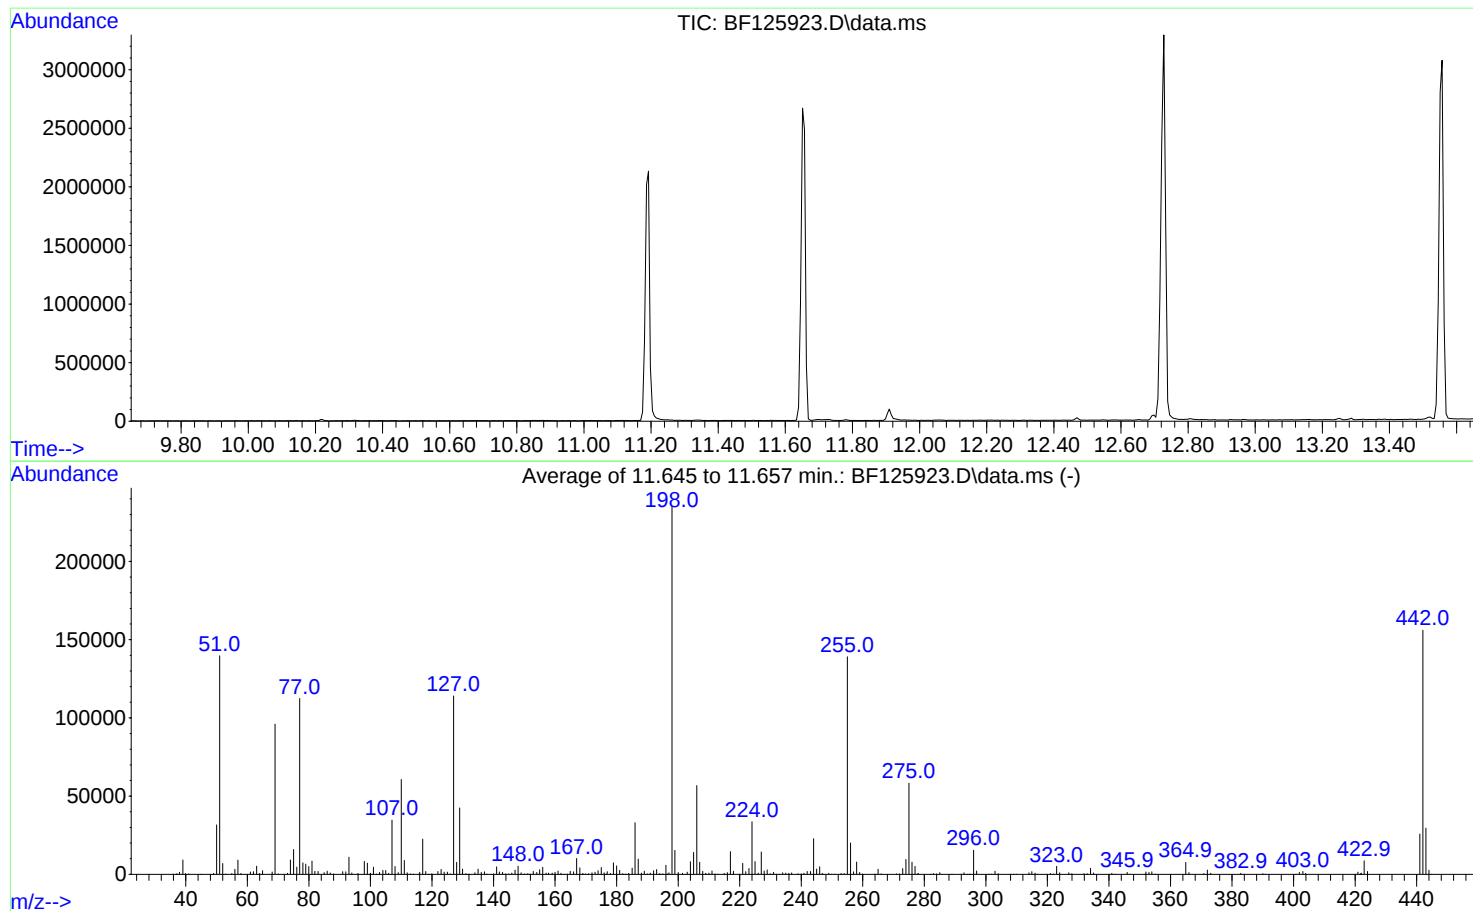




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.4	139699	PASS
68	69	0.00	2	1.6	1566	PASS
69	198	0.00	100	40.9	96051	PASS
70	69	0.00	2	0.3	269	PASS
127	198	10	80	48.5	114045	PASS
197	198	0.00	2	0.4	977	PASS
198	198	100	100	100.0	235107	PASS
199	198	5	9	6.5	15304	PASS
275	198	10	60	24.8	58315	PASS
365	198	1	100	3.3	7713	PASS
441	198	0.01	100	11.0	25794	PASS
442	442	50	100	100.0	156067	PASS
443	442	15	24	19.0	29576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
 Data File : BF125923.D
 Acq On : 26 Oct 2021 8:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 26 11:57:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 18:49:16 2021
 Response via : Initial Calibration

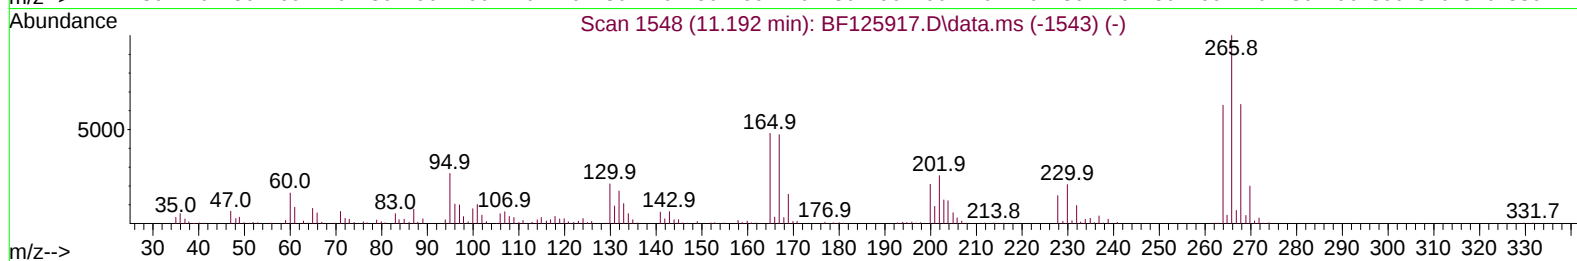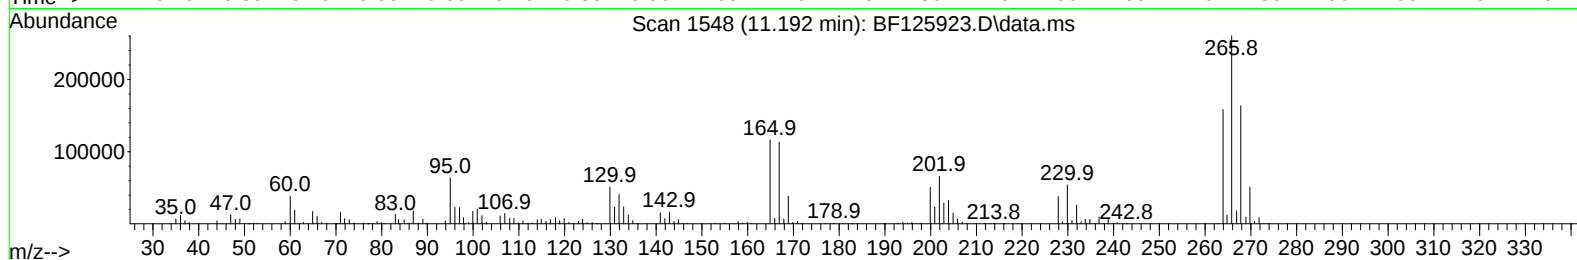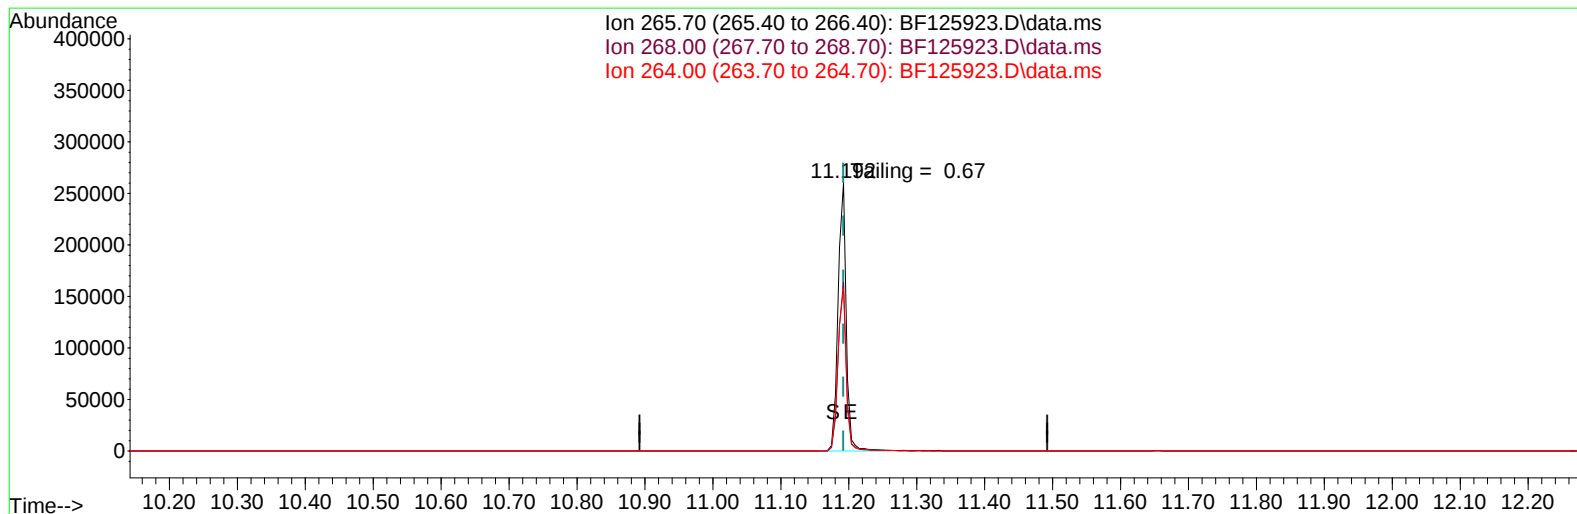

TIC: BF125923.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 227231.37 ng




response 218154

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.87
264.00	69.90	60.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
Data File : BF125923.D
Acq On : 26 Oct 2021 8:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 26 11:57:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 18:49:16 2021
Response via : Initial Calibration

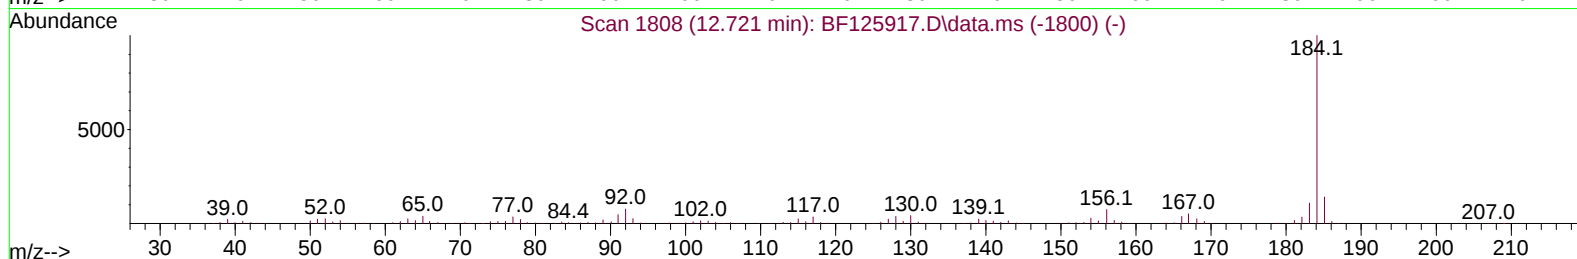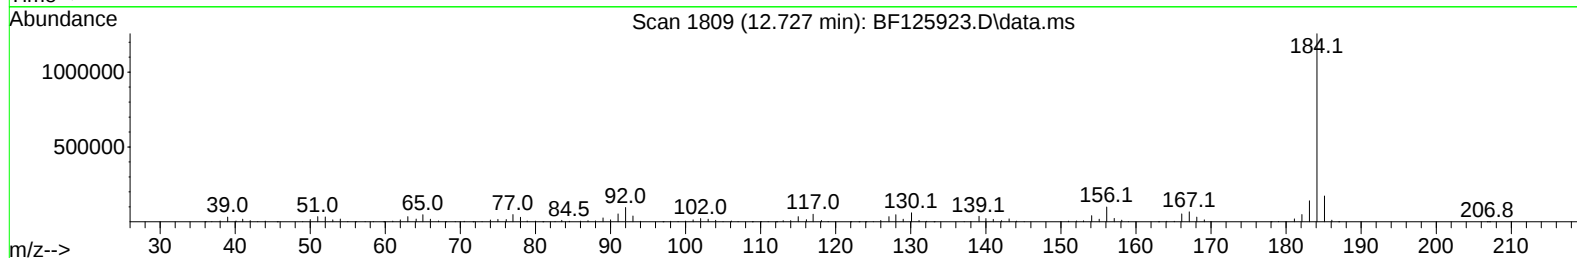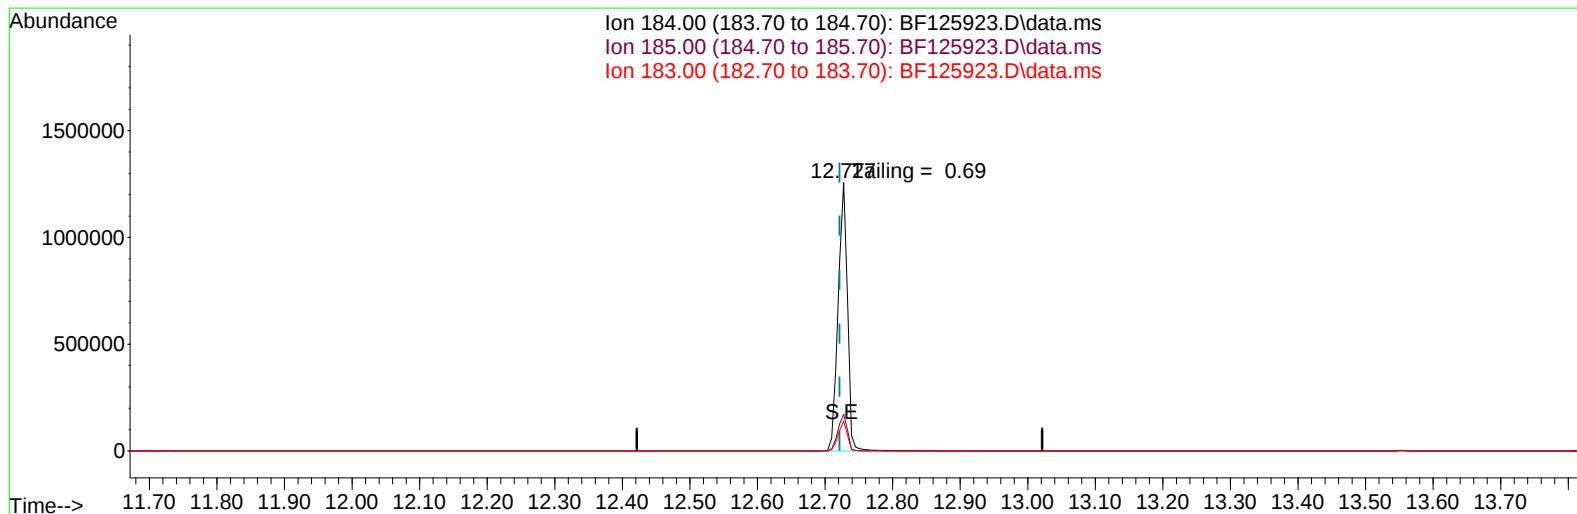

TIC: BF125923.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 72582.73 ng

response 1215801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.75
183.00	10.10	11.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2021	BNA_F	<u>BF125923.D</u>
Compound Name	Response	Retention Time
DDT	504334	13.55
DDD	1991	13.25
DDE	0	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1991	506325	0.39

Instrument :
BNA_F
ClientSampleId :
DFTPP