
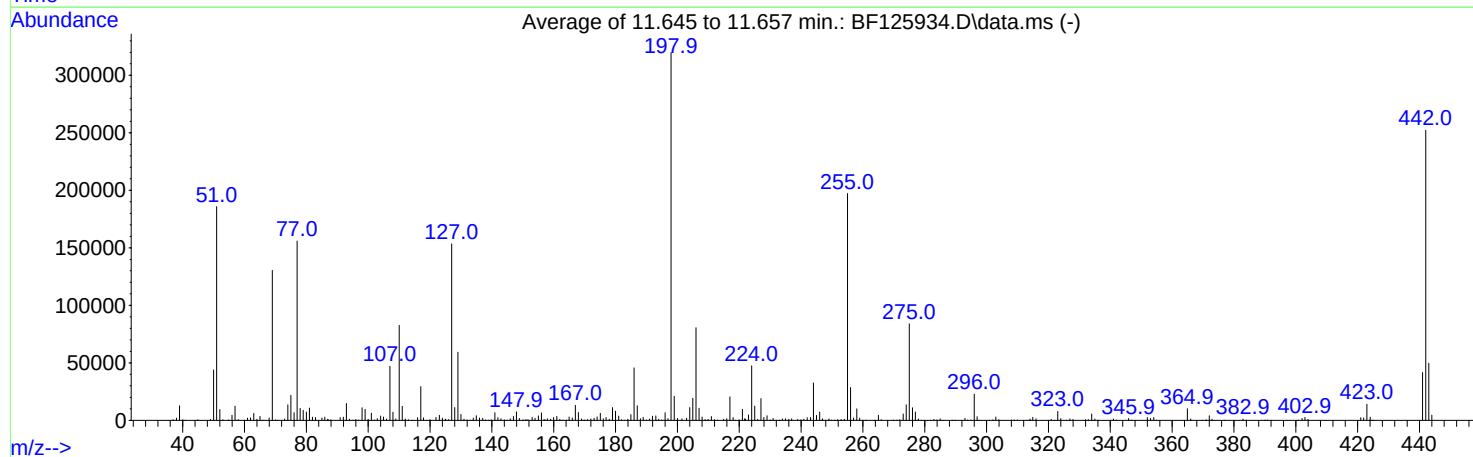


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
 Data File : BF125934.D
 Acq On : 26 Oct 2021 15:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 25 18:49:16 2021

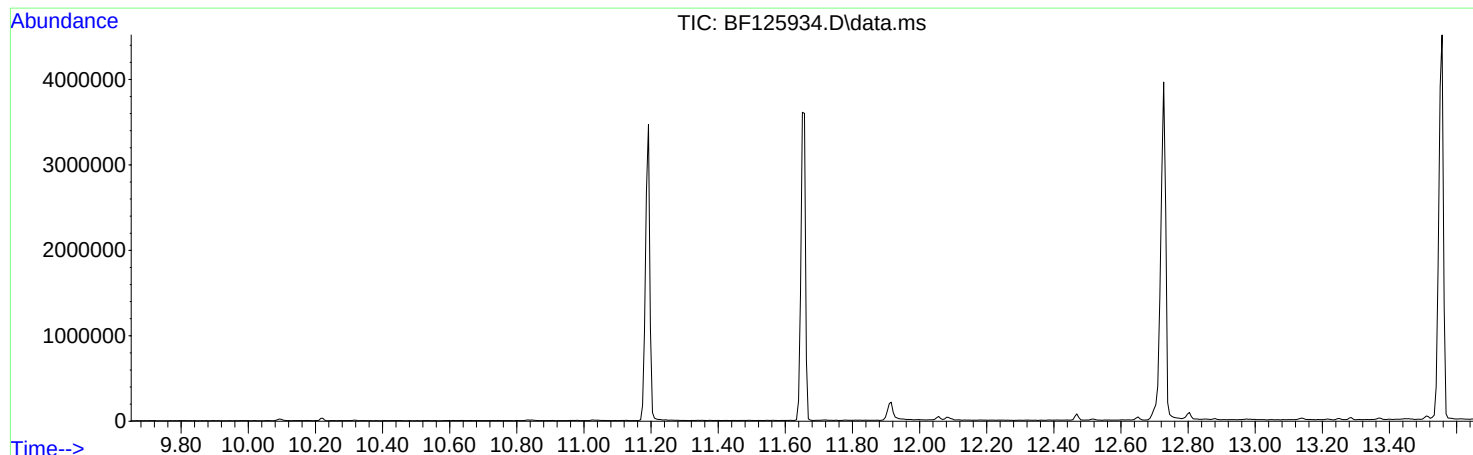




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	185899	PASS
68	69	0.00	2	1.6	2093	PASS
69	198	0.00	100	40.8	130408	PASS
70	69	0.00	2	0.3	408	PASS
127	198	10	80	48.0	153469	PASS
197	198	0.00	2	0.5	1545	PASS
198	198	100	100	100.0	319808	PASS
199	198	5	9	6.6	21021	PASS
275	198	10	60	26.2	83883	PASS
365	198	1	100	3.2	10229	PASS
441	198	0.01	100	13.0	41632	PASS
442	442	50	100	100.0	252203	PASS
443	442	15	24	19.7	49660	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
 Data File : BF125934.D
 Acq On : 26 Oct 2021 15:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 26 15:59:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 18:49:16 2021
 Response via : Initial Calibration

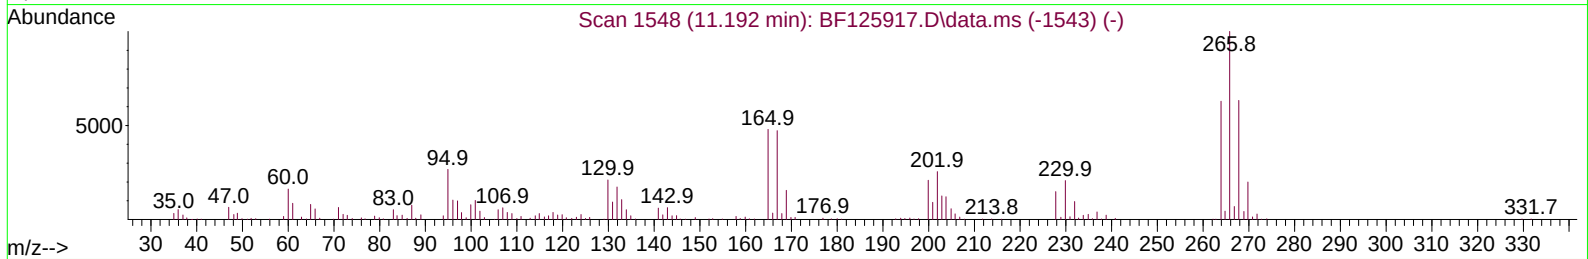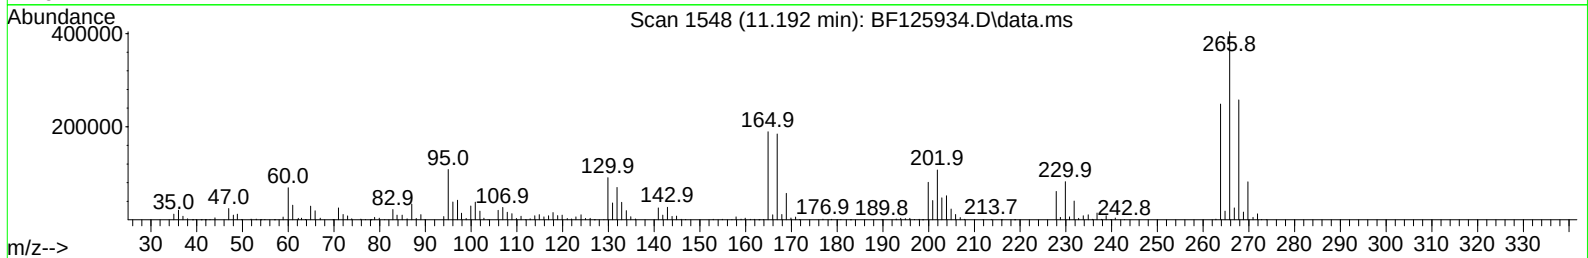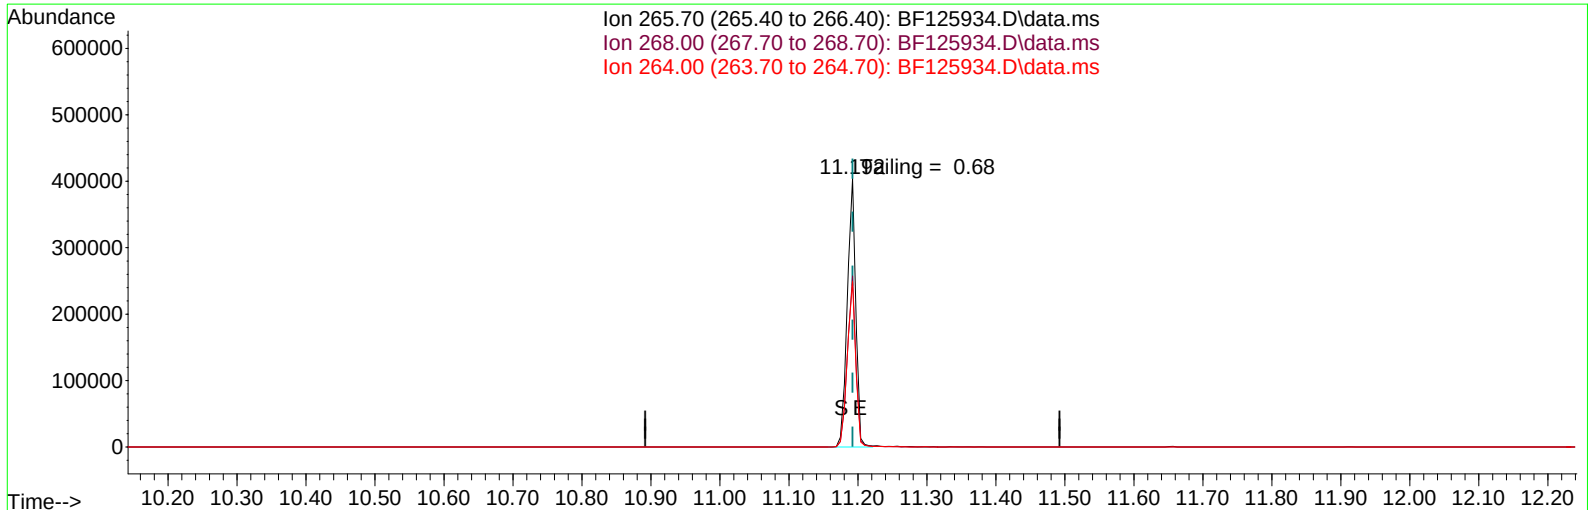

TIC: BF125934.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 35278.80 ng




response 347667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.77
264.00	69.90	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102621\
 Data File : BF125934.D
 Acq On : 26 Oct 2021 15:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 26 15:59:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 18:49:16 2021
 Response via : Initial Calibration

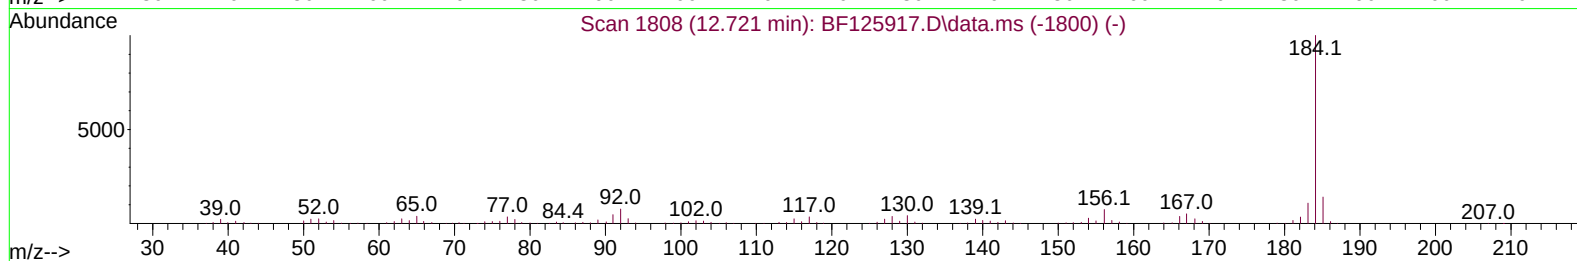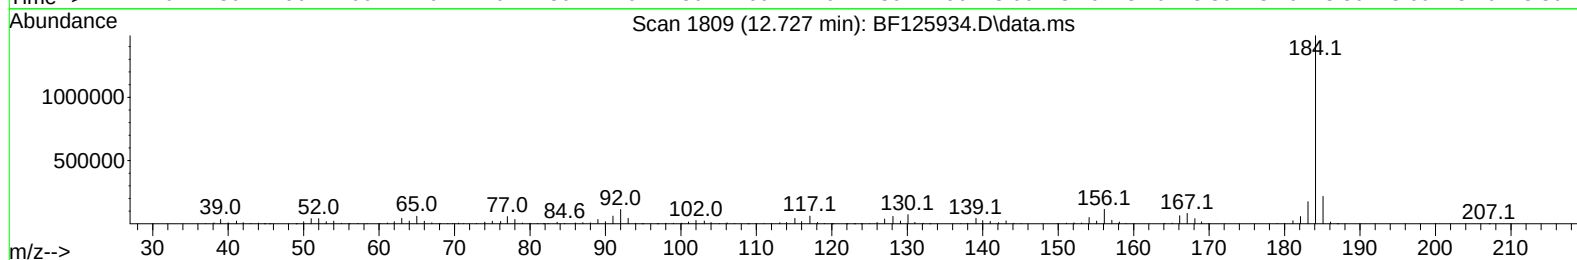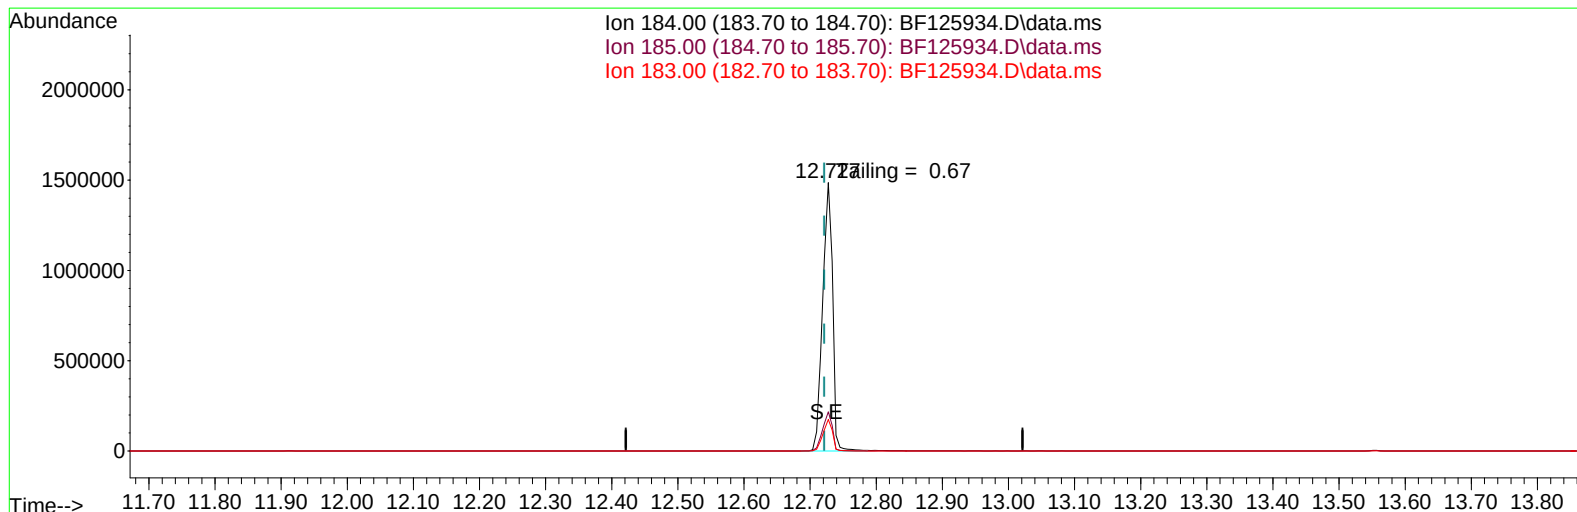

TIC: BF125934.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 1561530

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.61
183.00	10.10	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2021	BNA_F	<u>BF125934.D</u>
Compound Name	Response	Retention Time
DDT	806071	13.55
DDD	2933	13.25
DDE	0	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2933	809004	0.36