

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130782.D
 Acq On : 26 Oct 2022 13:12
 Operator : CG\JU
 Sample : PB148536BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148536BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.757	484	488	501	rBV	76718	140480	5.92%	1.058%
2	5.181	557	560	593	rBV	1319428	1586969	66.89%	11.953%
3	6.222	734	737	768	rBV	1460816	1601095	67.49%	12.059%
4	6.563	792	795	809	rVB	400682	368520	15.53%	2.776%
5	7.134	889	892	914	rBV	949404	1035897	43.66%	7.802%
6	7.845	1010	1013	1026	rBV	510556	498649	21.02%	3.756%
7	8.922	1191	1196	1199	rBV	2341286	2117880	89.27%	15.952%
8	9.592	1306	1310	1323	rBV	679411	585731	24.69%	4.412%
9	10.386	1441	1445	1470	rBV	1261171	1275107	53.75%	9.604%
10	11.075	1559	1562	1583	rBV	698512	609565	25.69%	4.591%
11	12.657	1827	1831	1835	rBV	2661662	2372451	100.00%	17.869%
12	13.710	2007	2010	2022	rBV	451118	460119	19.39%	3.466%
13	13.804	2022	2026	2034	rBV	58399	68337	2.88%	0.515%
14	14.757	2183	2188	2195	rBV2	22780	29212	1.23%	0.220%
15	15.098	2239	2246	2263	rBV	254136	396315	16.70%	2.985%
16	15.457	2302	2307	2313	rBV2	24585	34918	1.47%	0.263%
17	15.886	2374	2380	2386	rBV	22868	35927	1.51%	0.271%
18	16.380	2458	2464	2469	rBV2	15972	30199	1.27%	0.227%
19	16.974	2558	2565	2573	rVB4	13903	29454	1.24%	0.222%




Sum of corrected areas: 13276825

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130782.D
Acq On : 26 Oct 2022 13:12
Operator : CG\JU
Sample : PB148536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148536BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

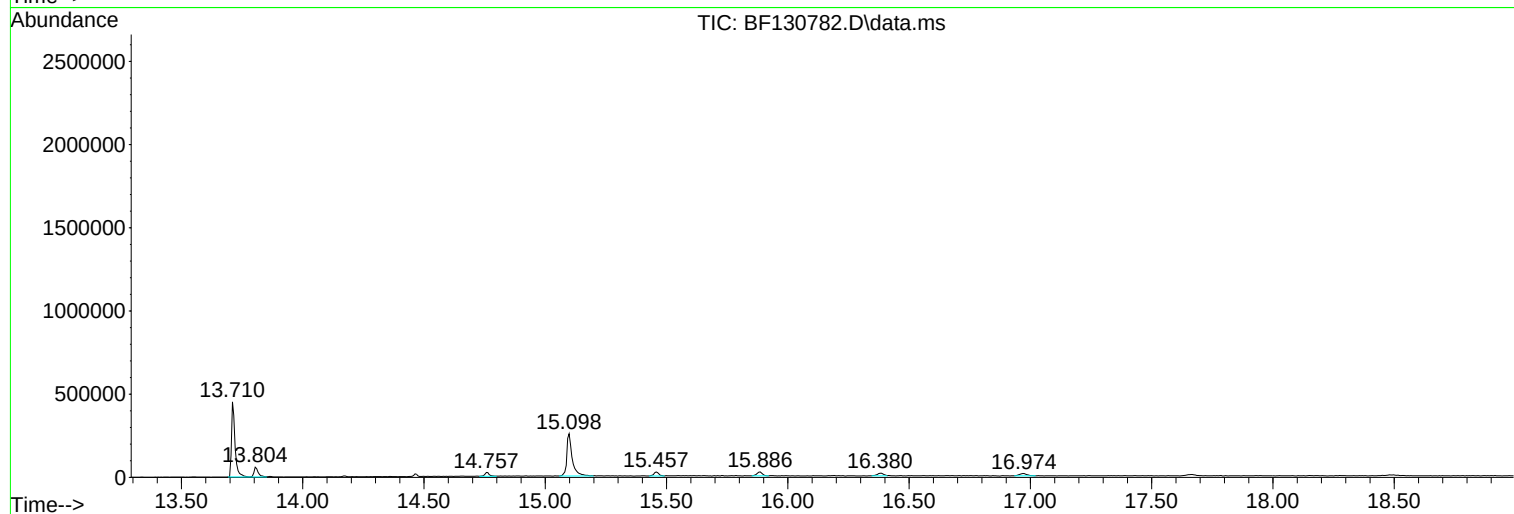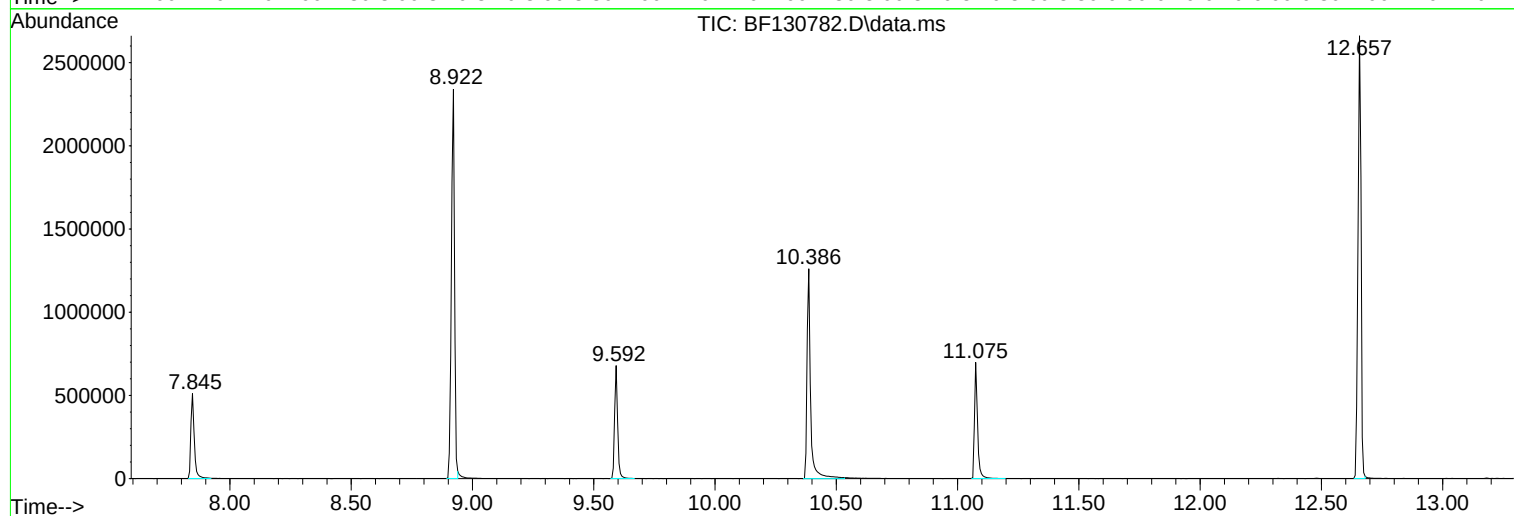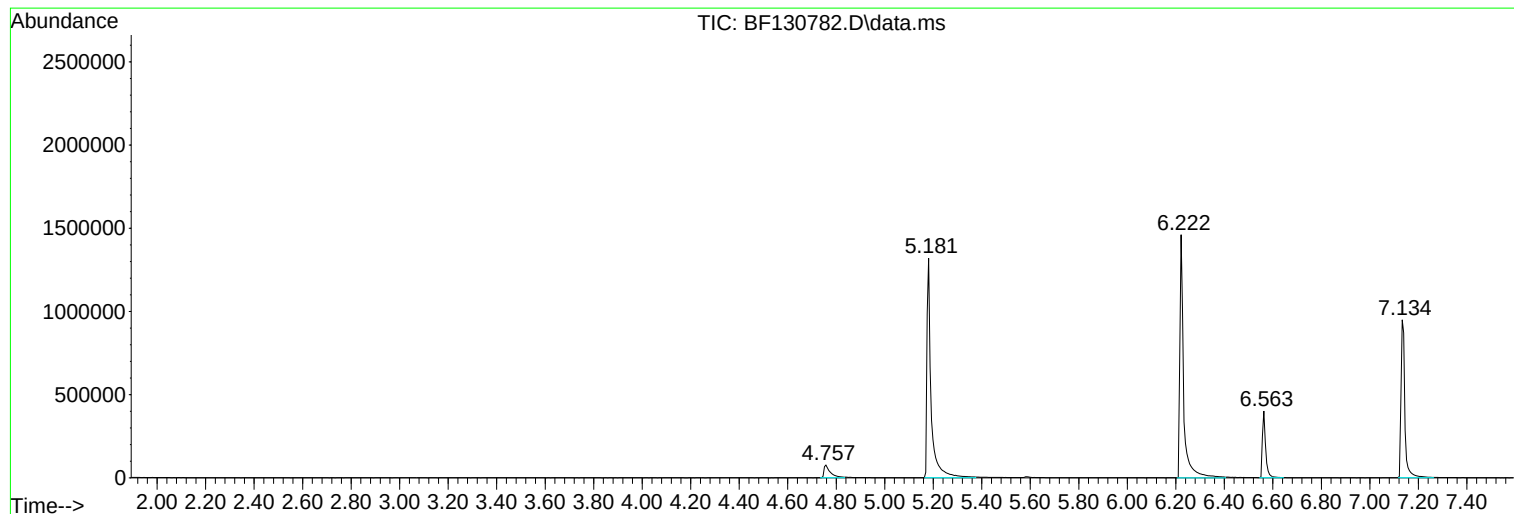

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130782.D
Acq On : 26 Oct 2022 13:12
Operator : CG\JU
Sample : PB148536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148536BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.757	7.62 ng	140480	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
5			Acetone	58	C3H6O	000067-64-1	9

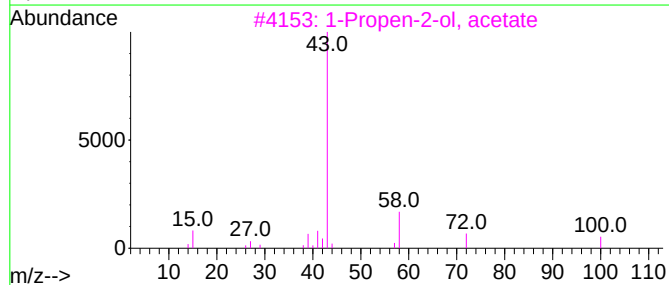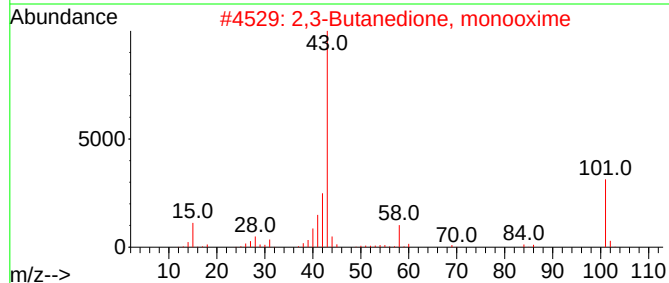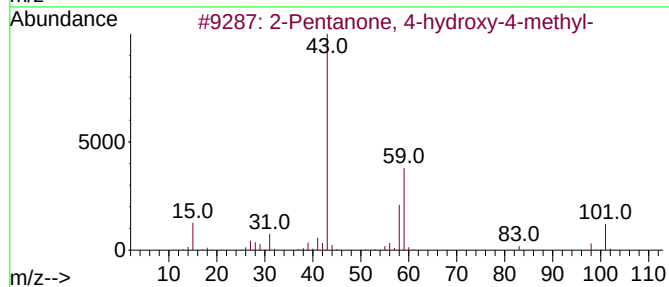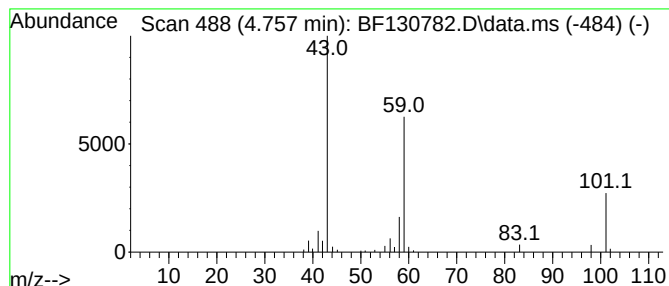

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130782.D
Acq On : 26 Oct 2022 13:12
Operator : CG\JU
Sample : PB148536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148536BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.804	2.97 ng	68337	Chrysene-d12	13.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	78
3			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	43
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	40
5			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	39

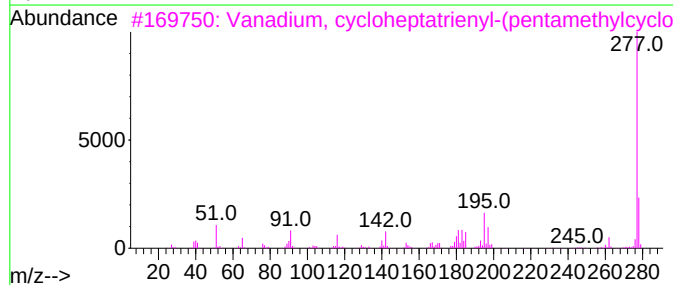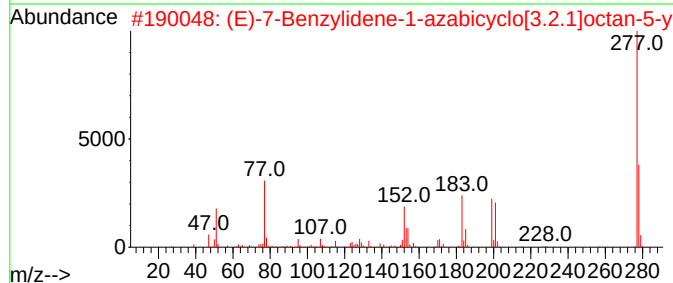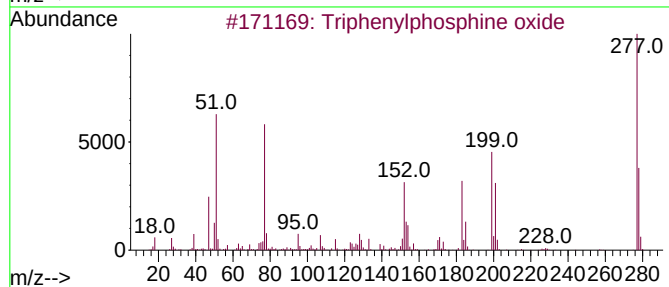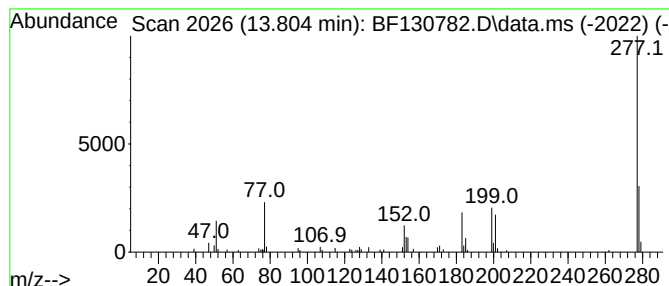

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130782.D
Acq On : 26 Oct 2022 13:12
Operator : CG\JU
Sample : PB148536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148536BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.757	7.6	ng	140480	1	6.563	368520	20.0
Triphenylphosph...	13.804	3.0	ng	68337	5	13.710	460119	20.0