

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130785.D
 Acq On : 26 Oct 2022 16:04
 Operator : CG\JU
 Sample : N5281-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.745	483	486	512	rBV	68964	124376	7.78%	1.259%
2	5.175	557	559	605	rBV	782498	1077551	67.44%	10.911%
3	6.222	735	737	763	rBV	1043719	1104321	69.11%	11.182%
4	6.563	792	795	808	rBV	398204	346899	21.71%	3.513%
5	7.133	890	892	916	rBV	665638	718558	44.97%	7.276%
6	7.845	1010	1013	1023	rBV	515684	473950	29.66%	4.799%
7	8.922	1192	1196	1208	rBV	1745944	1500344	93.89%	15.192%
8	9.592	1307	1310	1322	rBV	701803	581685	36.40%	5.890%
9	10.386	1441	1445	1461	rBV	858338	921332	57.66%	9.329%
10	11.074	1559	1562	1573	rBV	679796	601412	37.64%	6.090%
11	12.657	1827	1831	1834	rBV	1952413	1597910	100.00%	16.180%
12	13.710	2007	2010	2023	rVB	455397	468388	29.31%	4.743%
13	13.804	2023	2026	2035	rVB	29263	37710	2.36%	0.382%
14	15.098	2242	2246	2260	rVB	227647	321217	20.10%	3.253%




Sum of corrected areas: 9875653

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130785.D
Acq On : 26 Oct 2022 16:04
Operator : CG\JU
Sample : N5281-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

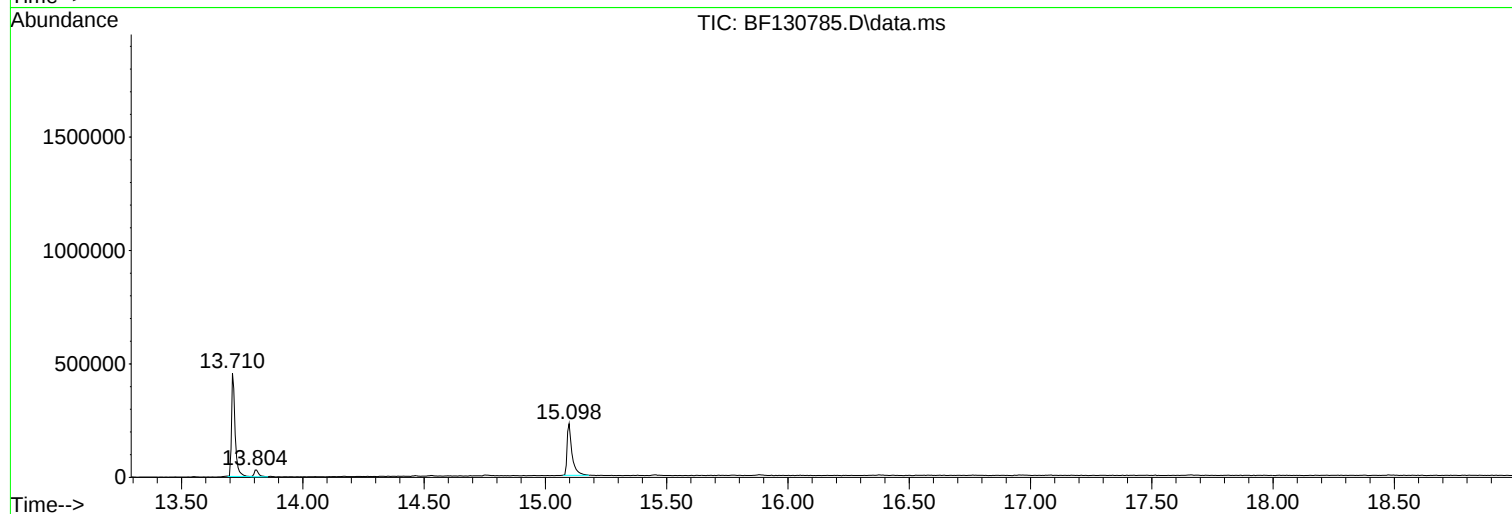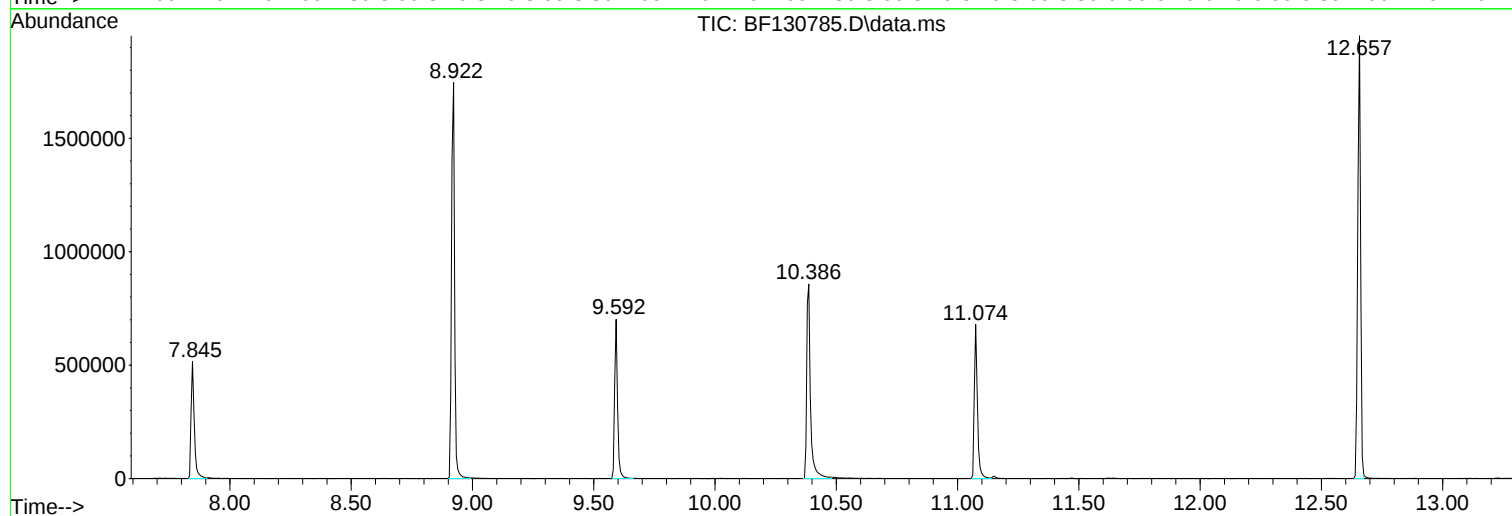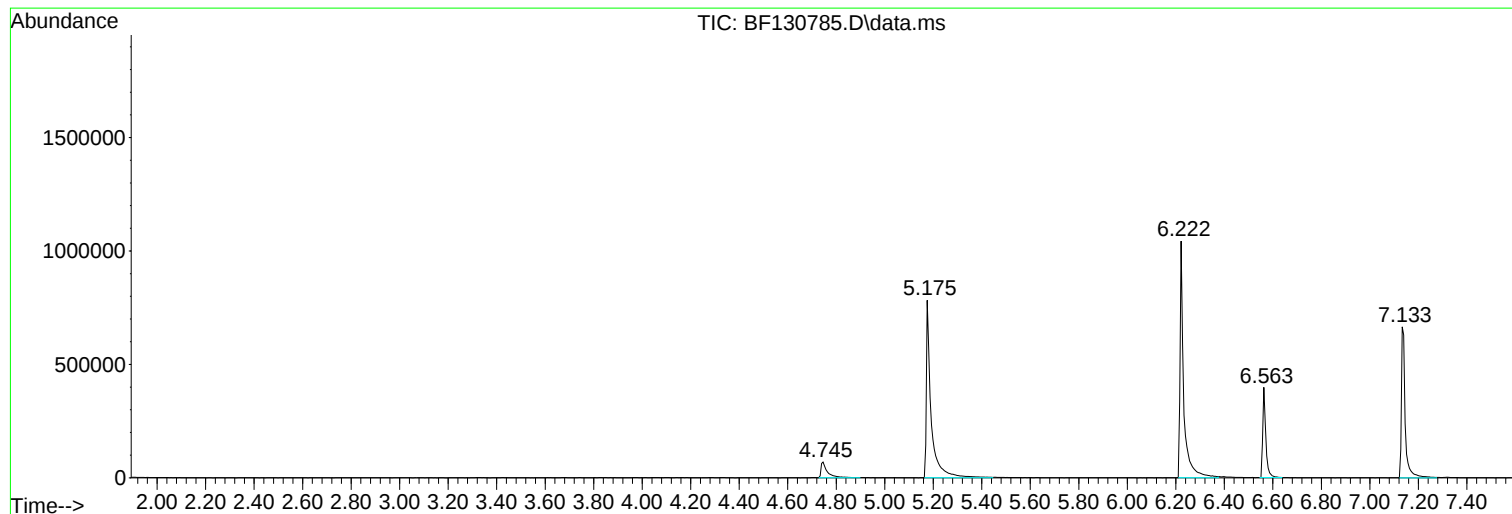

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130785.D
Acq On : 26 Oct 2022 16:04
Operator : CG\JU
Sample : N5281-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.745	7.17 ng	124376	1,4-Dichlorobenzene-d4	6.563

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

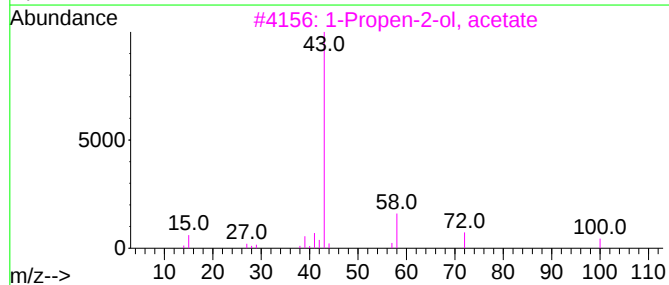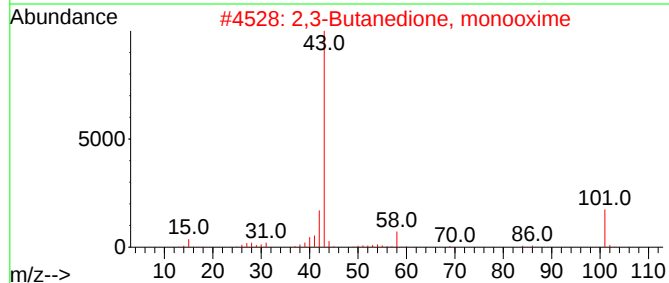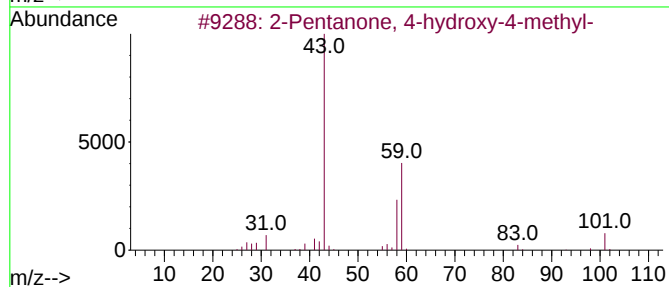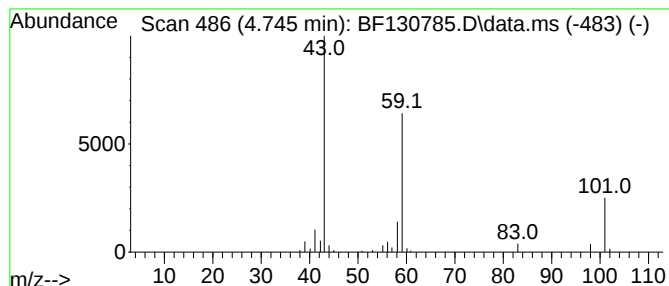

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130785.D
Acq On : 26 Oct 2022 16:04
Operator : CG\JU
Sample : N5281-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.745	7.2	ng	124376	1	6.563	346899	20.0