

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130787.D
 Acq On : 26 Oct 2022 17:14
 Operator : CG\JU
 Sample : N5281-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.740	482	485	513	rBV	131035	210041	12.82%	2.044%
2	5.175	556	559	581	rBV	841110	1079952	65.93%	10.507%
3	6.222	734	737	765	rBV	1119584	1194101	72.90%	11.618%
4	6.563	792	795	810	rBV	381146	345517	21.09%	3.362%
5	7.134	889	892	921	rBV	737377	786977	48.05%	7.657%
6	7.846	1010	1013	1028	rBV	517711	477069	29.13%	4.641%
7	8.922	1192	1196	1209	rBV	2024432	1637937	100.00%	15.936%
8	9.592	1307	1310	1329	rVB	681401	569579	34.77%	5.541%
9	10.387	1441	1445	1468	rBV	836495	940493	57.42%	9.150%
10	11.075	1559	1562	1573	rBV	661772	578525	35.32%	5.629%
11	12.657	1827	1831	1834	rBV	1895735	1610044	98.30%	15.664%
12	13.686	1990	2006	2007	rBV4	16368	44929	2.74%	0.437%
13	13.710	2007	2010	2023	rVV	426728	456294	27.86%	4.439%
14	13.804	2023	2026	2034	rVB	29896	38256	2.34%	0.372%
15	15.098	2242	2246	2261	rVB	210617	308731	18.85%	3.004%




Sum of corrected areas: 10278445

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130787.D
Acq On : 26 Oct 2022 17:14
Operator : CG\JU
Sample : N5281-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

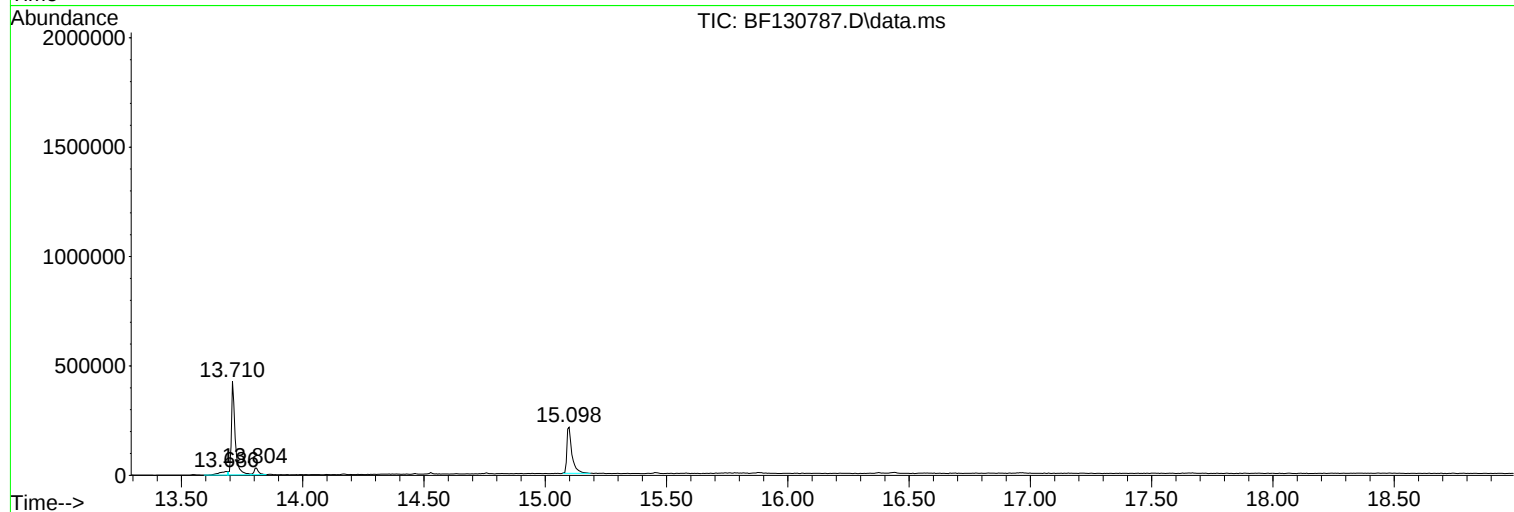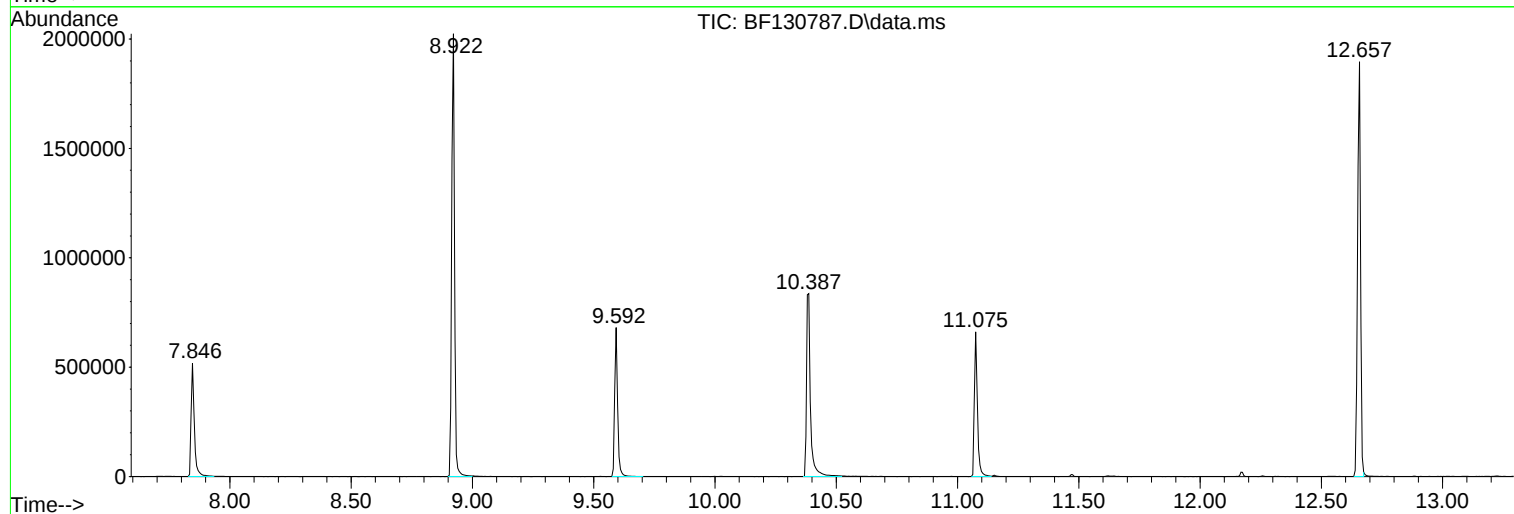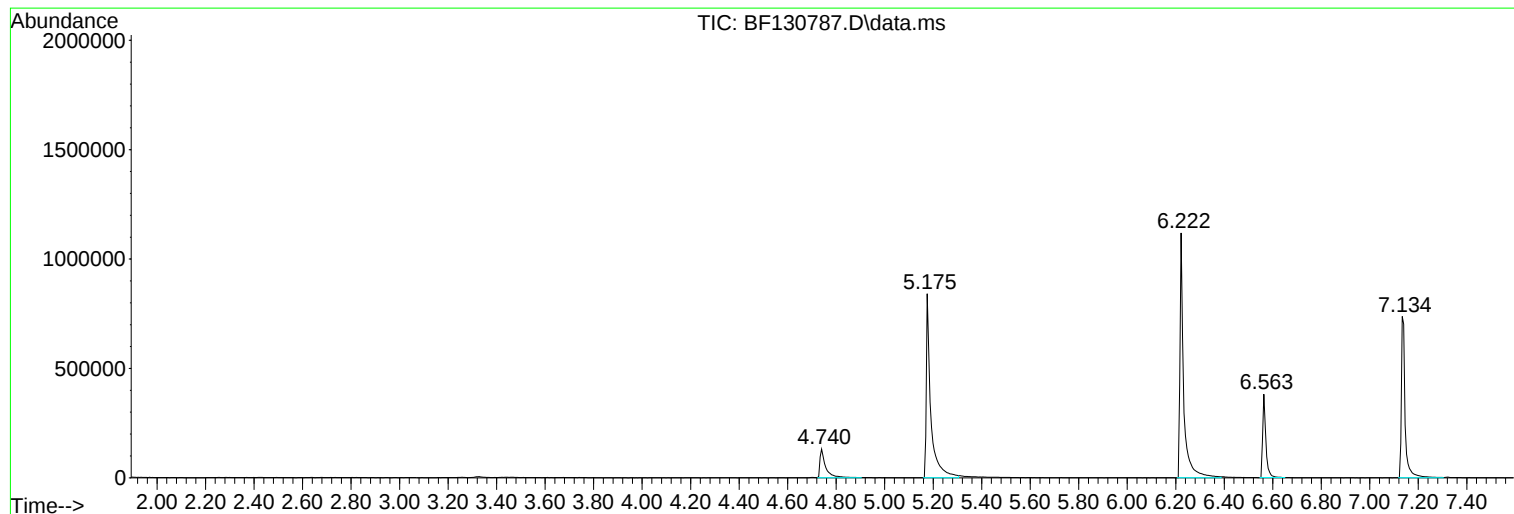

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130787.D
Acq On : 26 Oct 2022 17:14
Operator : CG\JU
Sample : N5281-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.740	12.16 ng	210041	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	53		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

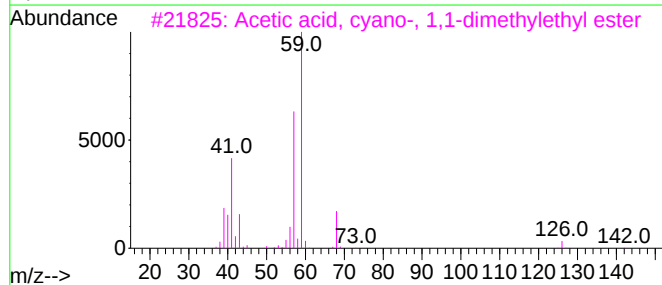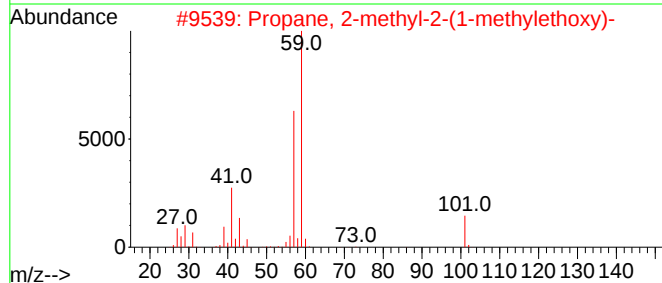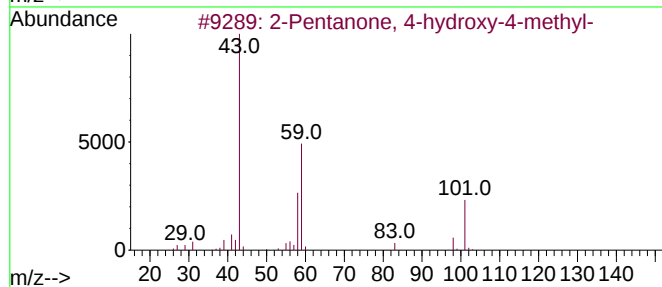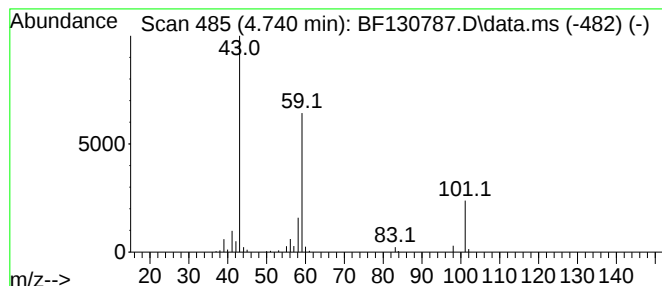

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130787.D
Acq On : 26 Oct 2022 17:14
Operator : CG\JU
Sample : N5281-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.740	12.2	ng	210041	1	6.563	345517	20.0