

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130788.D
 Acq On : 26 Oct 2022 17:48
 Operator : CG\JU
 Sample : N5281-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-5S

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.745	483	486	508	rBV	263517	442530	13.69%	1.973%
2	5.181	557	560	588	rBV	1917201	2724361	84.30%	12.144%
3	6.222	734	737	765	rBV	2429894	2713921	83.98%	12.098%
4	6.563	792	795	809	rBV	888714	802149	24.82%	3.576%
5	7.139	889	893	913	rBV	1643616	1757584	54.39%	7.835%
6	7.845	1010	1013	1038	rBV	1175420	1119925	34.66%	4.992%
7	8.922	1192	1196	1208	rBV	3613134	3231589	100.00%	14.405%
8	9.592	1307	1310	1325	rBV	1409063	1272642	39.38%	5.673%
9	10.386	1441	1445	1462	rBV	1949064	1984610	61.41%	8.847%
10	11.074	1559	1562	1572	rBV	1456724	1277481	39.53%	5.695%
11	12.657	1827	1831	1842	rBV	3617896	3140921	97.19%	14.001%
12	13.686	1990	2006	2008	rBV3	46606	145405	4.50%	0.648%
13	13.710	2008	2010	2023	rVV	917757	1007887	31.19%	4.493%
14	13.810	2023	2027	2034	rVB	55718	75874	2.35%	0.338%
15	14.527	2145	2149	2156	rBV	46854	47995	1.49%	0.214%
16	15.098	2242	2246	2264	rVB2	447935	688261	21.30%	3.068%




Sum of corrected areas: 22433135

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130788.D
Acq On : 26 Oct 2022 17:48
Operator : CG\JU
Sample : N5281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-5S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

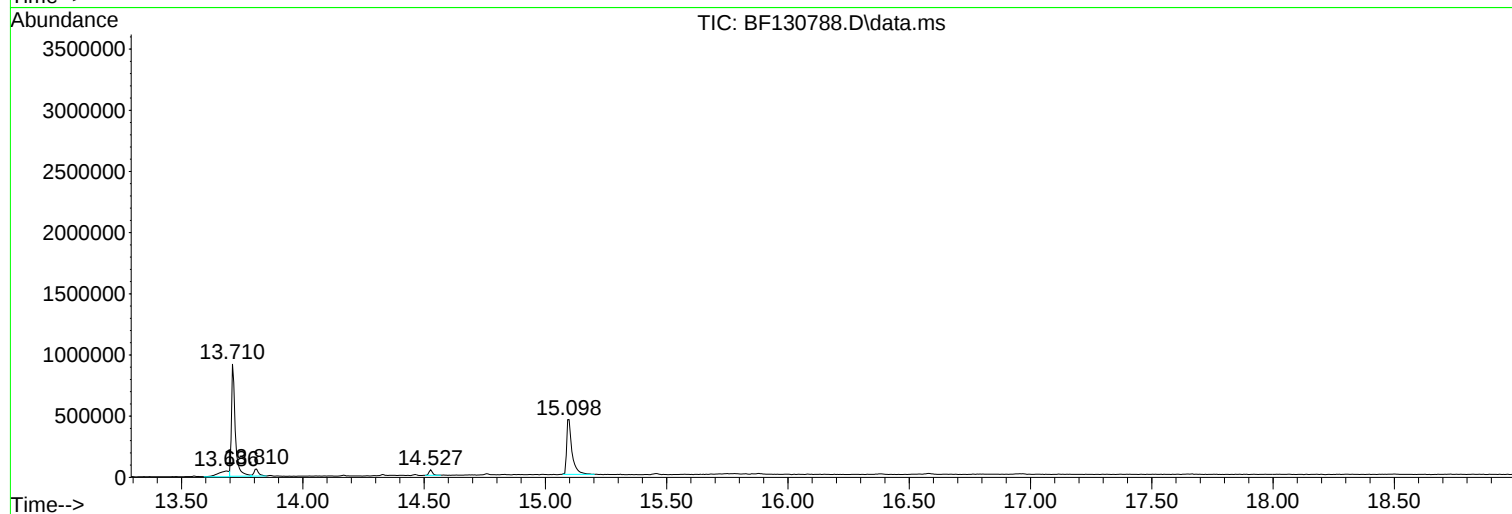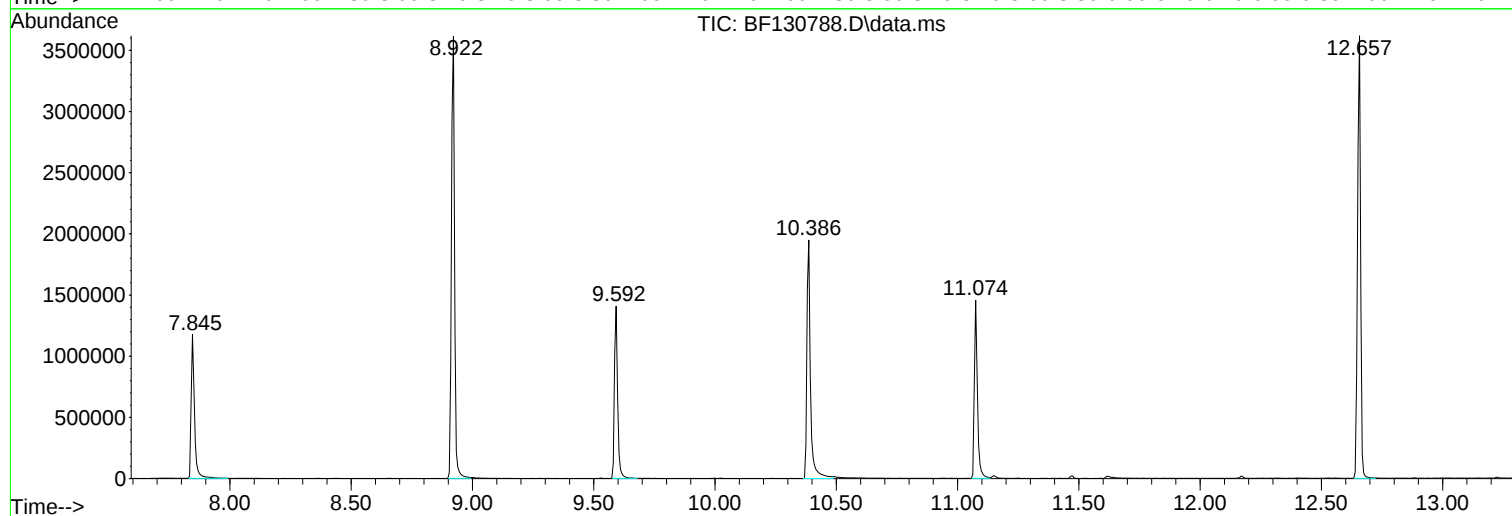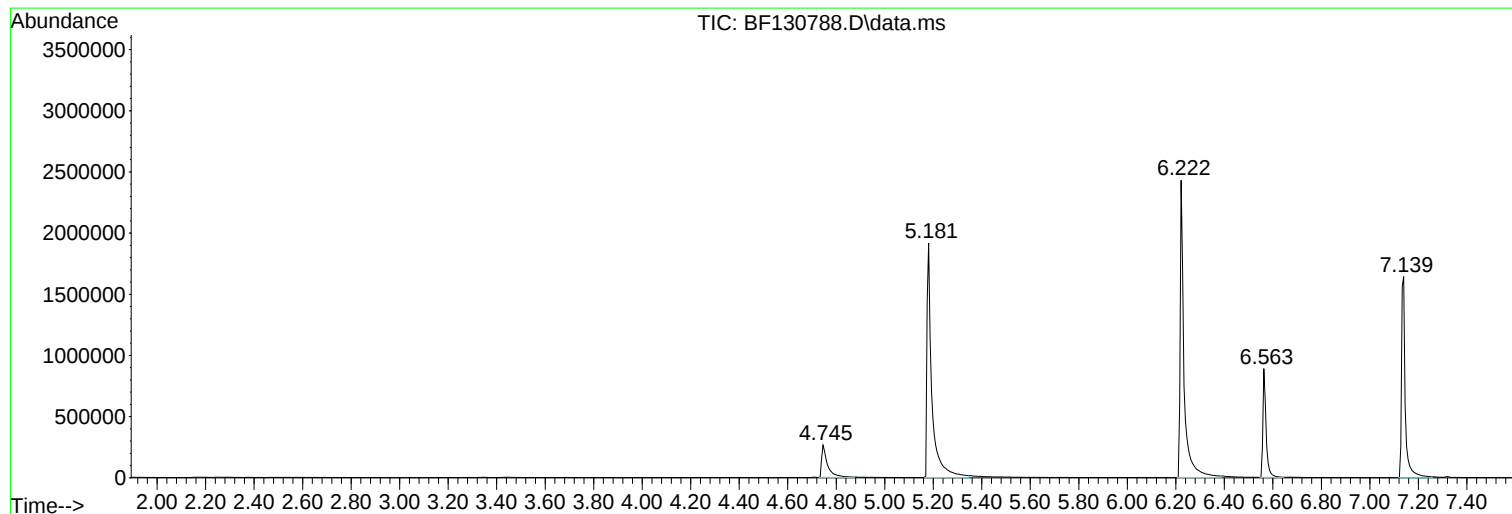

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130788.D
Acq On : 26 Oct 2022 17:48
Operator : CG\JU
Sample : N5281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-5S










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.745	11.03 ng	442530	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	25		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
4	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	23		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		

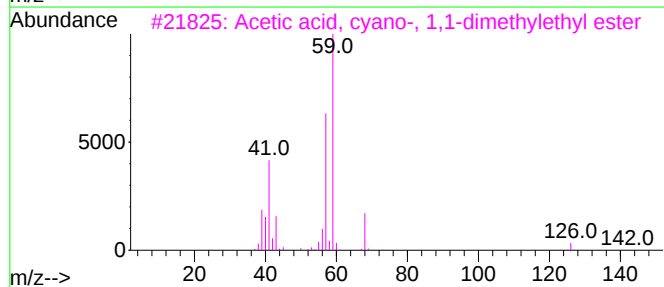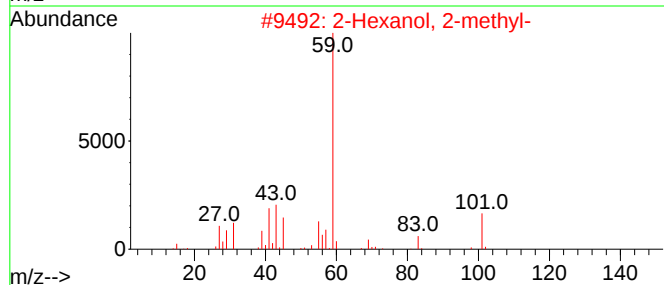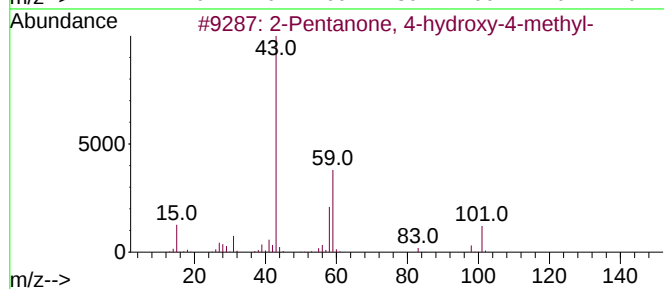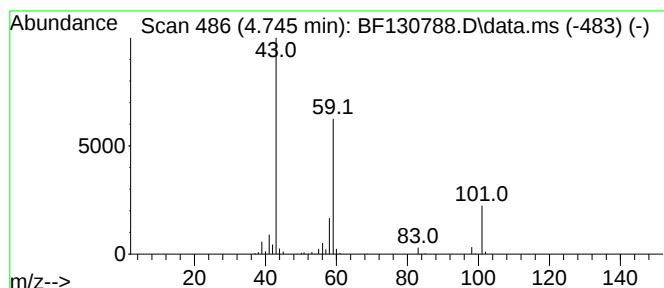

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130788.D
Acq On : 26 Oct 2022 17:48
Operator : CG\JU
Sample : N5281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-5S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.745	11.0	ng	442530	1	6.563	802149	20.0