

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130790.D
 Acq On : 26 Oct 2022 18:57
 Operator : CG\JU
 Sample : N5281-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.745	483	486	507	rBV	231844	416292	14.01%	2.672%
2	5.175	556	559	589	rBV	2203818	2971696	100.00%	19.073%
3	6.222	734	737	757	rBV	2605835	2717535	91.45%	17.441%
4	6.563	792	795	808	rBV	403328	359465	12.10%	2.307%
5	7.139	890	893	914	rBV	936749	995683	33.51%	6.390%
6	7.845	1010	1013	1025	rBV	530755	496729	16.72%	3.188%
7	8.922	1192	1196	1199	rBV	2561061	2084983	70.16%	13.382%
8	9.592	1307	1310	1332	rVB	703518	597170	20.10%	3.833%
9	10.386	1441	1445	1461	rBV	1313669	1289805	43.40%	8.278%
10	11.074	1559	1562	1572	rBV	704687	609781	20.52%	3.914%
11	12.657	1827	1831	1834	rBV	2537780	2135478	71.86%	13.706%
12	13.686	1989	2006	2008	rBV5	23515	80700	2.72%	0.518%
13	13.710	2008	2010	2023	rVV	426882	467759	15.74%	3.002%
14	13.804	2023	2026	2034	rVB	37612	46000	1.55%	0.295%
15	15.098	2242	2246	2258	rVB	225041	311960	10.50%	2.002%




Sum of corrected areas: 15581036

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130790.D
Acq On : 26 Oct 2022 18:57
Operator : CG\JU
Sample : N5281-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

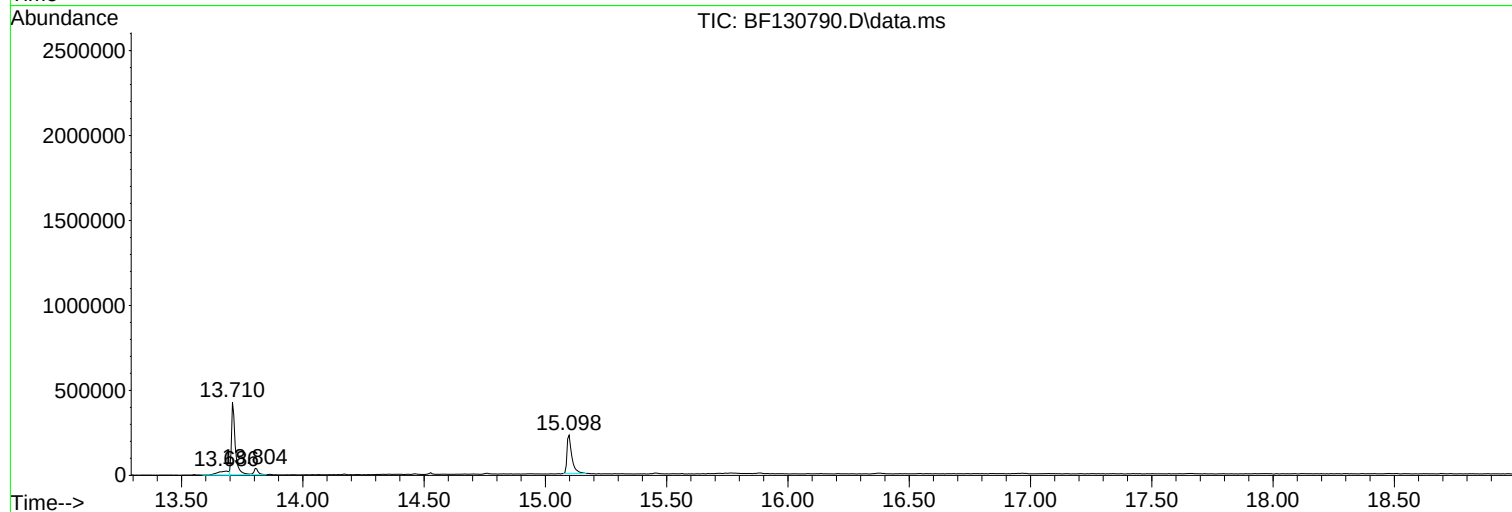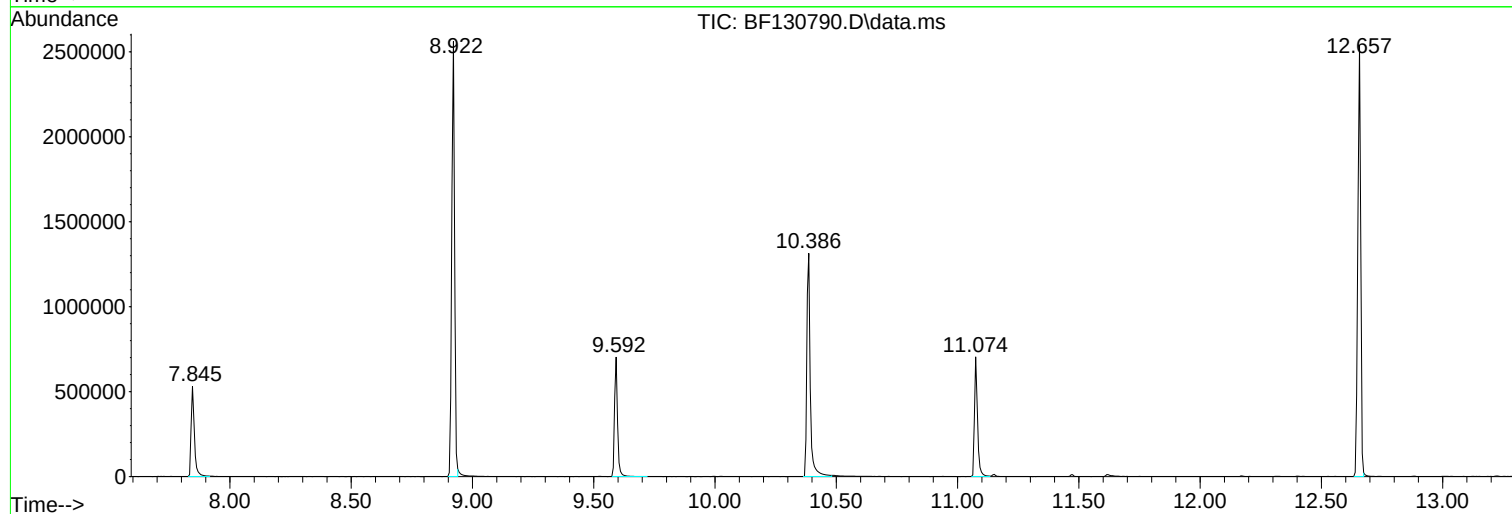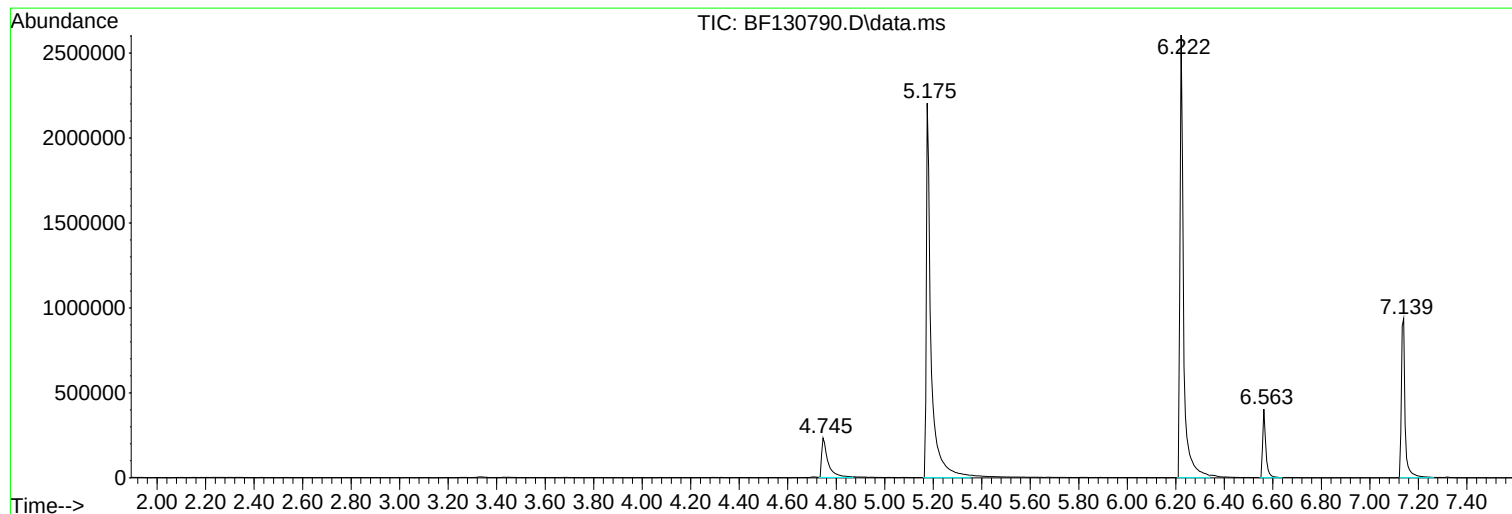

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130790.D
Acq On : 26 Oct 2022 18:57
Operator : CG\JU
Sample : N5281-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.745	23.16 ng	416292	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

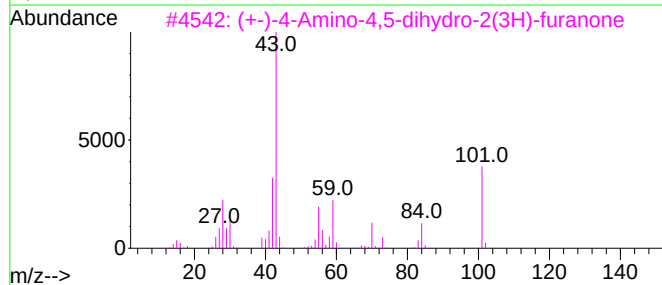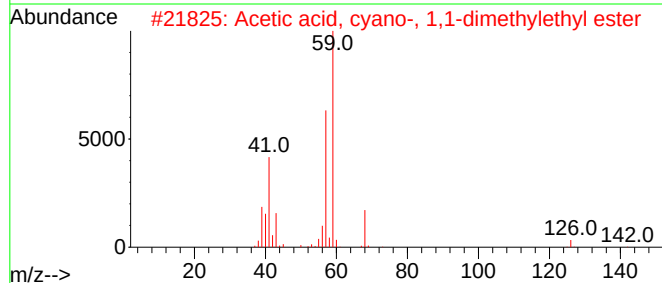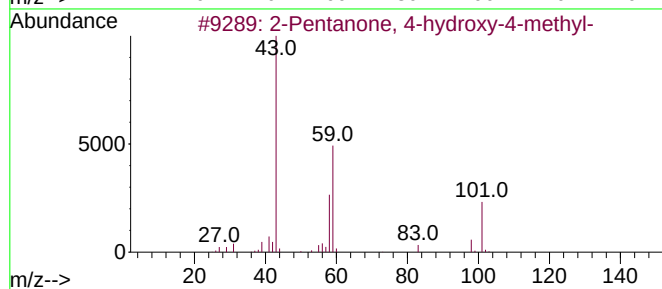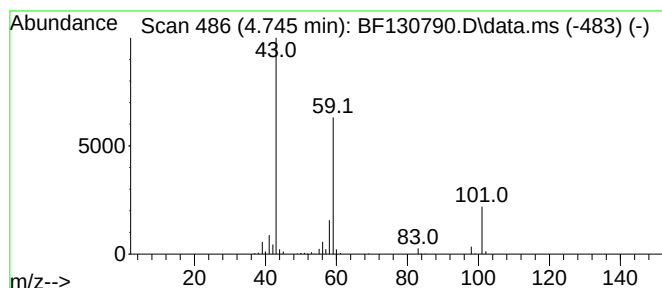

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130790.D
Acq On : 26 Oct 2022 18:57
Operator : CG\JU
Sample : N5281-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.745	23.2	ng	416292	1	6.563	359465	20.0