

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130791.D
 Acq On : 26 Oct 2022 19:31
 Operator : CG\JU
 Sample : N5281-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.745	483	486	510	rBV	221535	393243	13.53%	2.358%
2	5.175	556	559	601	rBV	2179196	2906560	100.00%	17.428%
3	6.222	734	737	765	rBV	2607138	2884895	99.25%	17.298%
4	6.563	792	795	809	rVB	801649	727967	25.05%	4.365%
5	7.134	889	892	915	rBV	1653790	1842593	63.39%	11.048%
6	7.845	1010	1013	1035	rBV	1088210	1017005	34.99%	6.098%
7	8.922	1192	1196	1209	rBV	2185294	1881860	64.75%	11.284%
8	9.592	1307	1310	1324	rBV	723543	606362	20.86%	3.636%
9	10.386	1441	1445	1465	rBV	1144298	1225330	42.16%	7.347%
10	11.075	1559	1562	1572	rBV	708252	617881	21.26%	3.705%
11	12.657	1827	1831	1834	rBV	2186421	1815367	62.46%	10.885%
12	13.710	2007	2010	2024	rVV	413248	431279	14.84%	2.586%
13	15.098	2242	2246	2263	rVB	219515	327014	11.25%	1.961%




Sum of corrected areas: 16677356

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130791.D
Acq On : 26 Oct 2022 19:31
Operator : CG\JU
Sample : N5281-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

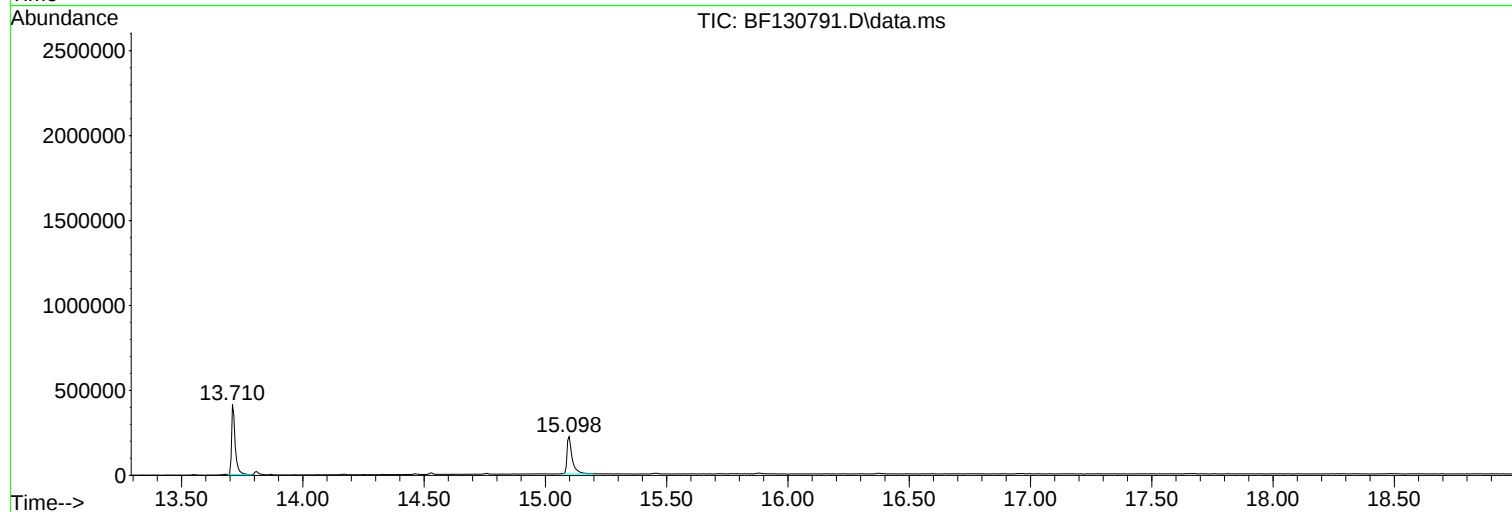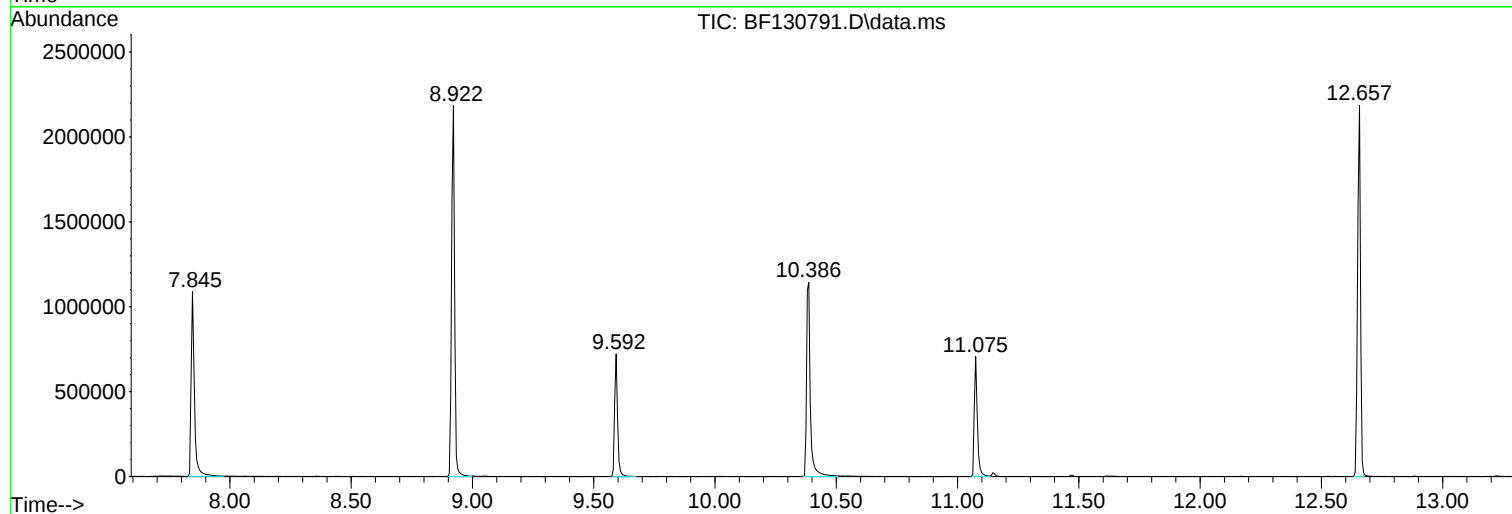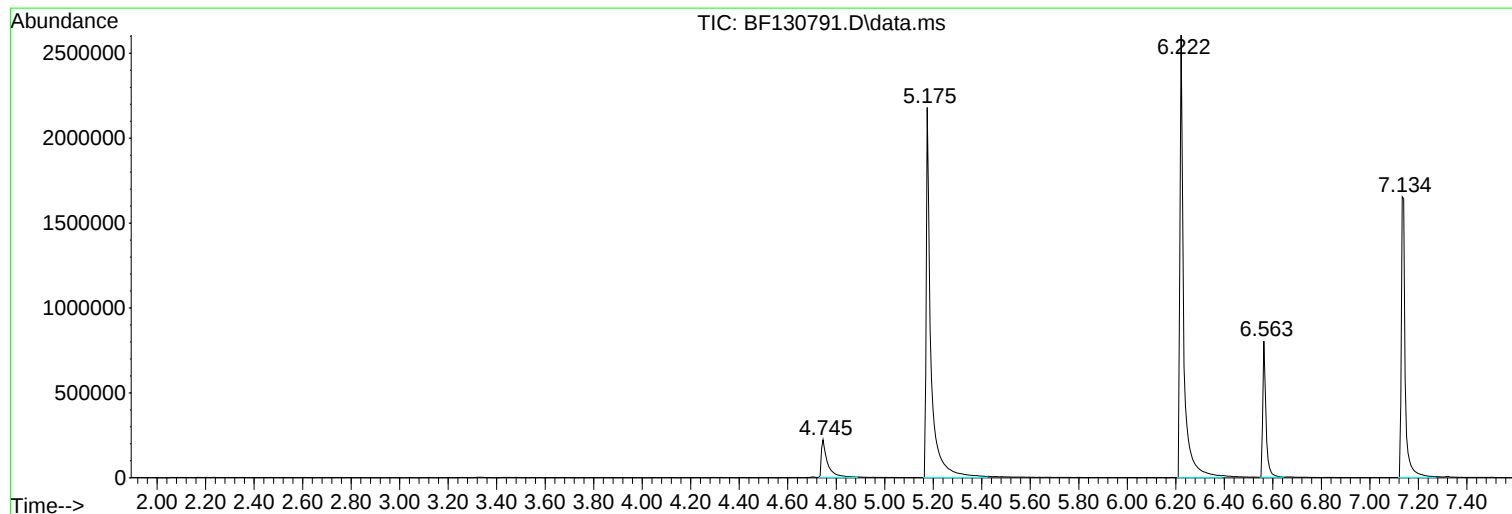

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130791.D
Acq On : 26 Oct 2022 19:31
Operator : CG\JU
Sample : N5281-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.745	10.80 ng	393243	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

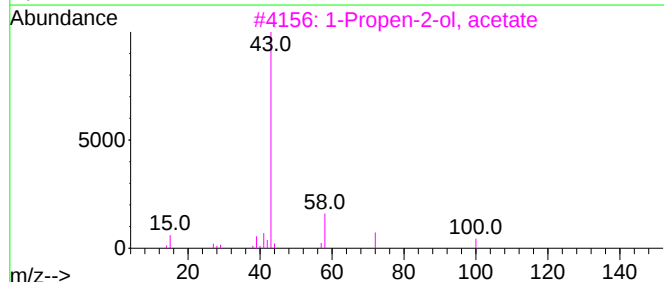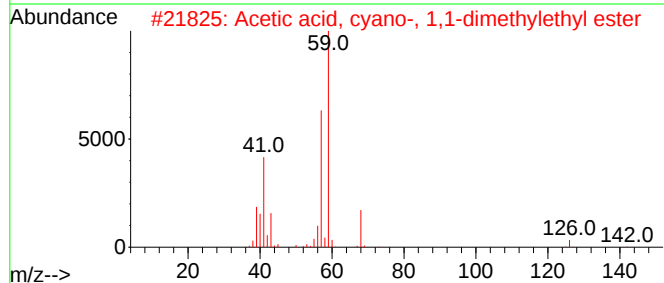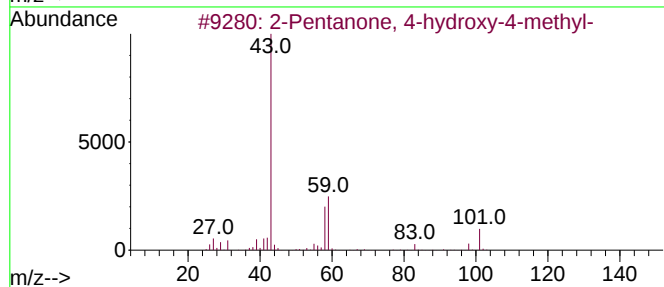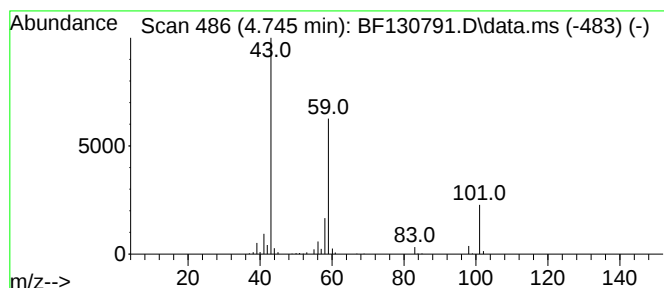

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130791.D
Acq On : 26 Oct 2022 19:31
Operator : CG\JU
Sample : N5281-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.745	10.8	ng	393243	1	6.563	727967	20.0