

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130792.D
 Acq On : 26 Oct 2022 20:05
 Operator : CG\JU
 Sample : N5281-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.746	483	486	509	rBV	284351	487477	20.08%	3.545%
2	5.175	556	559	585	rBV	1806971	2427150	100.00%	17.652%
3	6.222	734	737	762	rBV	1470147	1512161	62.30%	10.997%
4	6.563	792	795	809	rBV	402602	362784	14.95%	2.638%
5	7.140	889	893	911	rBV	938026	990523	40.81%	7.204%
6	7.845	1010	1013	1032	rBV	531997	505458	20.83%	3.676%
7	8.922	1192	1196	1208	rBV	2319045	2065399	85.10%	15.021%
8	9.592	1307	1310	1322	rBV	696242	603417	24.86%	4.388%
9	10.386	1441	1445	1461	rBV	1187379	1221764	50.34%	8.886%
10	11.075	1559	1562	1572	rBV	703891	617158	25.43%	4.488%
11	12.657	1827	1831	1834	rBV	2572001	2112349	87.03%	15.362%
12	13.669	1992	2003	2004	rBV6	18902	43816	1.81%	0.319%
13	13.710	2008	2010	2023	rVV	395150	466200	19.21%	3.391%
14	13.810	2023	2027	2034	rVB	20302	29543	1.22%	0.215%
15	15.098	2242	2246	2259	rVB	214473	304866	12.56%	2.217%




Sum of corrected areas: 13750065

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130792.D
Acq On : 26 Oct 2022 20:05
Operator : CG\JU
Sample : N5281-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

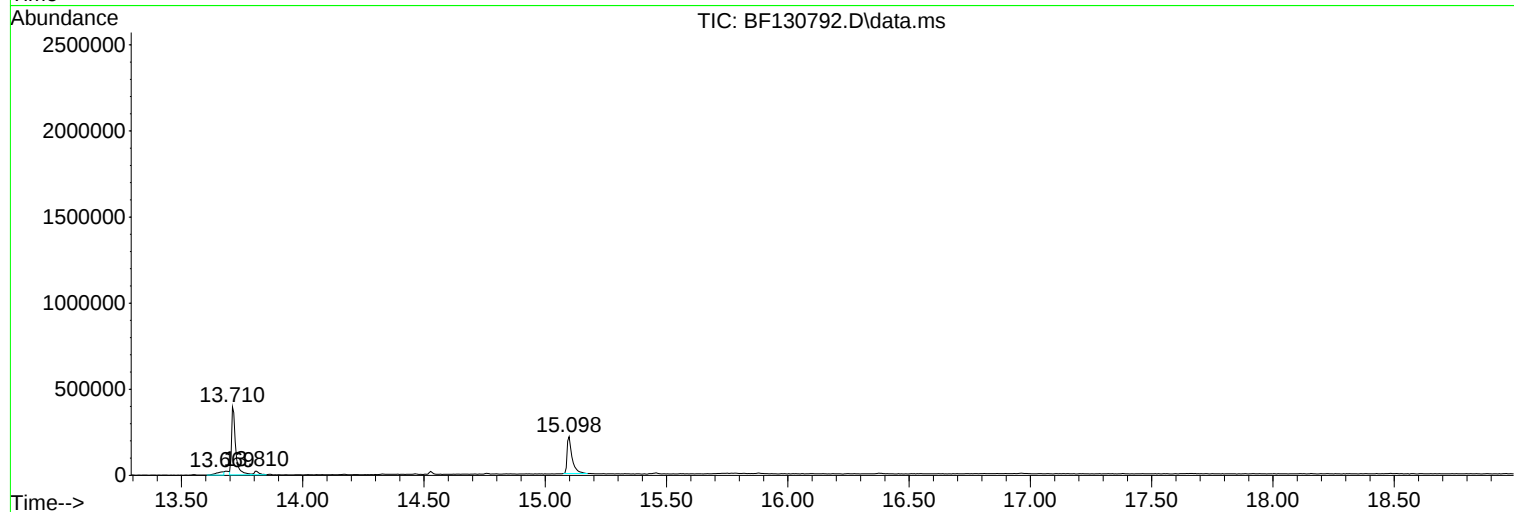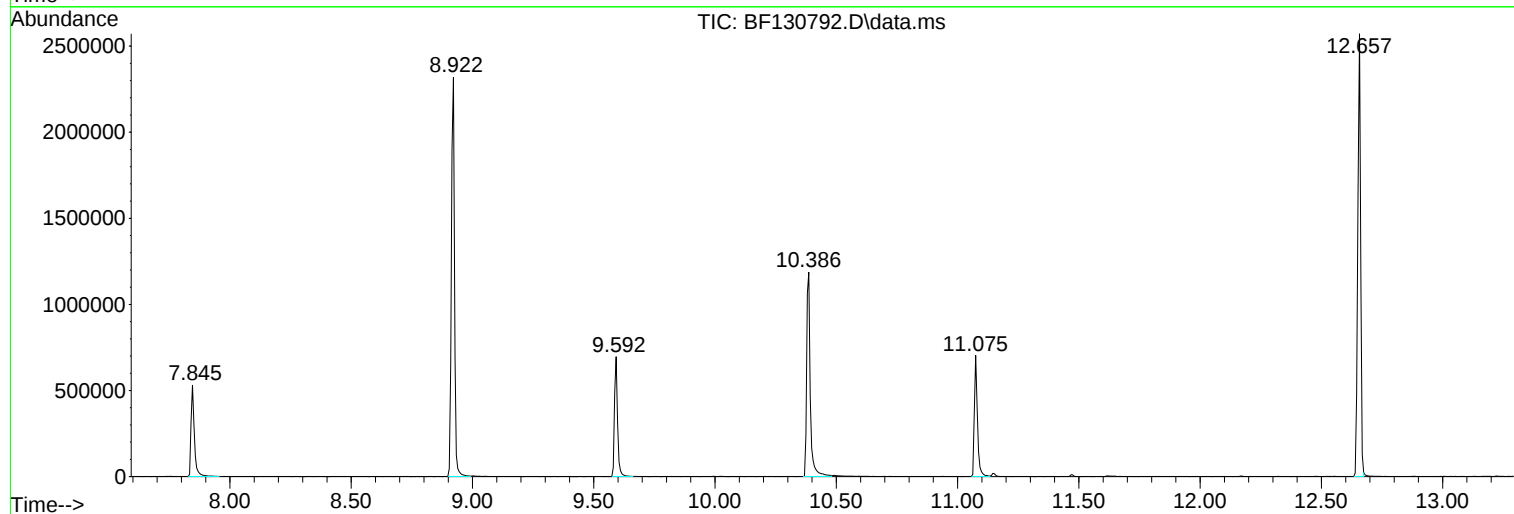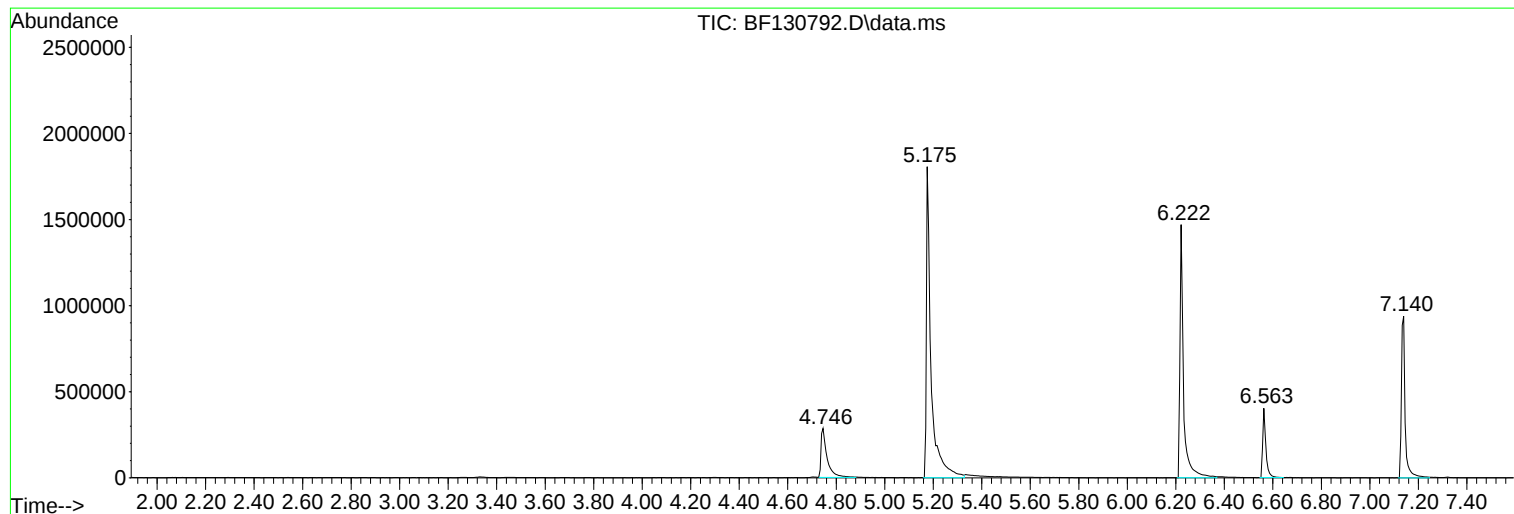

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130792.D
Acq On : 26 Oct 2022 20:05
Operator : CG\JU
Sample : N5281-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.746	26.87 ng	487477	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

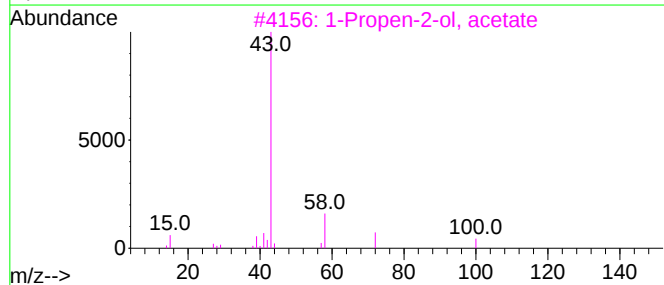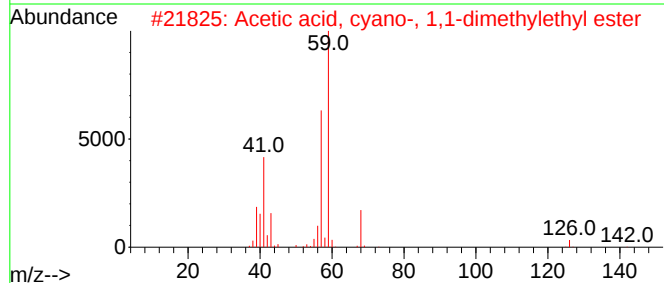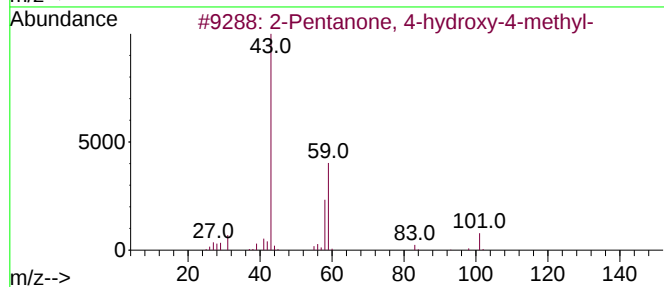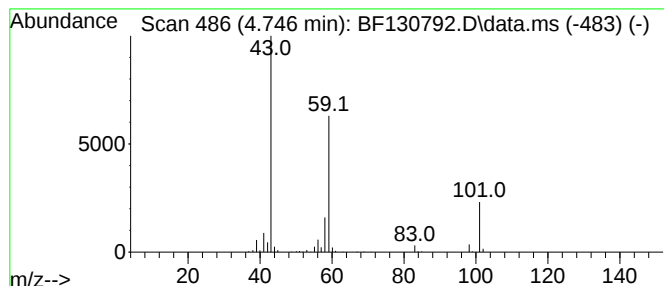

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130792.D
Acq On : 26 Oct 2022 20:05
Operator : CG\JU
Sample : N5281-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.746	26.9	ng	487477	1	6.563	362784	20.0