

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130795.D
 Acq On : 26 Oct 2022 21:46
 Operator : CG\JU
 Sample : N5281-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.740	482	485	510	rBV	303891	513058	17.88%	3.062%
2	5.175	557	559	596	rBV	2075611	2795739	97.46%	16.686%
3	6.222	734	737	765	rBV	2601653	2868742	100.00%	17.122%
4	6.563	792	795	808	rBV	828220	754280	26.29%	4.502%
5	7.139	890	893	920	rBV	1783119	1858259	64.78%	11.091%
6	7.845	1010	1013	1022	rBV	1113420	1011908	35.27%	6.040%
7	8.922	1192	1196	1206	rBV	2486908	2074530	72.31%	12.382%
8	9.592	1307	1310	1321	rVB	760230	656013	22.87%	3.915%
9	10.380	1442	1444	1460	rBV	973776	1061925	37.02%	6.338%
10	10.492	1460	1463	1472	rVB	38734	48016	1.67%	0.287%
11	11.074	1559	1562	1572	rBV	709647	635666	22.16%	3.794%
12	12.657	1827	1831	1840	rVB	1951879	1732633	60.40%	10.341%
13	13.715	2008	2011	2024	rVB	328568	384011	13.39%	2.292%
14	15.098	2243	2246	2256	rVB	266504	359925	12.55%	2.148%




Sum of corrected areas: 16754705

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130795.D
Acq On : 26 Oct 2022 21:46
Operator : CG\JU
Sample : N5281-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

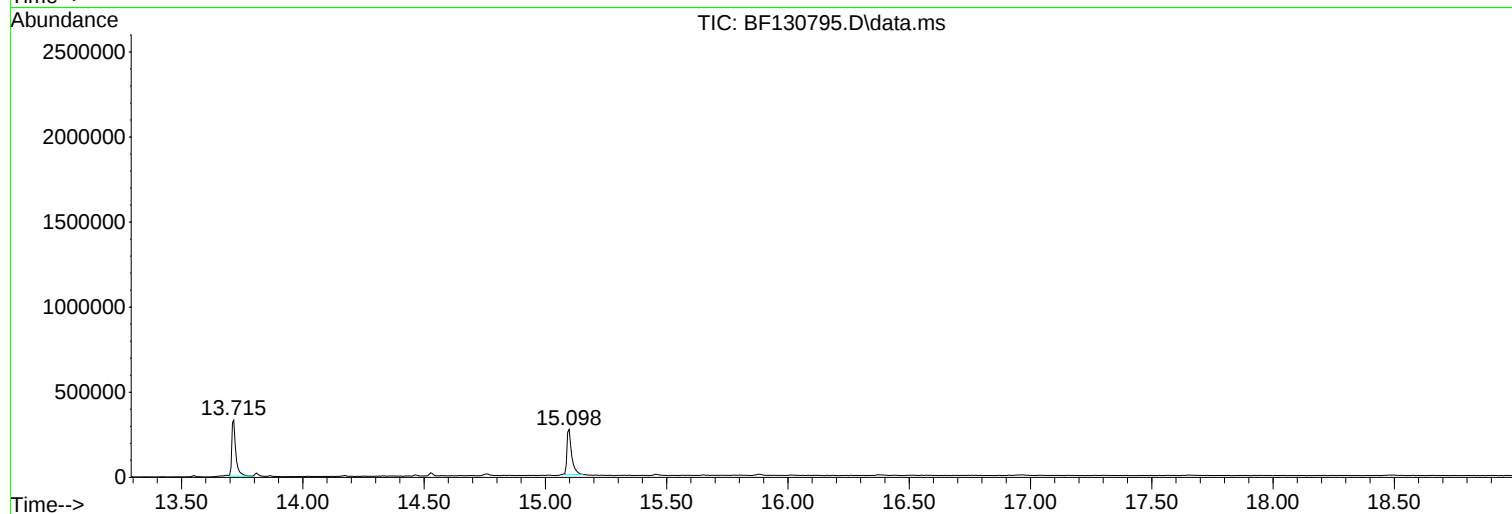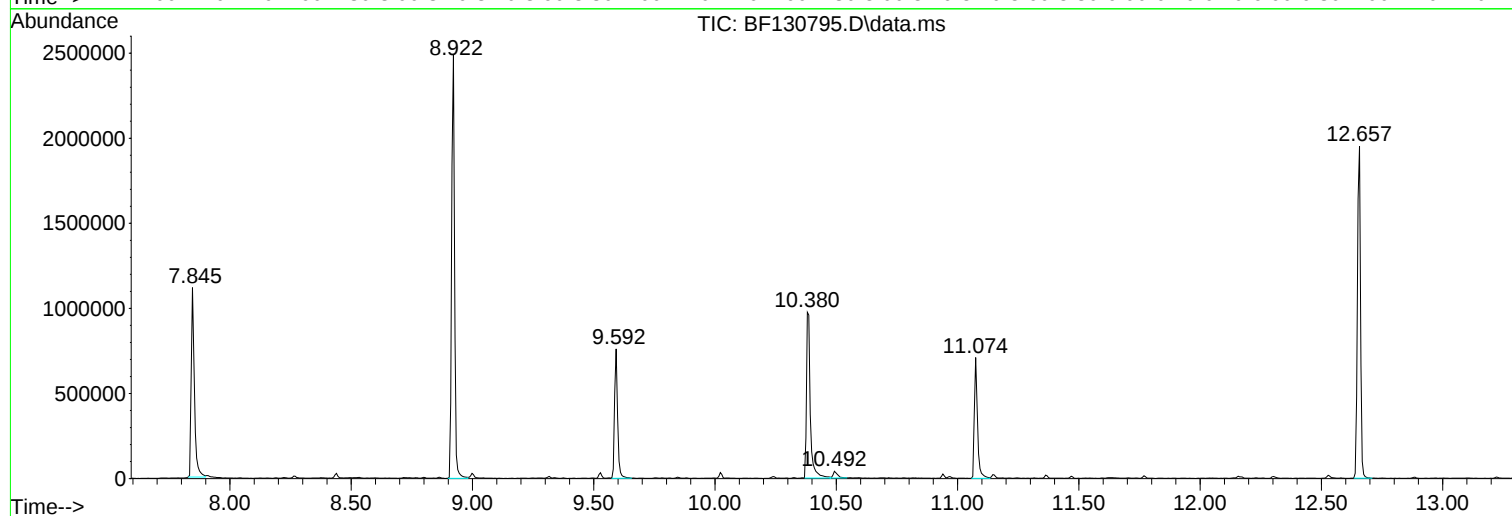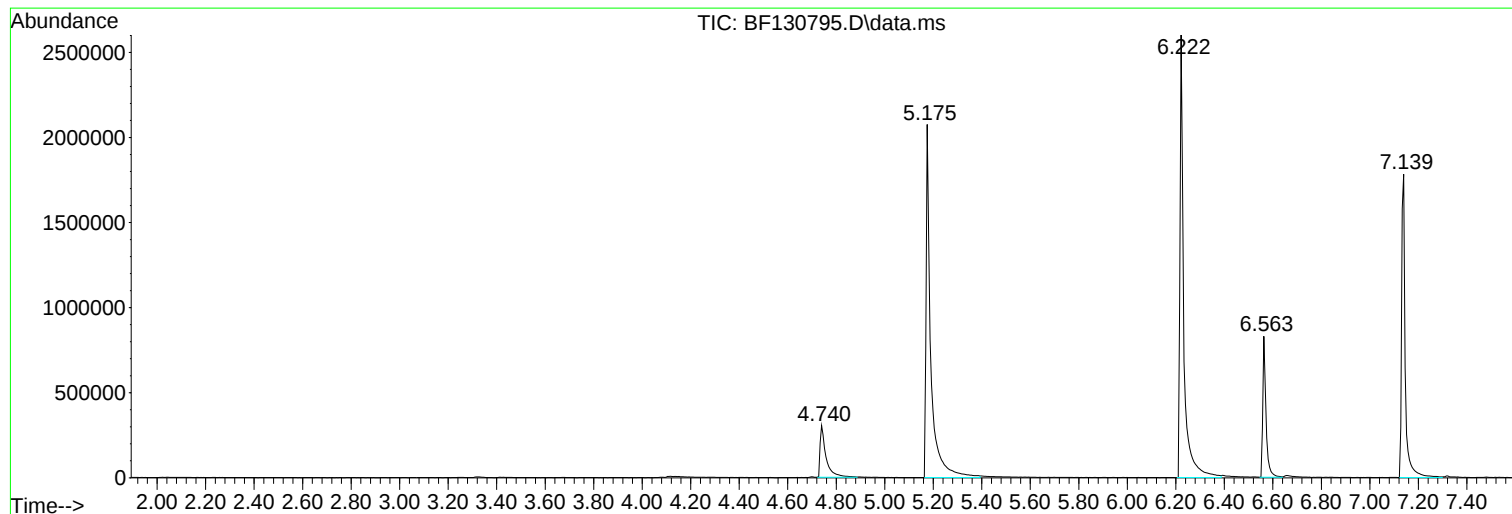

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130795.D
Acq On : 26 Oct 2022 21:46
Operator : CG\JU
Sample : N5281-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.740	13.60 ng	513058	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9
5			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

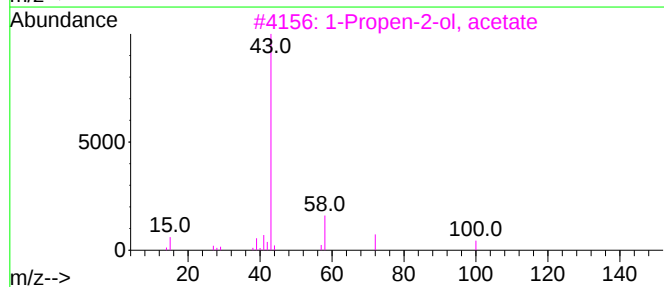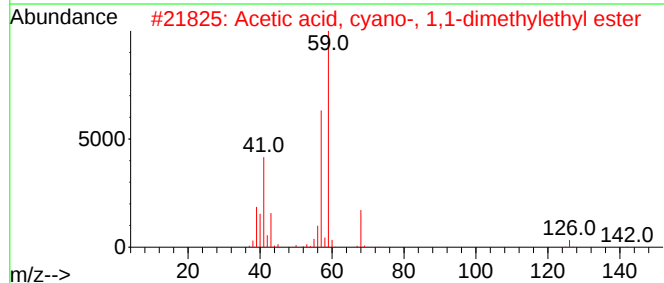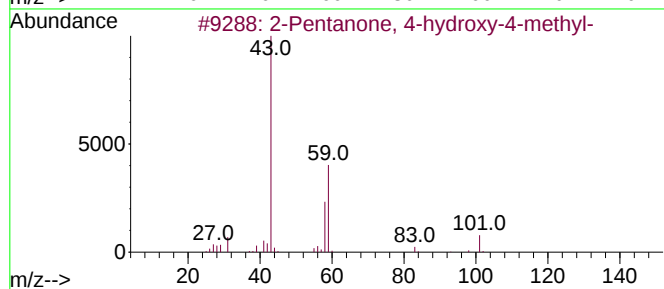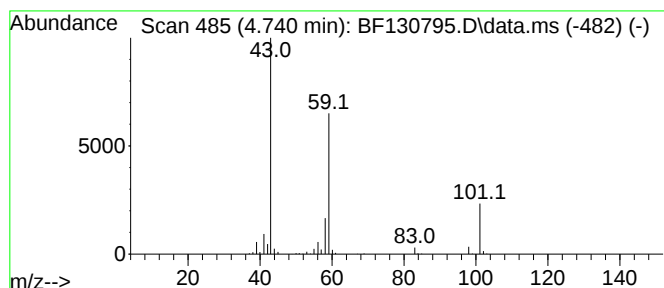

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130795.D
Acq On : 26 Oct 2022 21:46
Operator : CG\JU
Sample : N5281-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.740	13.6	ng	513058	1	6.563	754280	20.0