


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130780.D
 Acq On : 26 Oct 2022 11:20
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 27 08:55:38 2022

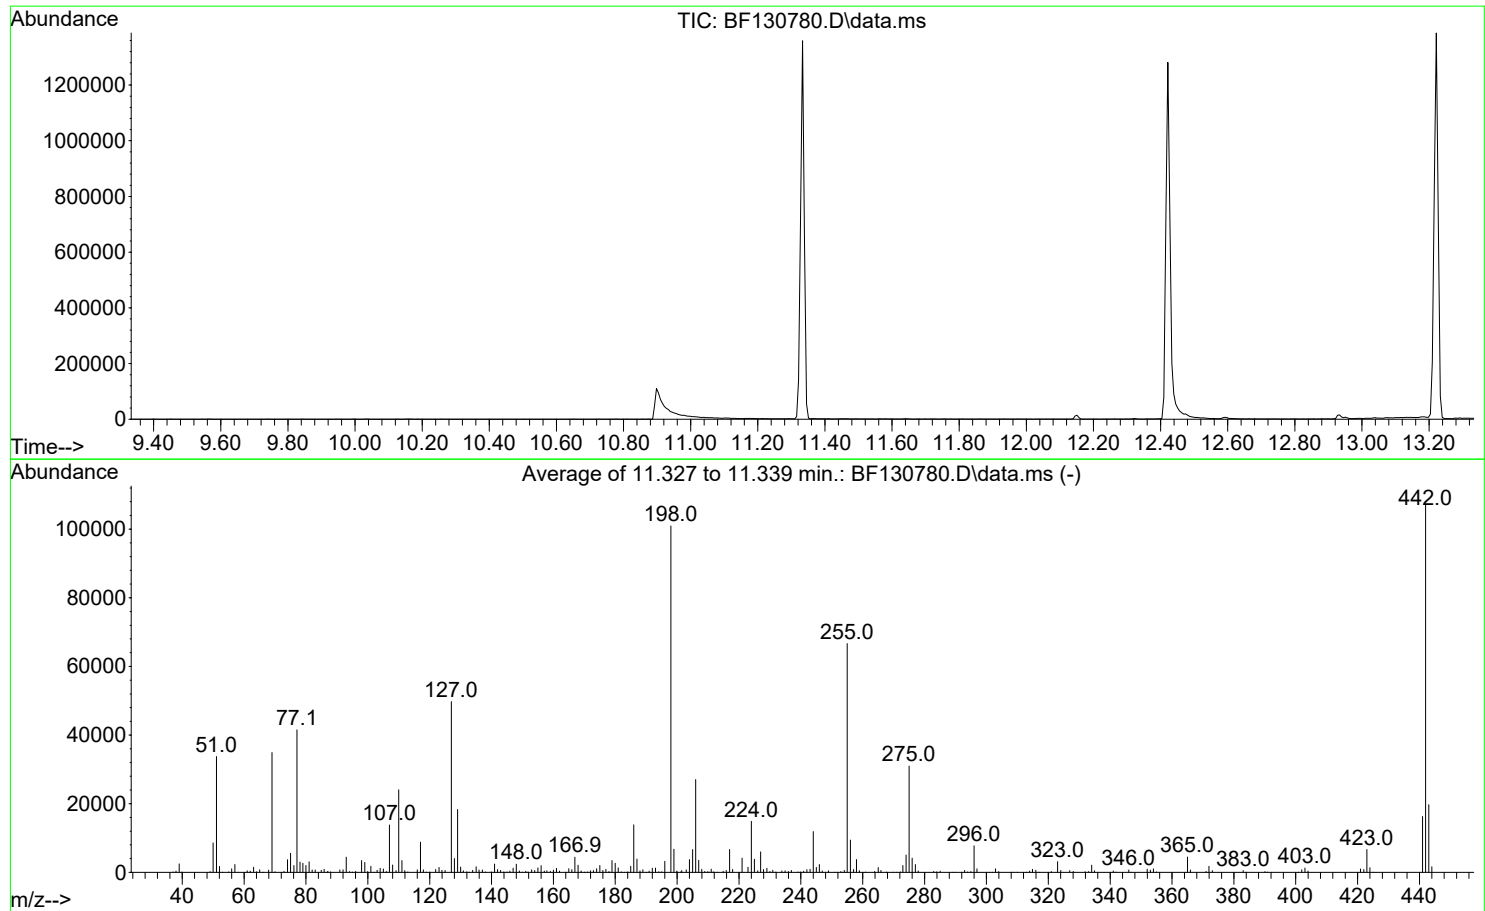

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	33748	PASS
68	69	0.00	2	1.9	648	PASS
69	198	0.00	100	34.6	34925	PASS
70	69	0.00	2	0.5	184	PASS
127	198	10	80	49.3	49749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100939	PASS
199	198	5	9	6.7	6780	PASS
275	198	10	60	30.7	30968	PASS
365	198	1	100	4.4	4472	PASS
441	198	0.01	100	16.1	16267	PASS
442	442	50	100	100.0	107179	PASS
443	442	15	24	18.4	19746	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/26/2022	BNA_F	<u>BF130780.D</u>
Compound Name	Response	Retention Time
DDT	234146	13.221
DDD	4646	12.933
DDE	1410	12.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6056	240202	2.52

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
Data File : BF130780.D
Acq On : 26 Oct 2022 11:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 09:13:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 27 08:55:38 2022
Response via : Initial Calibration

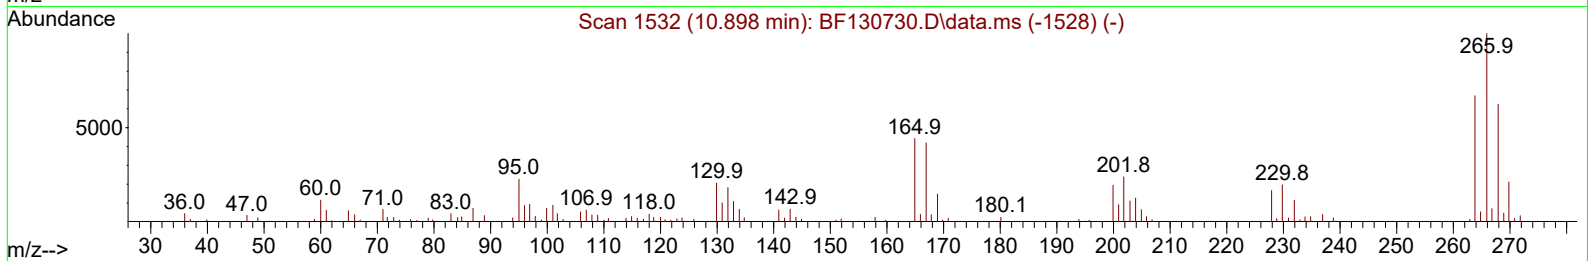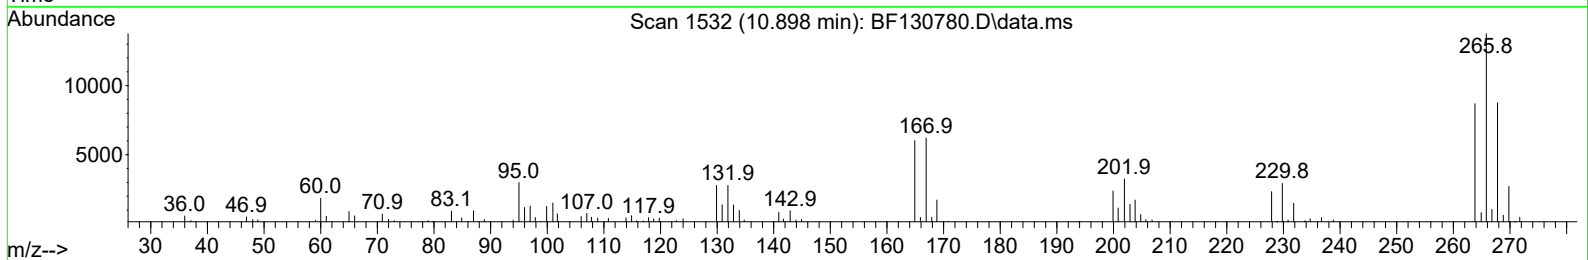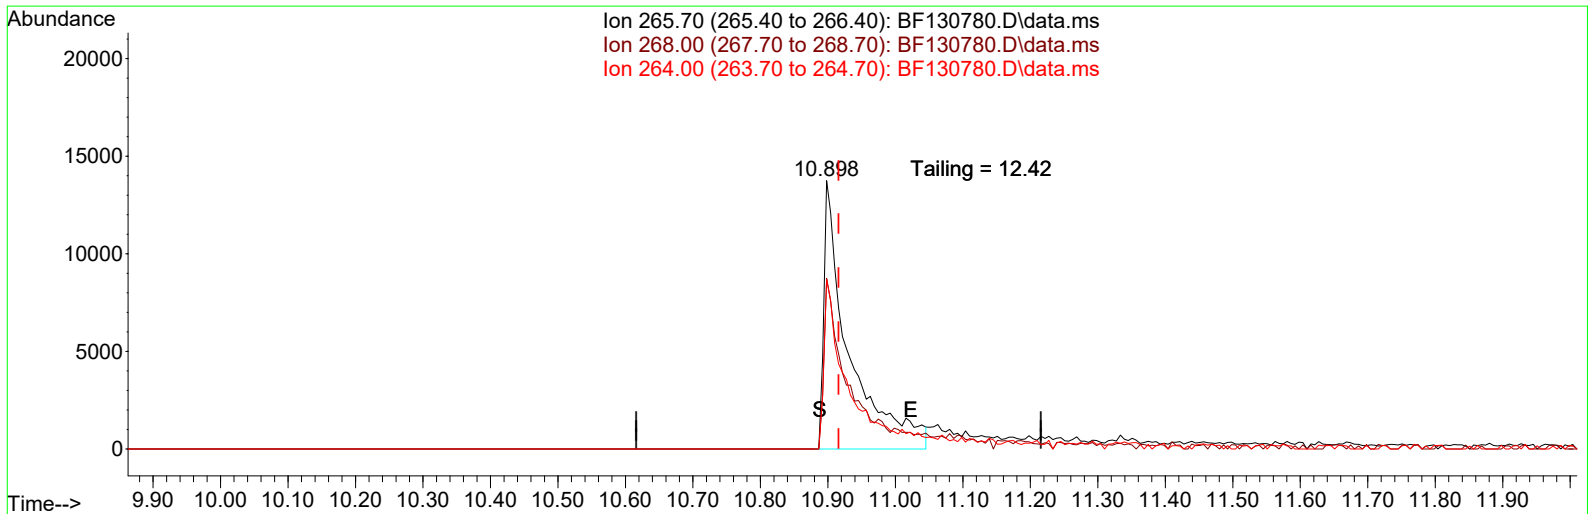

TIC: BF130780.D\data.ms

(70) Pentachlorophenol (C)

10.898min (-0.018) 2084.88 ng




response 32618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.65
264.00	67.00	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102622\
 Data File : BF130780.D
 Acq On : 26 Oct 2022 11:20
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 28 09:13:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 27 08:55:38 2022
 Response via : Initial Calibration

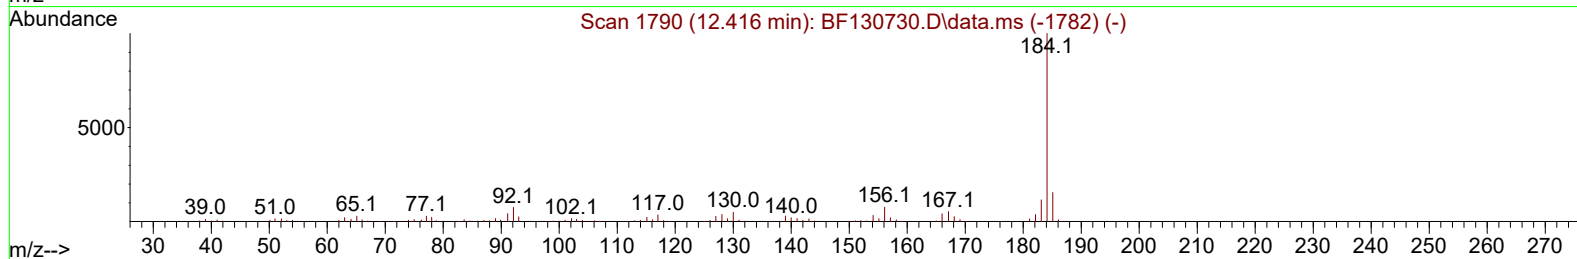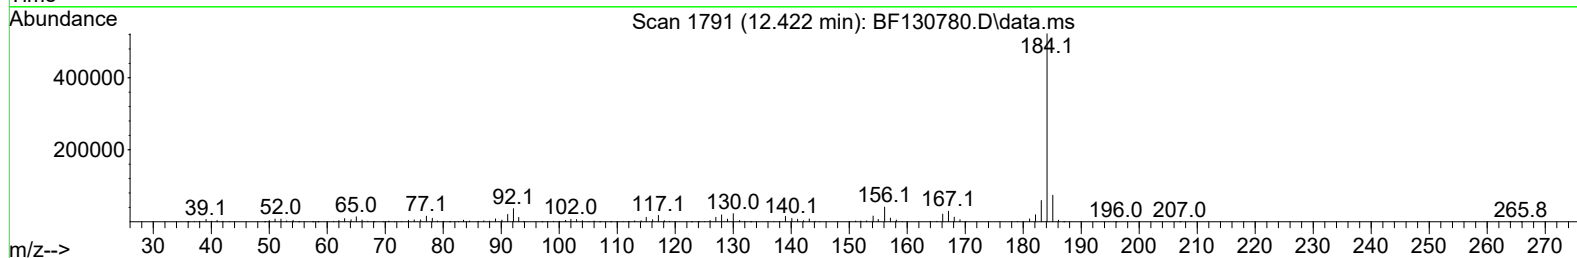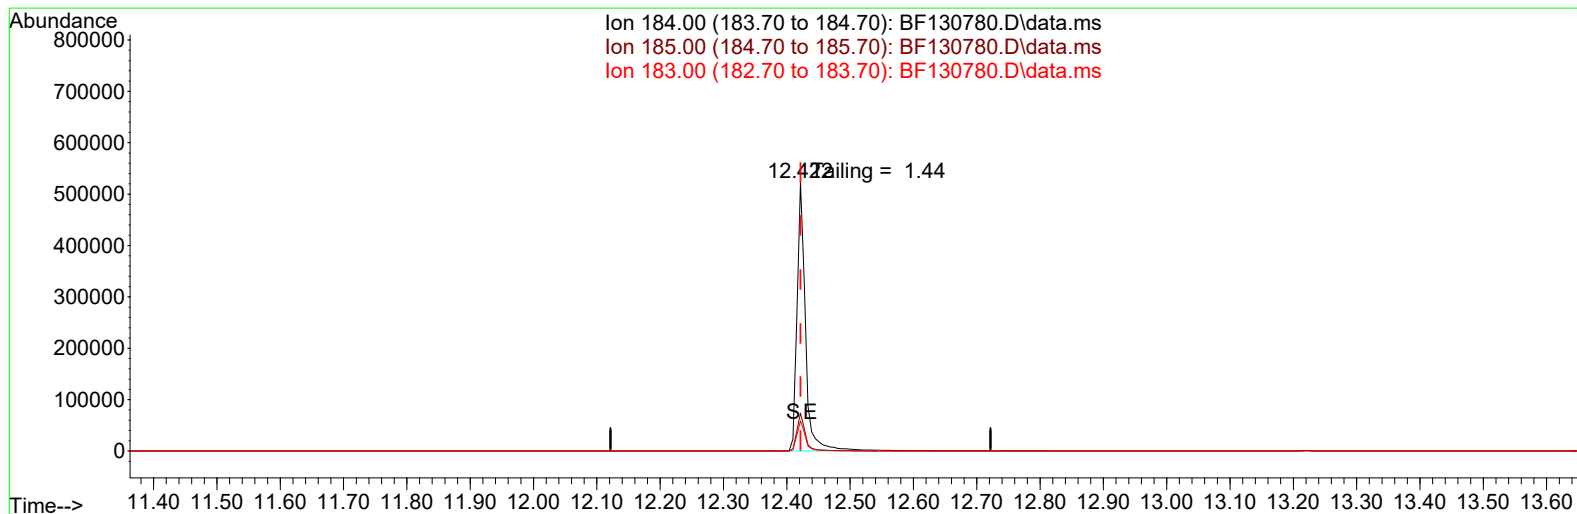

TIC: BF130780.D\data.ms

(77) Benzidine

12.422min (+ 0.000) 0.00 ng

response 492493

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	11.60	11.31
0.00	0.00	0.00