

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140051.D
Acq On : 26 Oct 2024 11:06
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	575	582	587	rBV	2486291	3510981	83.57%	13.567%
2	6.510	743	751	756	rBV	2350207	3505923	83.45%	13.548%
3	6.887	810	815	820	rBV	626658	764139	18.19%	2.953%
4	7.445	903	910	916	rBV	1630348	2363252	56.25%	9.132%
5	8.169	1027	1033	1038	rBV	773104	1000502	23.82%	3.866%
6	9.245	1208	1216	1221	rBV	3041867	4184127	99.60%	16.169%
7	9.922	1325	1331	1346	rBV	879712	1154476	27.48%	4.461%
8	10.710	1459	1465	1484	rBV	1837731	2539191	60.44%	9.812%
9	11.410	1579	1584	1592	rBV	934903	1163286	27.69%	4.495%
10	12.998	1848	1854	1859	rBV	3190345	4201133	100.00%	16.234%
11	14.051	2025	2033	2052	rBV	600467	854095	20.33%	3.300%
12	15.527	2278	2284	2303	rVB	356810	636984	15.16%	2.461%




Sum of corrected areas: 25878089

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140051.D
Acq On : 26 Oct 2024 11:06
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

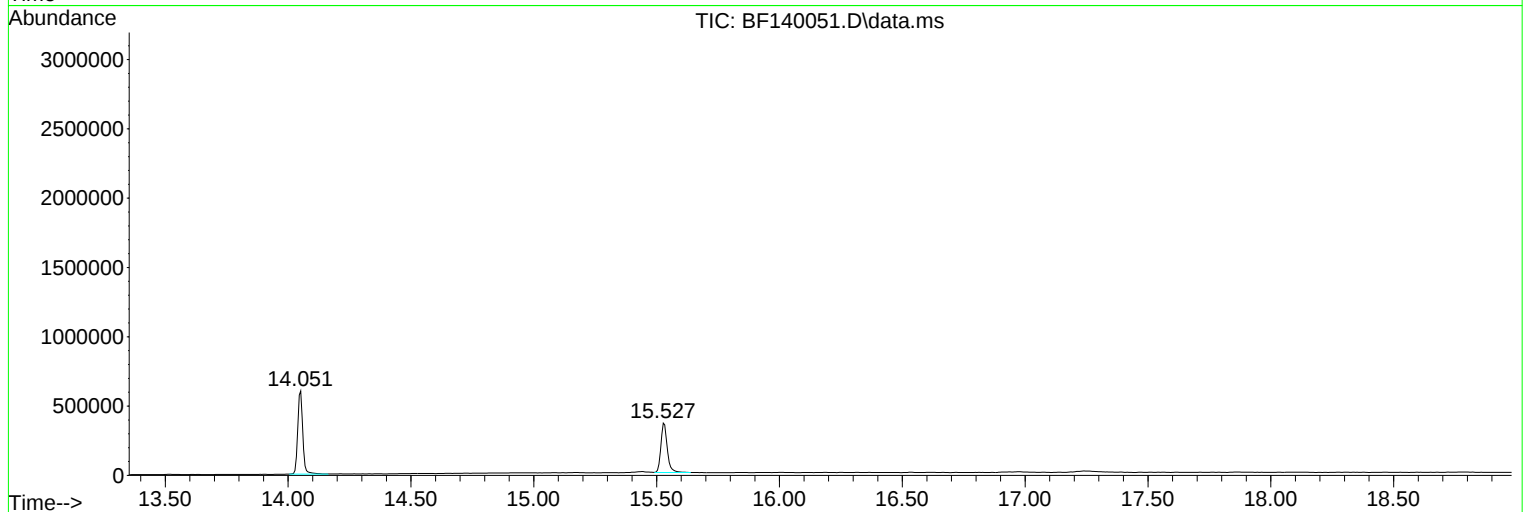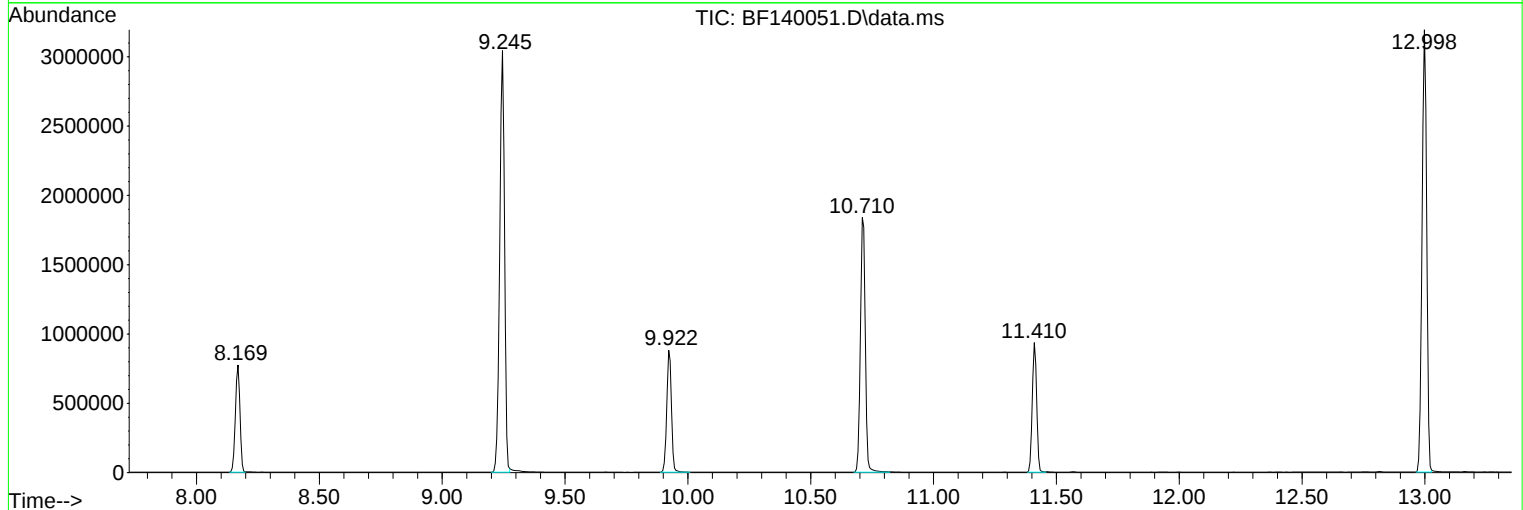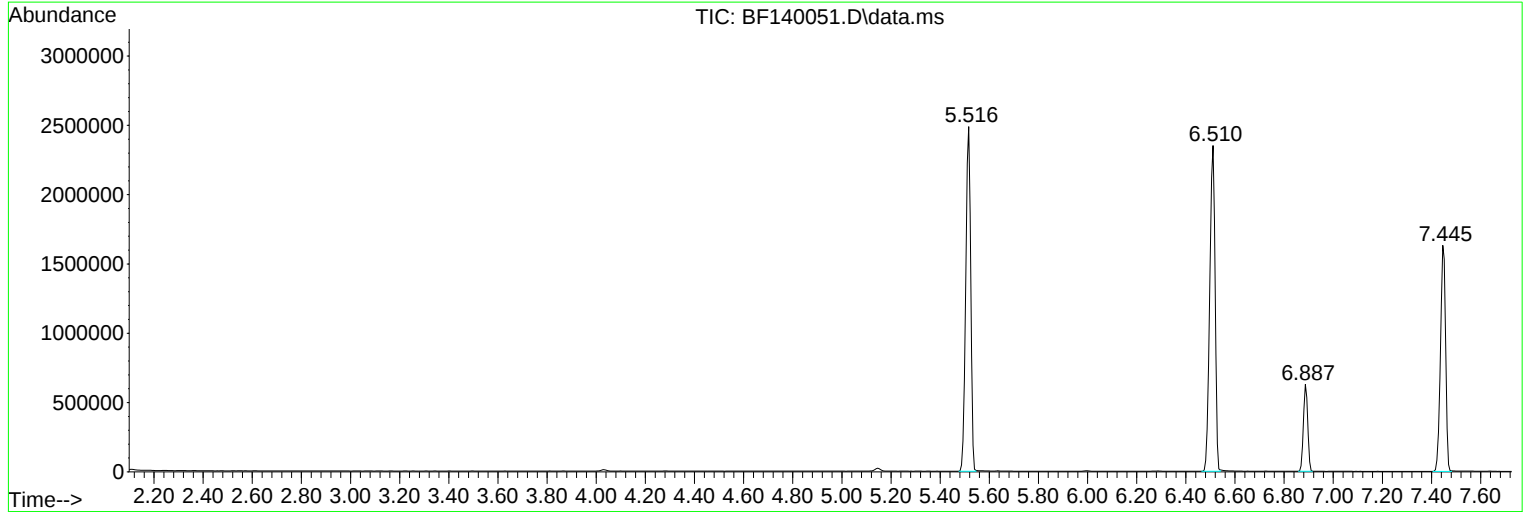

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140051.D
Acq On : 26 Oct 2024 11:06
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140051.D
Acq On : 26 Oct 2024 11:06
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------