
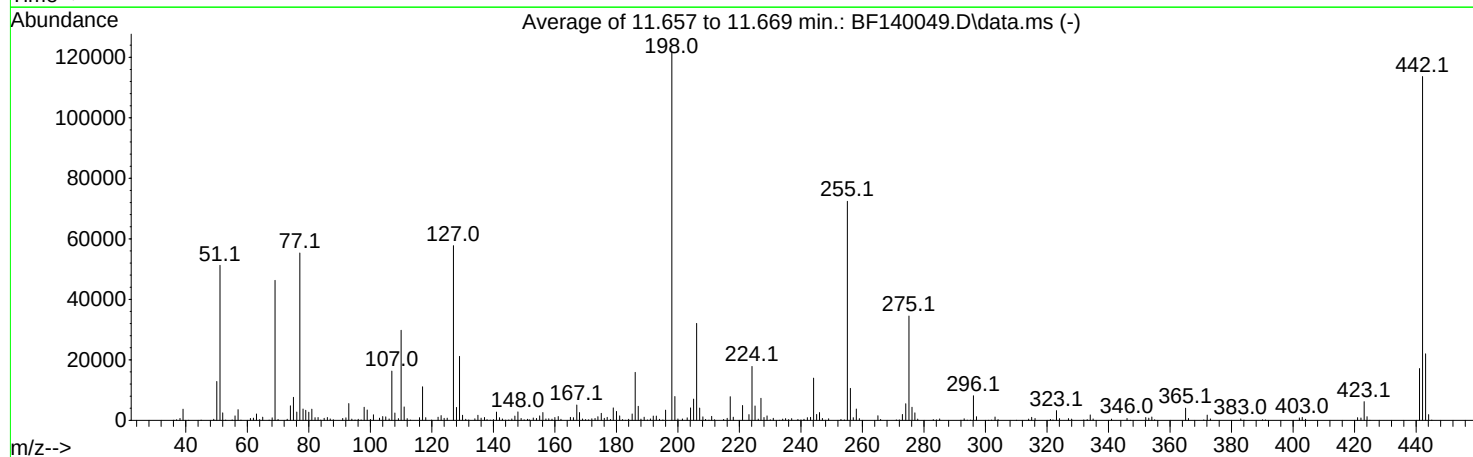


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140049.D
Acq On : 26 Oct 2024 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

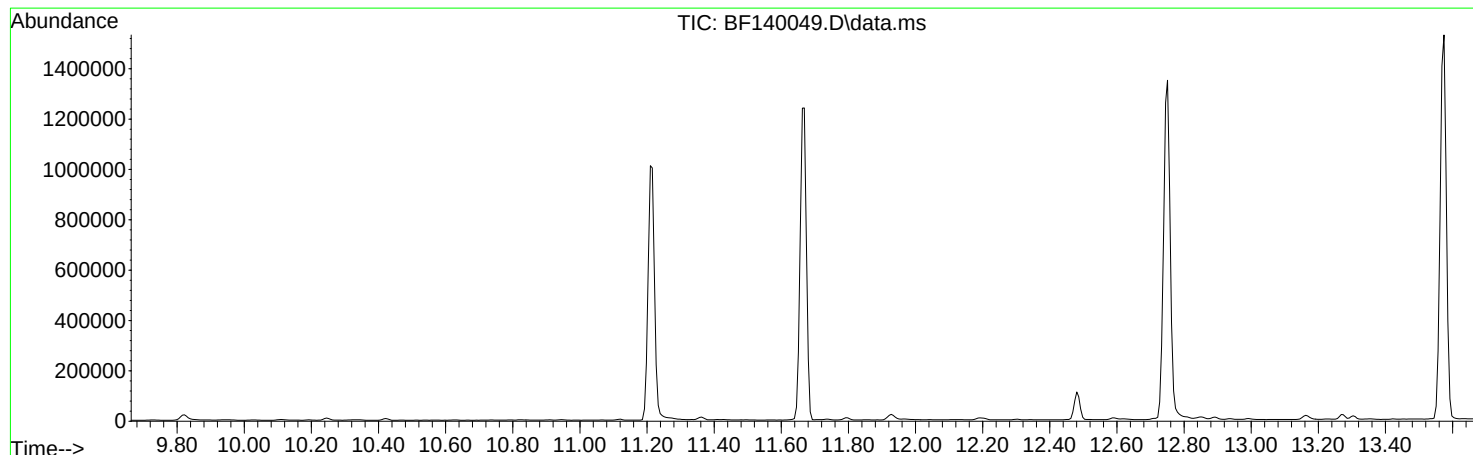




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	42.1	51240	PASS
68	69	0.00	2	1.8	856	PASS
69	198	0.00	100	38.1	46282	PASS
70	69	0.00	2	0.7	328	PASS
127	198	10	80	47.5	57773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121589	PASS
199	198	5	9	6.5	7892	PASS
275	198	10	60	28.3	34461	PASS
365	198	1	100	3.3	4026	PASS
441	198	0.01	100	14.1	17140	PASS
442	442	50	100	100.0	113635	PASS
443	442	15	24	19.4	22013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140049.D
Acq On : 26 Oct 2024 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 01:04:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

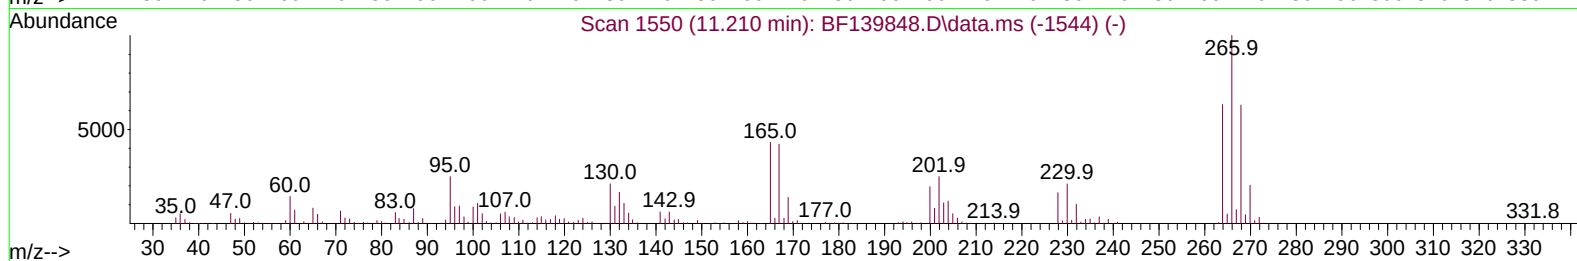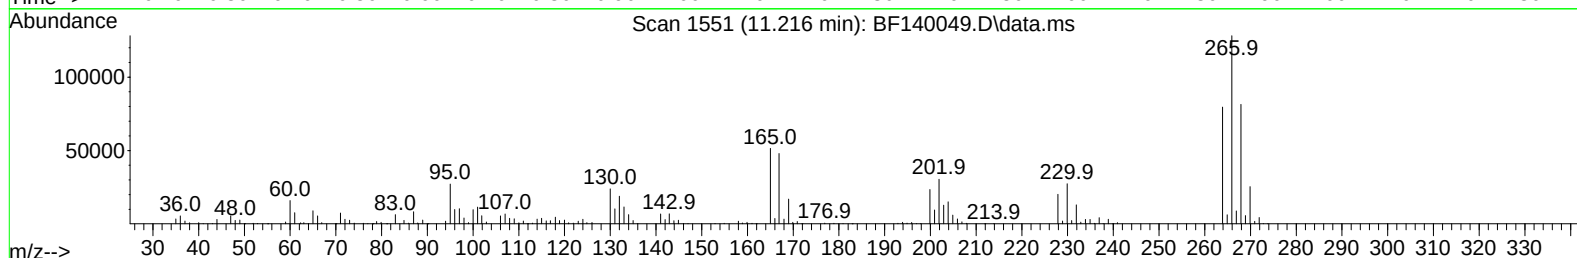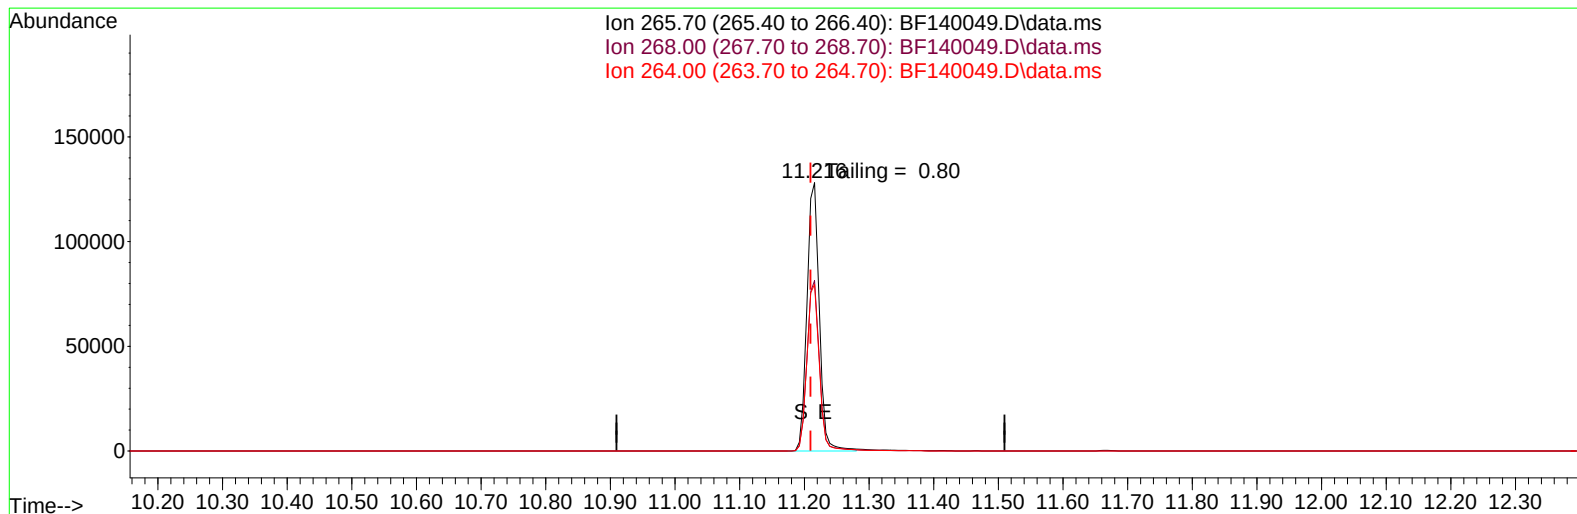

TIC: BF140049.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 14128.66 ng




response 173165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.52
264.00	63.20	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102624\
Data File : BF140049.D
Acq On : 26 Oct 2024 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 01:04:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

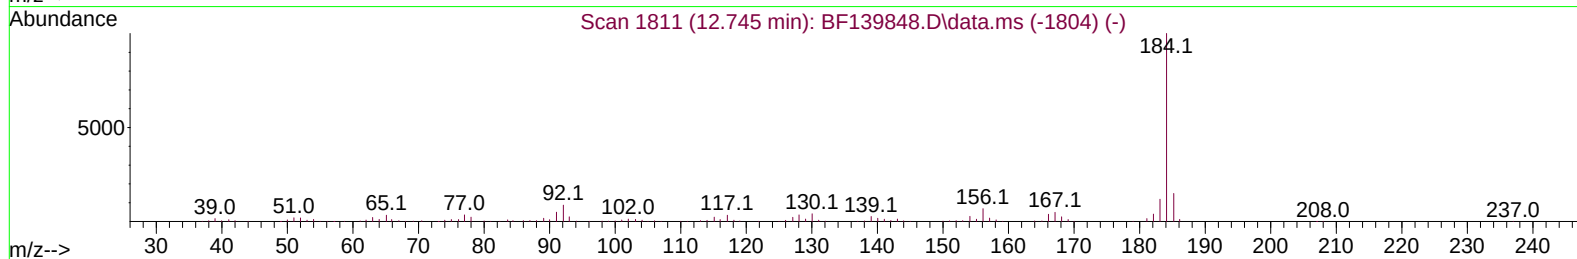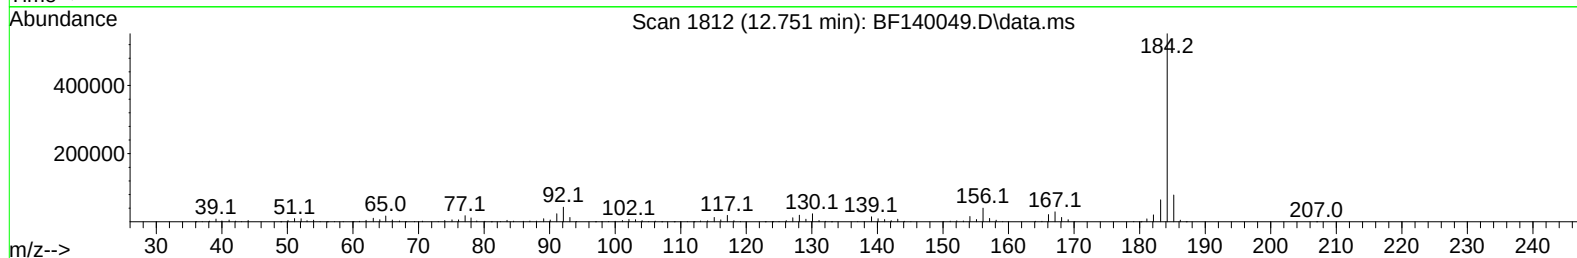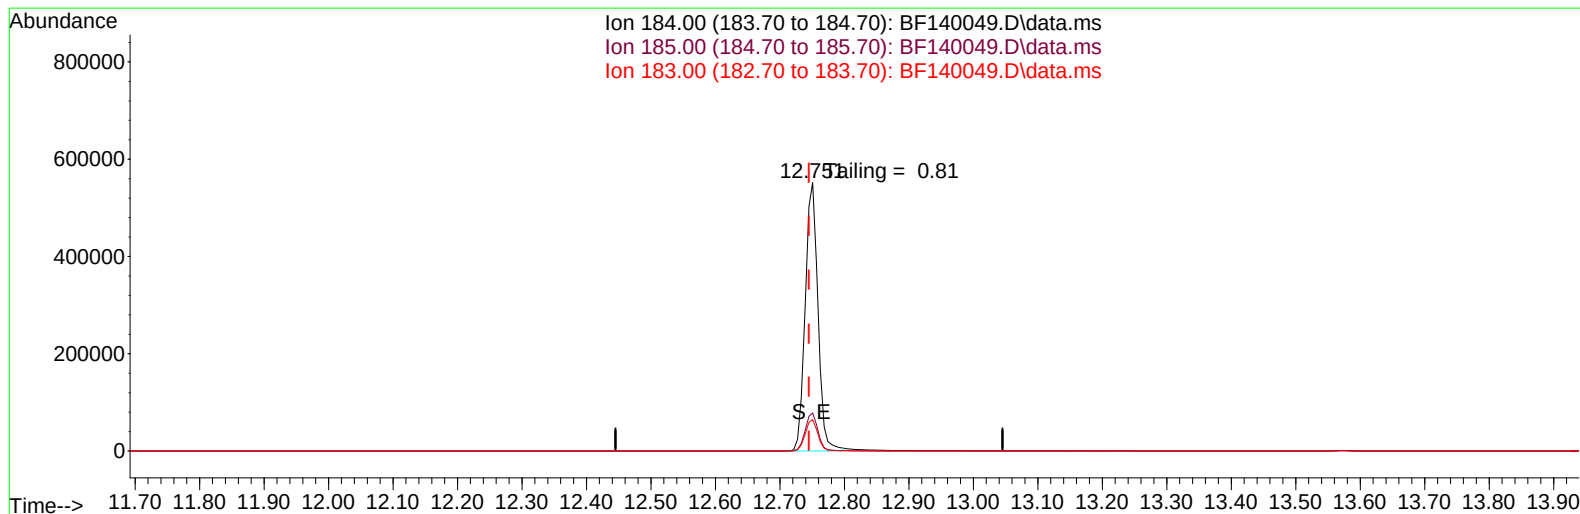

TIC: BF140049.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 46047.22 ng

response 771559

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.21
183.00	11.80	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2024	BNA_F	<u>BF140049.D</u>
Compound Name	Response	Retention Time
DDT	384498	13.574
DDD	9181	13.274
DDE	1042	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10223	394721	2.59

Instrument :
BNA_F
ClientSampleId :
DFTPP