
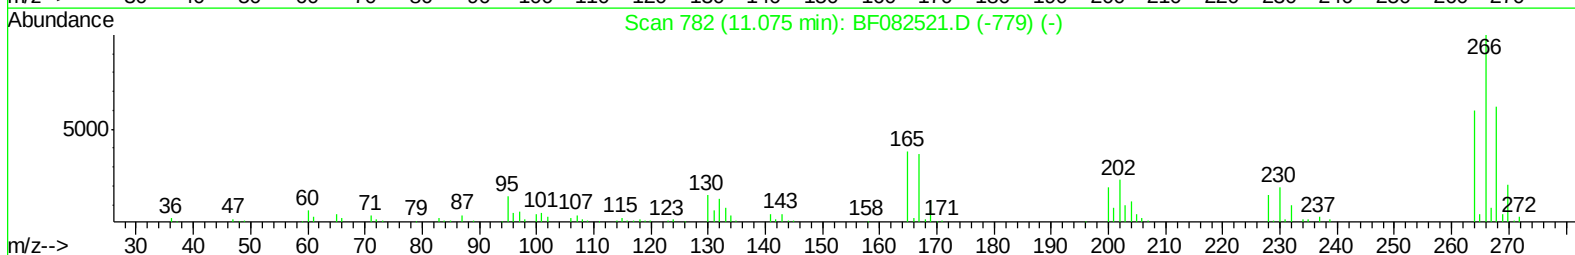
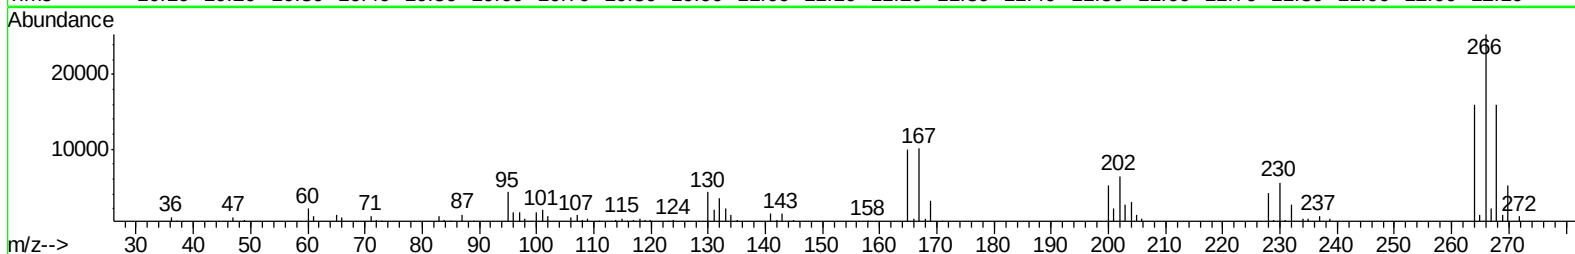


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102715\
Data File : BF082569.D
Acq On : 28 Oct 2015 2:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 06:29:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

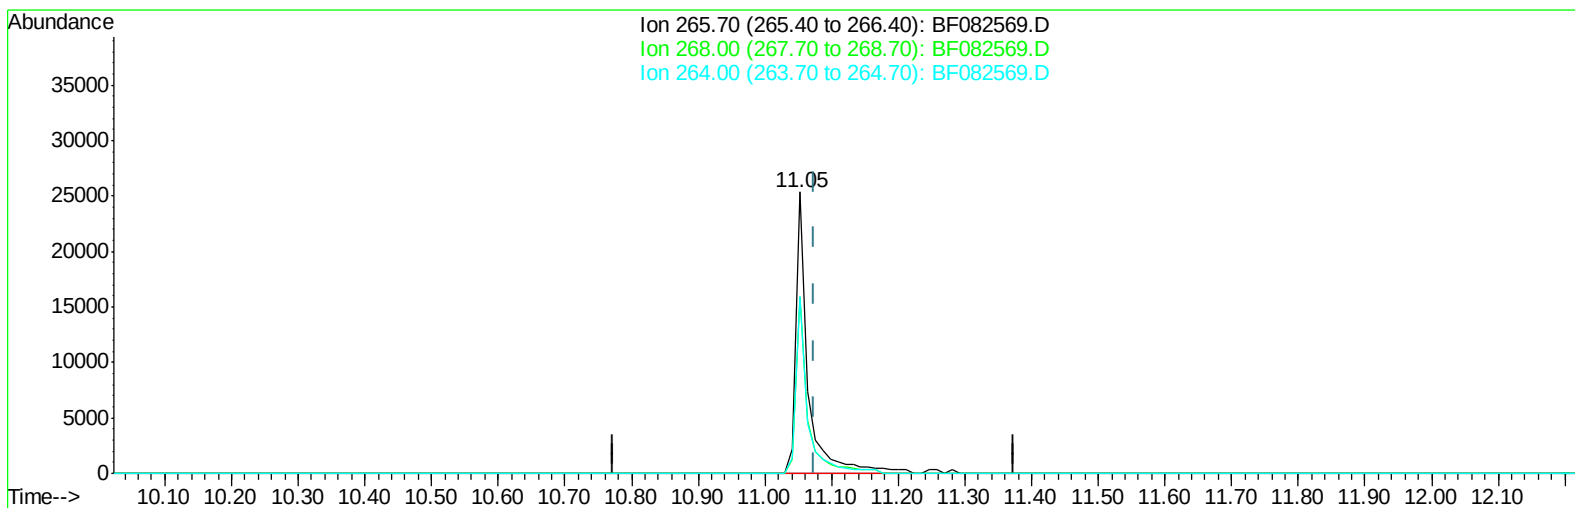

TIC: BF082569.D

(69) Pentachlorophenol (C)




11.052min (-0.022) 0.00ng

response 32371

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	62.85
264.00	60.00	62.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102715\
Data File : BF082569.D
Acq On : 28 Oct 2015 2:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 06:29:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

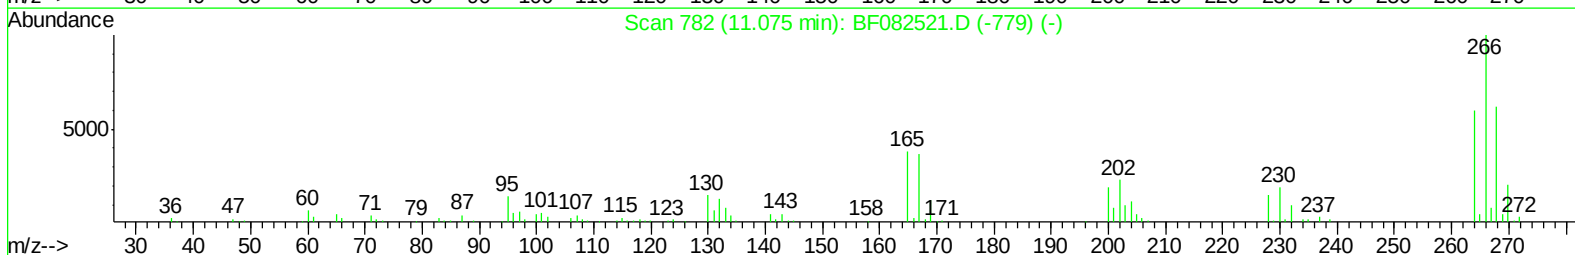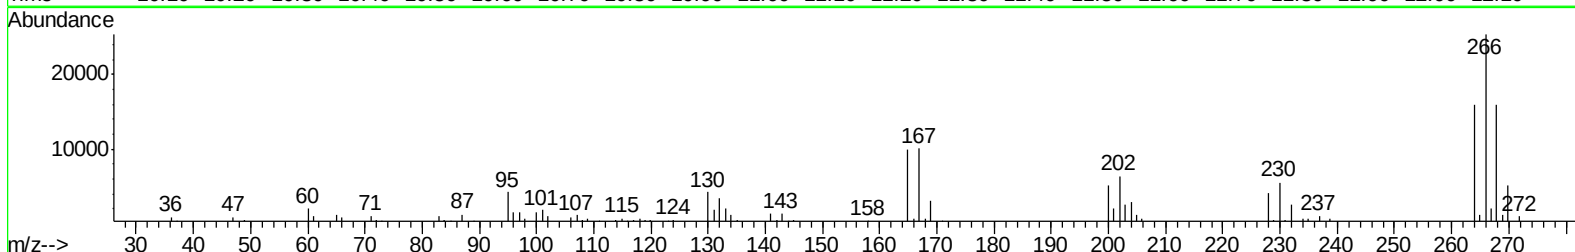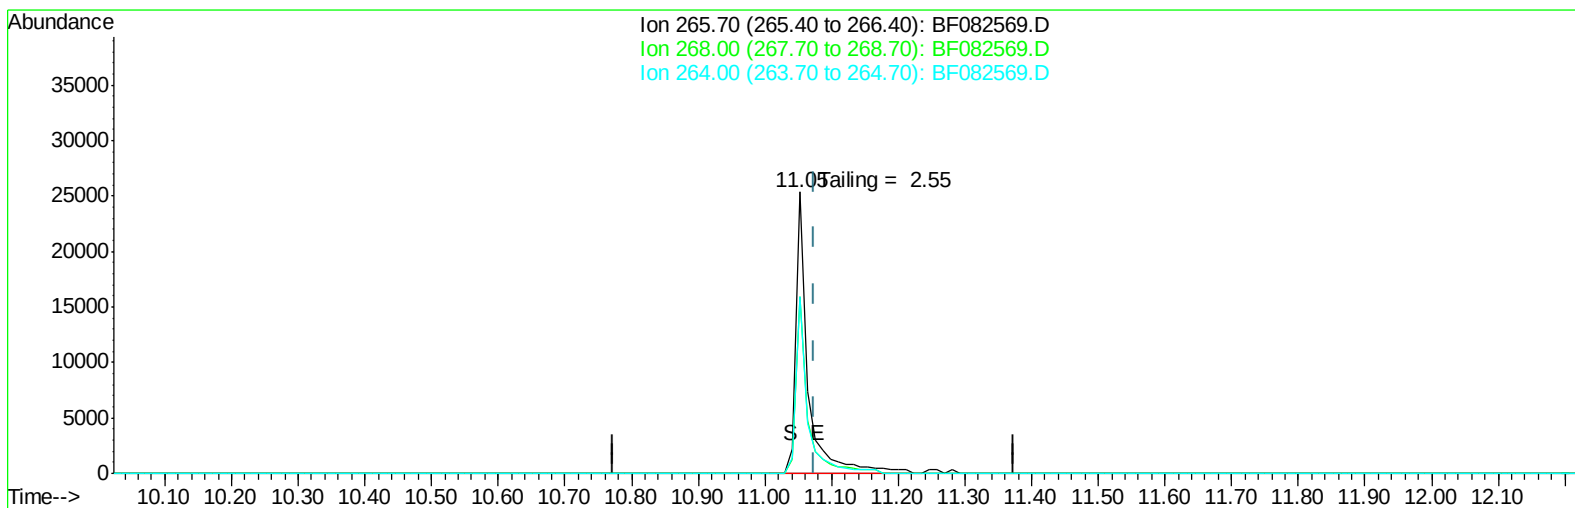

TIC: BF082569.D

(69) Pentachlorophenol (C)




11.052min (-0.022) 0.00ng

response 32371

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	62.85
264.00	60.00	62.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102715\
Data File : BF082569.D
Acq On : 28 Oct 2015 2:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 06:29:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

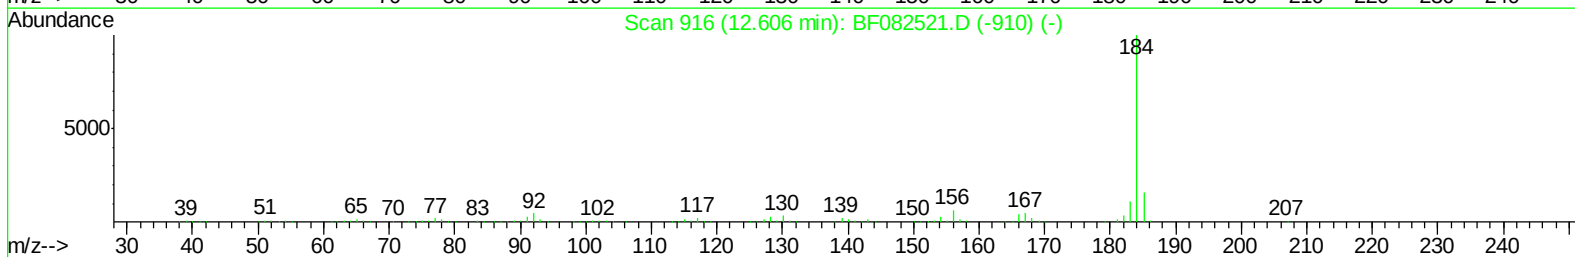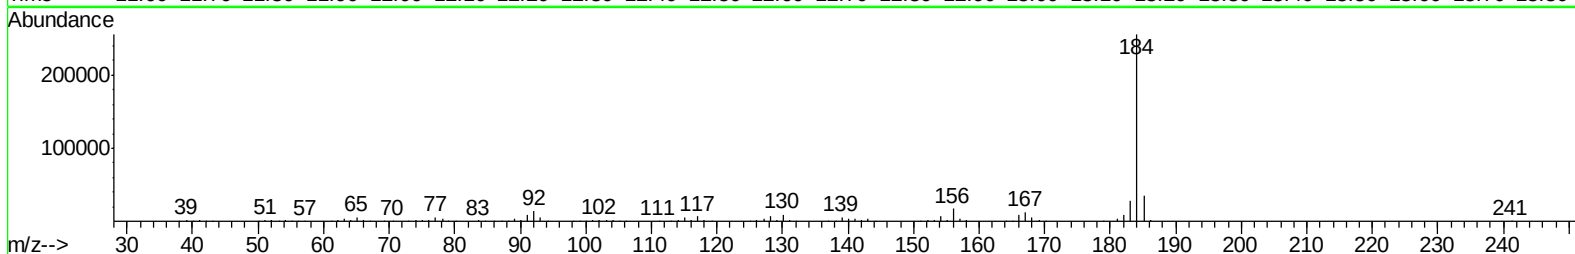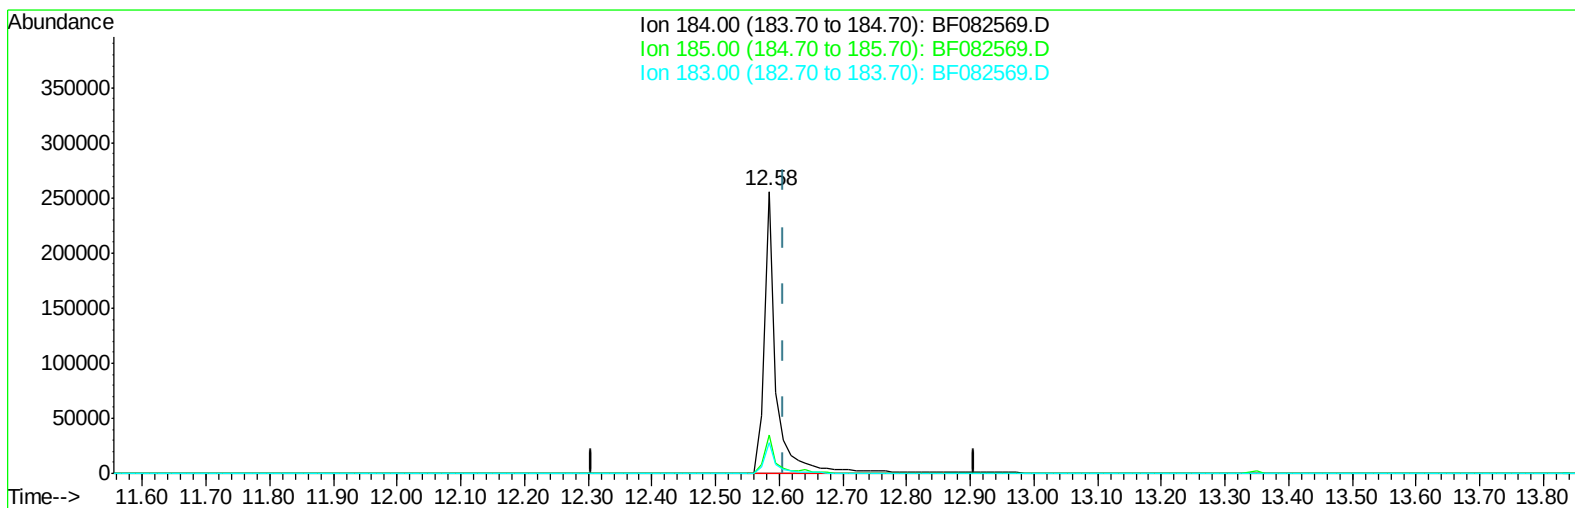

TIC: BF082569.D

(76) Benzidine




12.584min (-0.023) 0.00ng

response 341515

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	13.87
183.00	11.10	11.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102715\
Data File : BF082569.D
Acq On : 28 Oct 2015 2:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 06:29:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

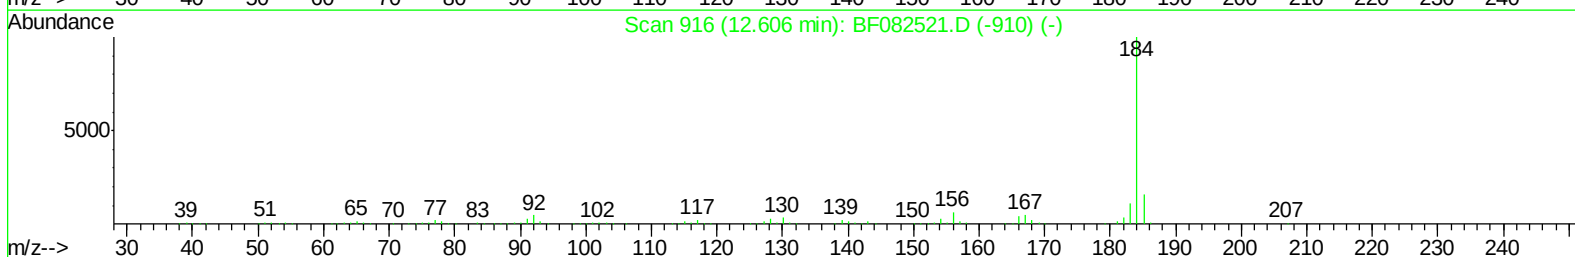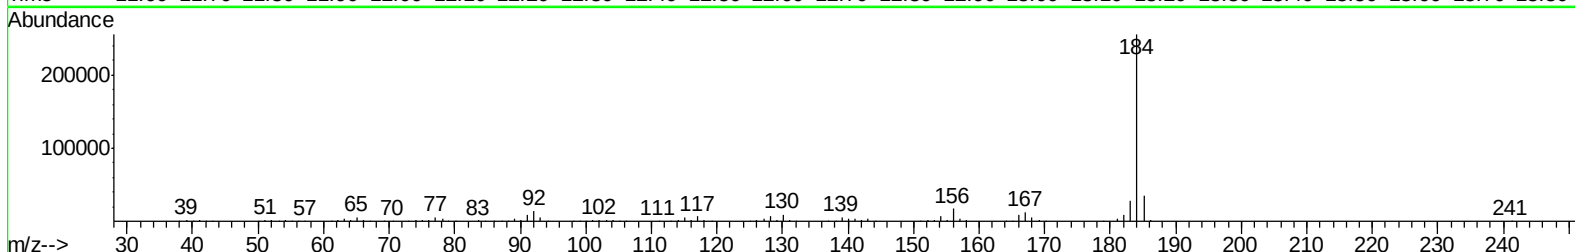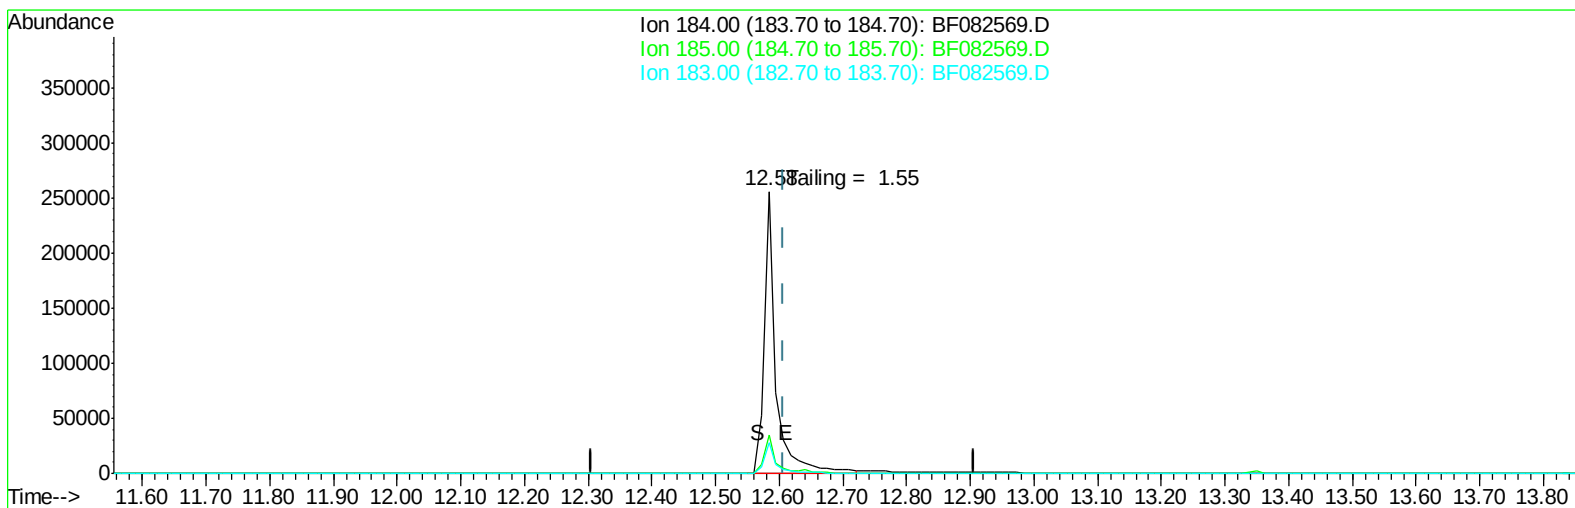

TIC: BF082569.D

(76) Benzidine

12.584min (-0.023) 0.00ng

response 341515

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	13.87
183.00	11.10	11.14
0.00	0.00	0.00