


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102715\
 Data File : BF082550.D
 Acq On : 27 Oct 2015 15:43
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 27 02:43:58 2015

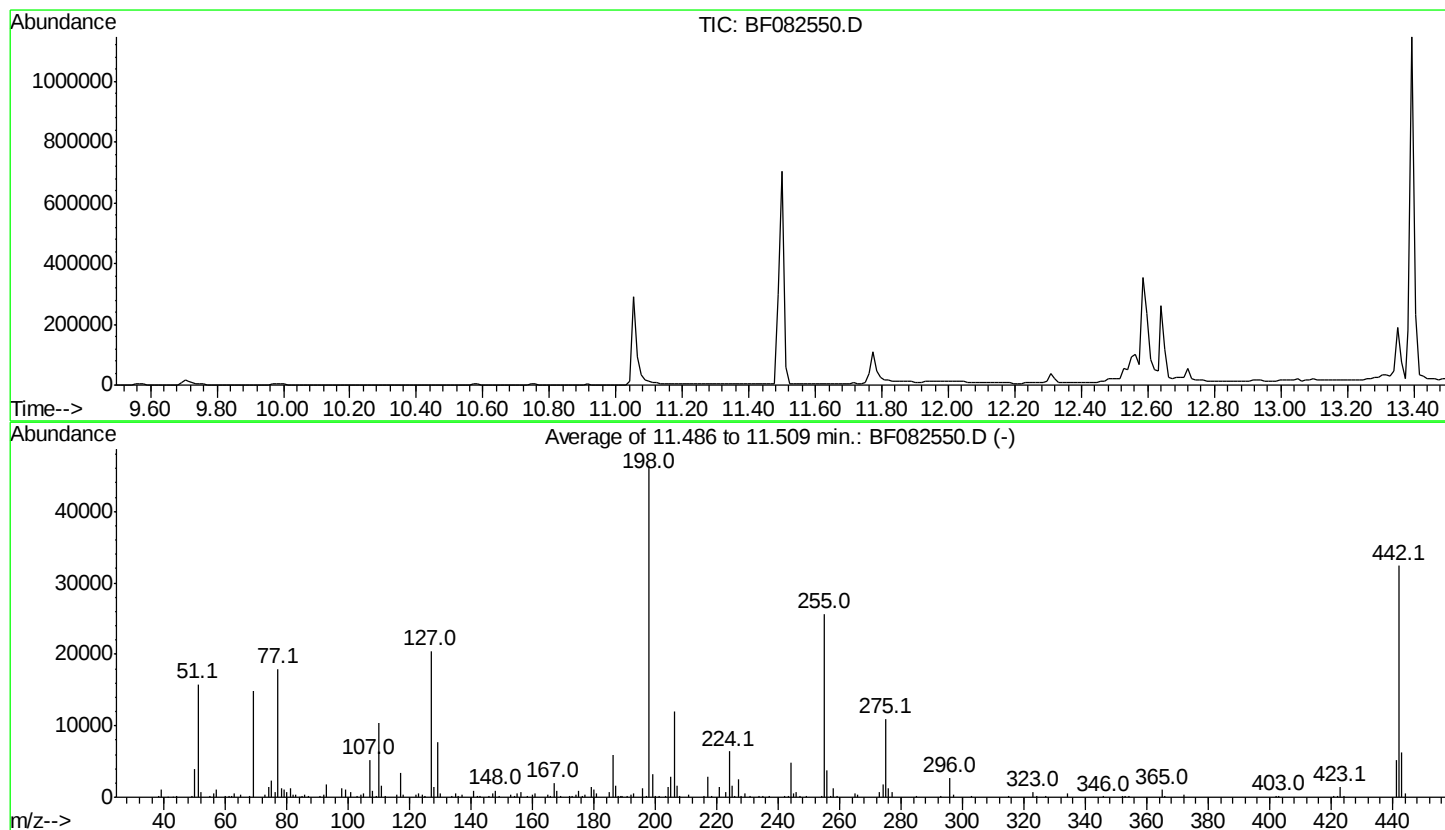

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	15792	PASS
68	69	0.00	2	1.8	263	PASS
69	198	0.00	100	32.0	14867	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	20508	PASS
197	198	0.00	2	0.4	202	PASS
198	198	100	100	100.0	46411	PASS
199	198	5	9	6.9	3190	PASS
275	198	10	60	23.6	10976	PASS
365	198	1	100	2.3	1057	PASS
441	442	0.01	24	16.3	5274	PASS
442	198	50	100	69.8	32378	PASS
443	442	15	24	19.1	6190	PASS