


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102715\
 Data File : BF082569.D
 Acq On : 28 Oct 2015 2:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 27 02:43:58 2015

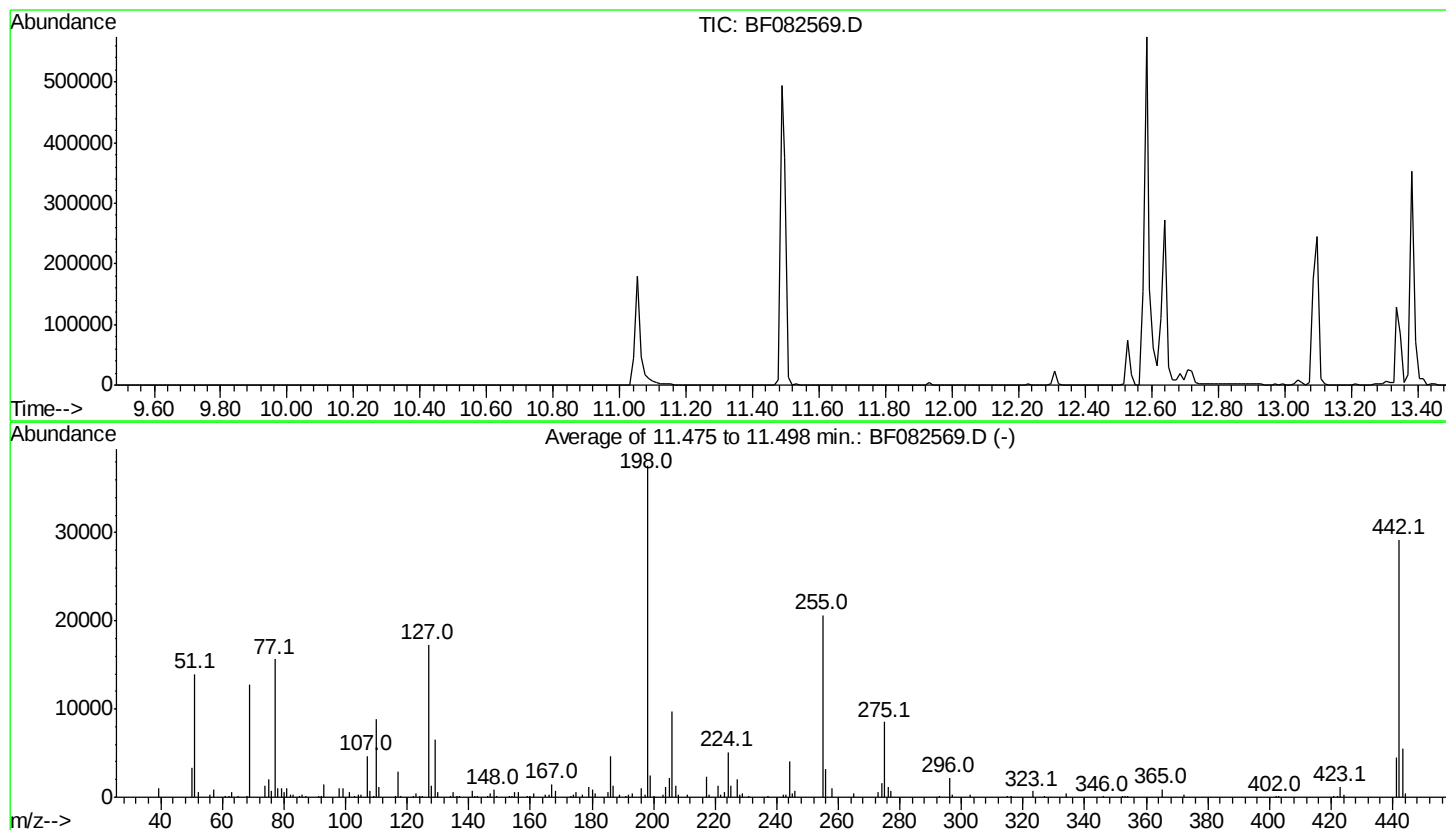

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	14002	PASS
68	69	0.00	2	1.3	173	PASS
69	198	0.00	100	34.1	12826	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	17311	PASS
197	198	0.00	2	0.7	253	PASS
198	198	100	100	100.0	37626	PASS
199	198	5	9	6.6	2488	PASS
275	198	10	60	22.8	8564	PASS
365	198	1	100	2.5	939	PASS
441	442	0.01	24	15.6	4553	PASS
442	198	50	100	77.6	29206	PASS
443	442	15	24	18.9	5515	PASS