
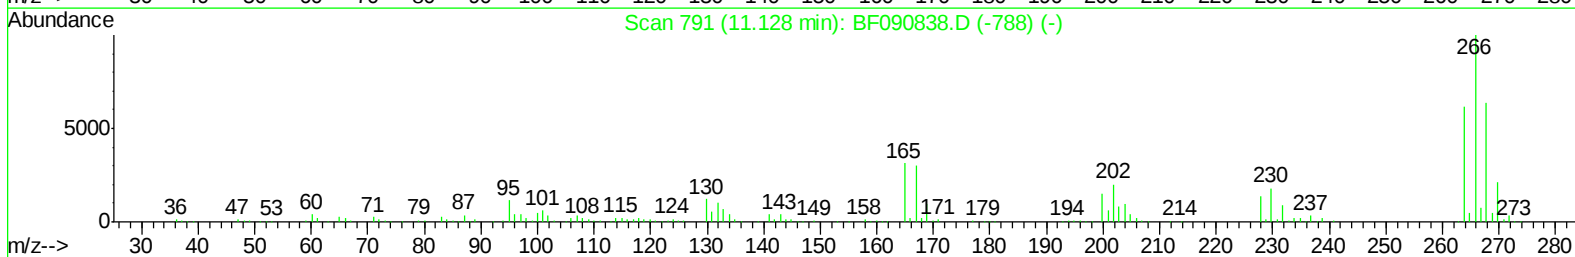
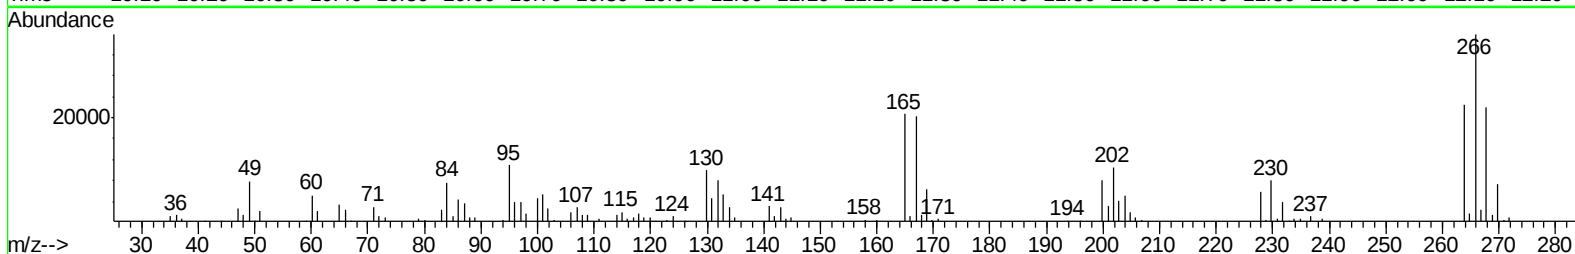


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data File : BF090866.D
Acq On : 27 Oct 2016 11:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:09:16 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 27 18:46:43 2016
Response via : Initial Calibration

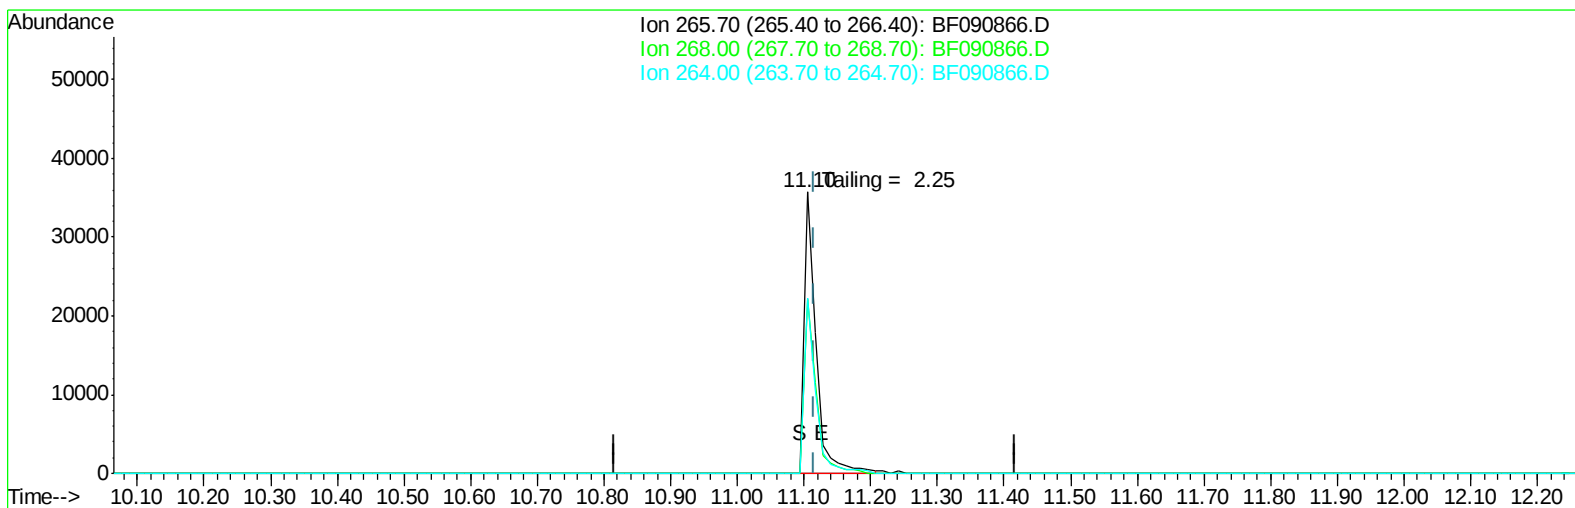

TIC: BF090866.D

(69) Pentachlorophenol (C)




11.105min (-0.012) 0.00ng

response 44139

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	61.61
264.00	62.70	62.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data File : BF090866.D
Acq On : 27 Oct 2016 11:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:09:16 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 27 18:46:43 2016
Response via : Initial Calibration

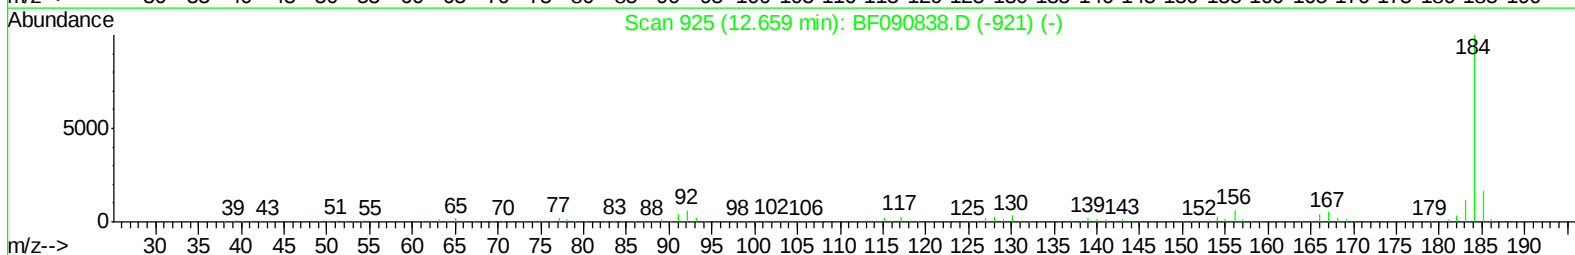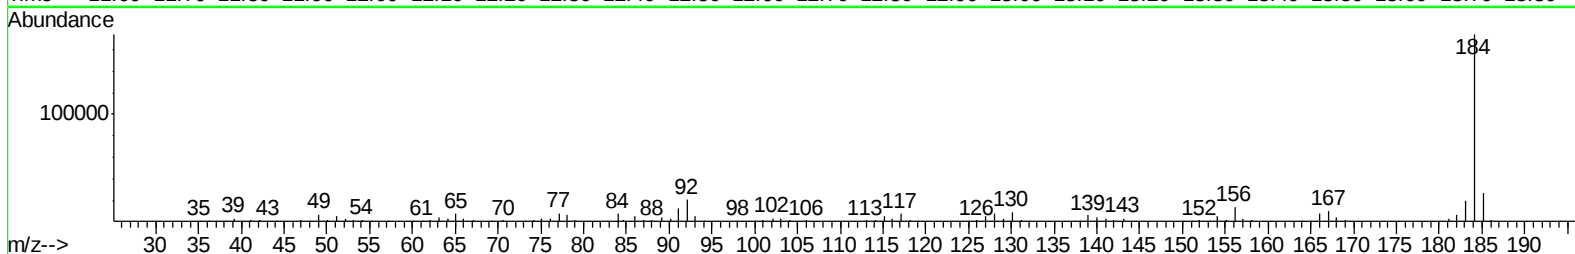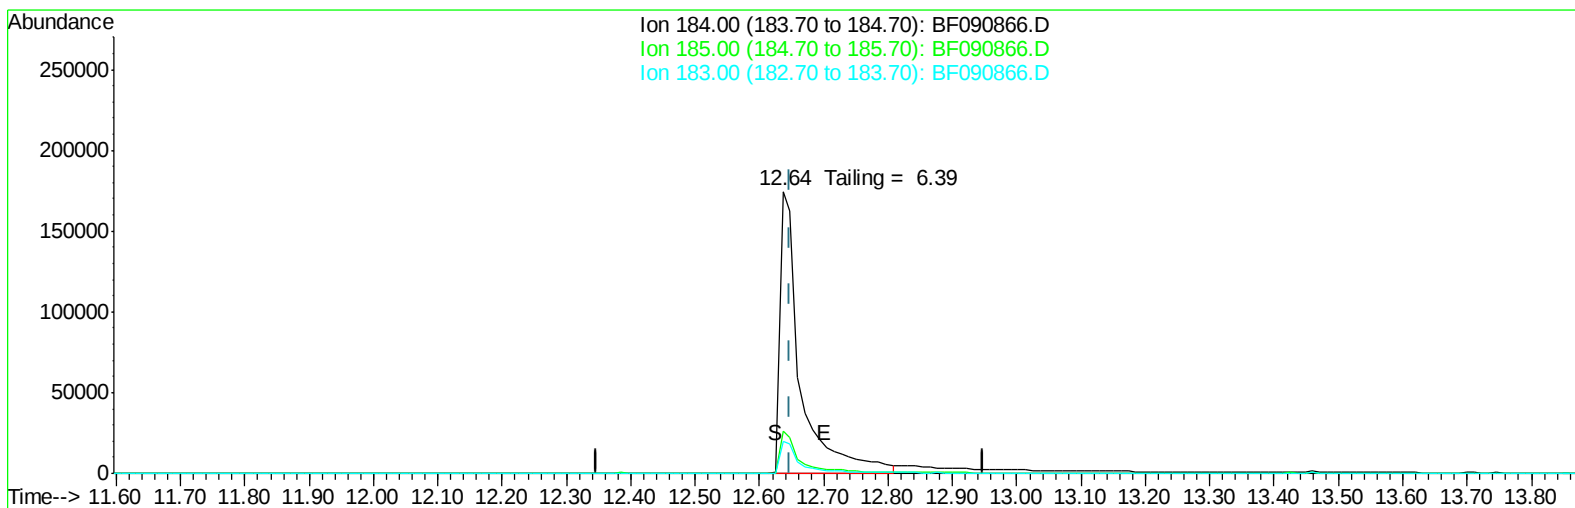

TIC: BF090866.D

(76) Benzidine

12.636min (-0.012) 39428.90ng m

response 395164

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.01
183.00	9.50	11.36
0.00	0.00	0.00