
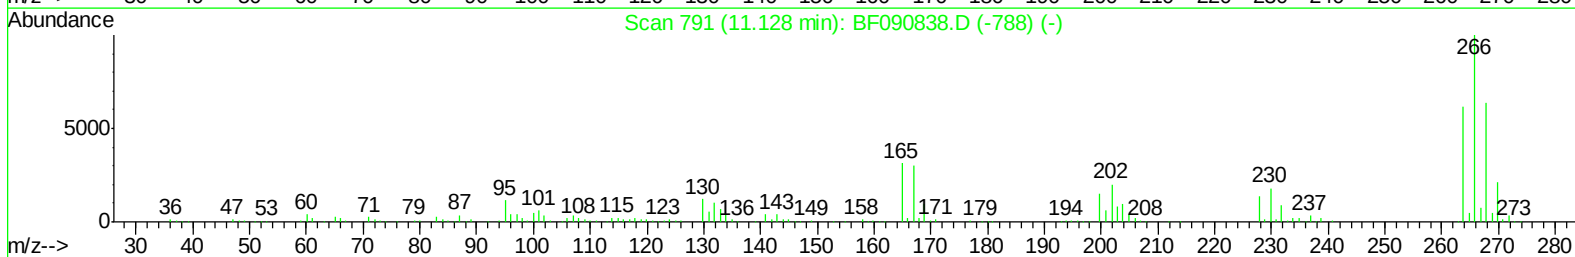
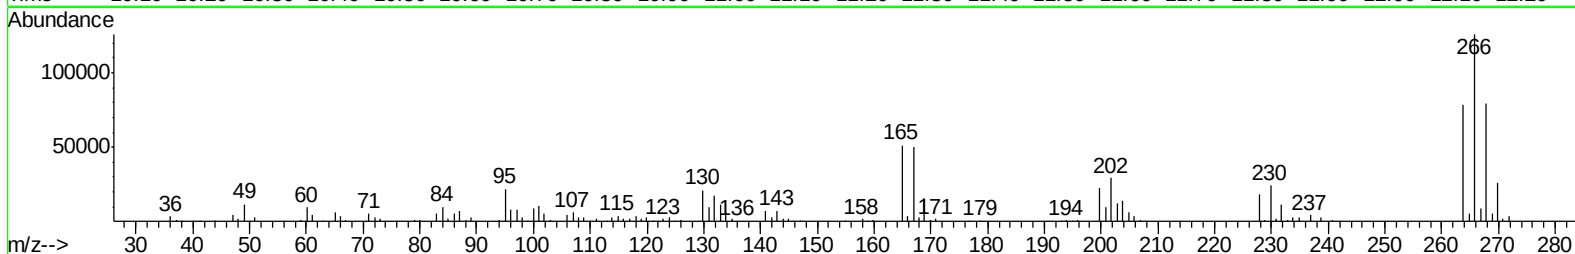


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data File : BF090873.D
Acq On : 27 Oct 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:10:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 27 18:46:43 2016
Response via : Initial Calibration

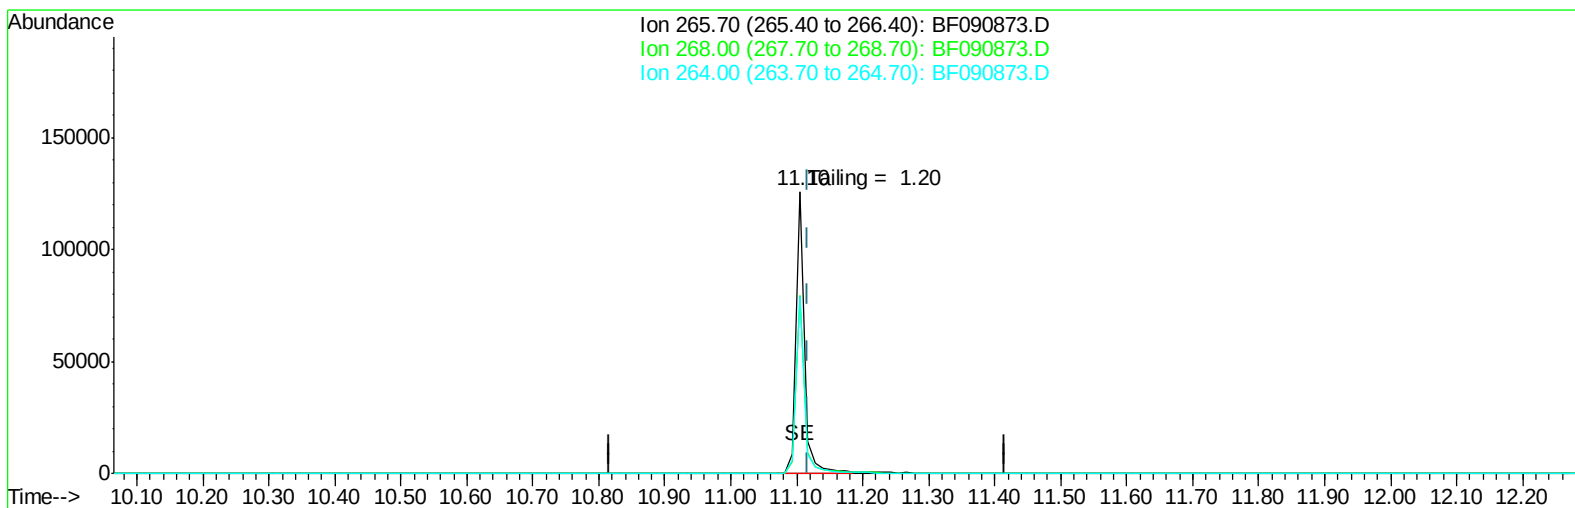

TIC: BF090873.D

(69) Pentachlorophenol (C)




11.105min (-0.011) 0.00ng

response 111443

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.99
264.00	62.70	62.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data File : BF090873.D
Acq On : 27 Oct 2016 16:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:10:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 27 18:46:43 2016
Response via : Initial Calibration

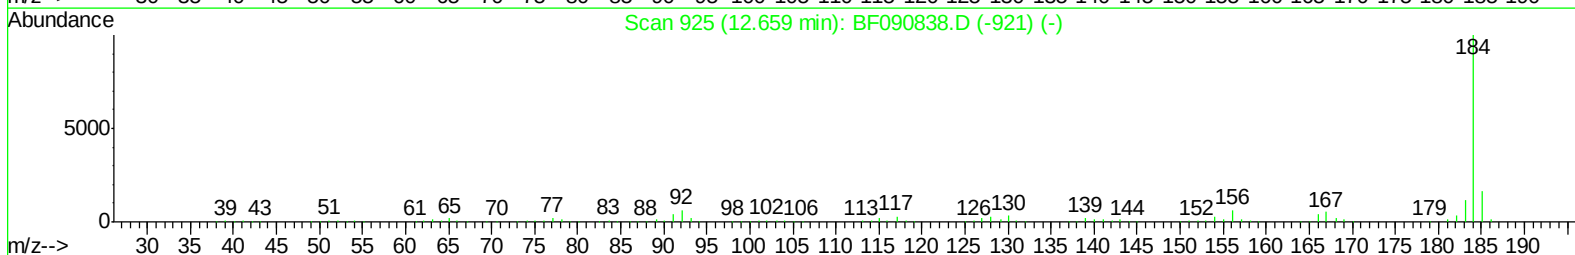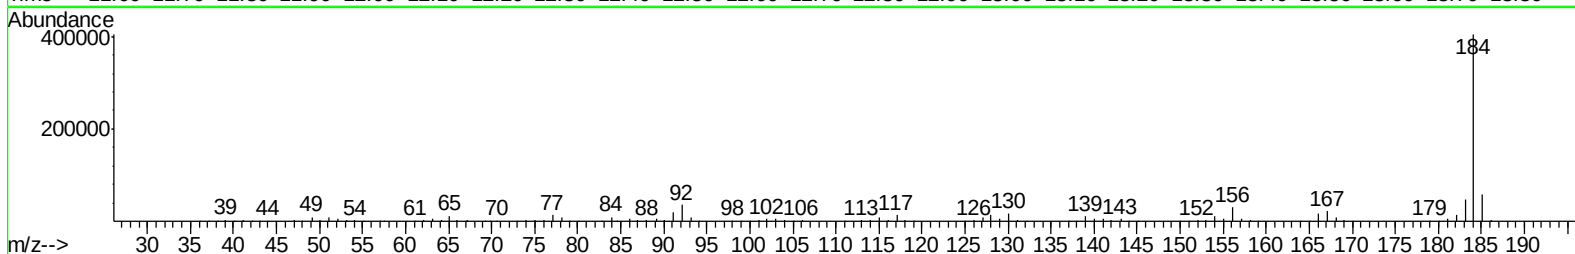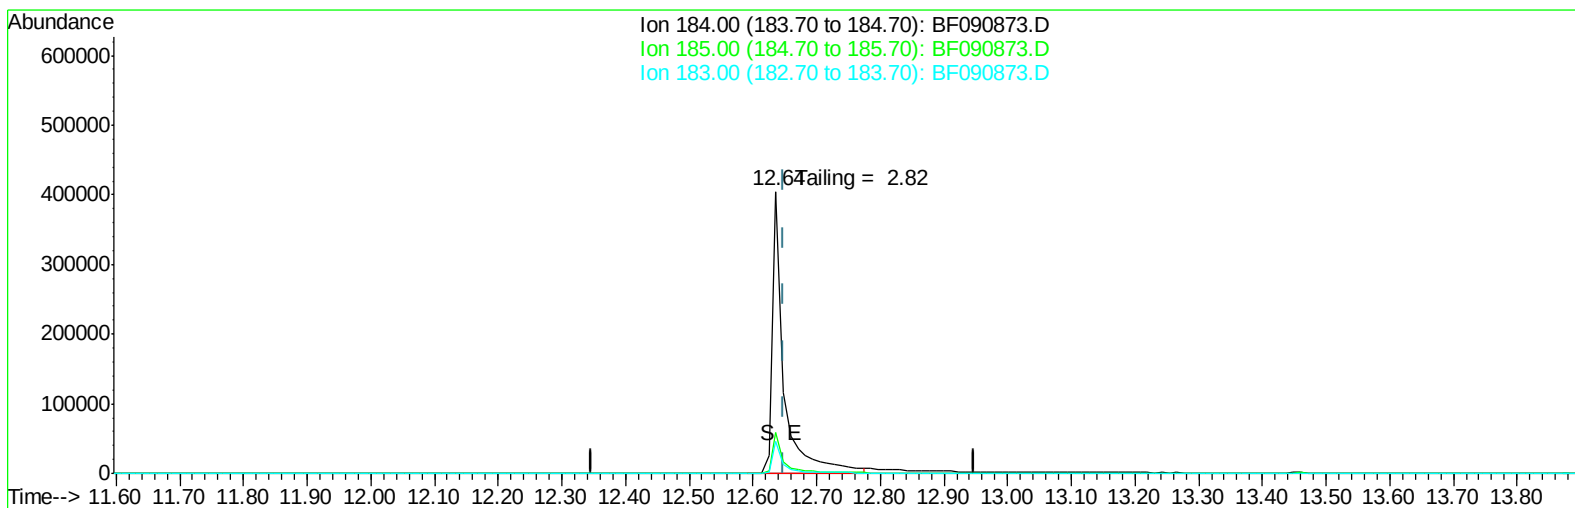

TIC: BF090873.D

(76) Benzidine

12.637min (-0.011) 0.00ng

response 553677

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.51
183.00	9.50	11.44#
0.00	0.00	0.00