

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102716\
 Data File : BF090881.D
 Acq On : 27 Oct 2016 21:58
 Operator : UM/SJ
 Sample : H5423-19
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-10 COMP(0-16FEET)

Quant Time: Oct 28 01:34:30 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 27 18:46:43 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.77	152	135630	20.00	ng	0.00
21) Naphthalene-d8	8.05	136	558364	20.00	ng	-0.01
38) Acenaphthene-d10	9.81	164	325530	20.00	ng	-0.01
63) Phenanthrene-d10	11.30	188	539695	20.00	ng	-0.01
75) Chrysene-d12	13.93	240	476082	20.00	ng	-0.02
86) Perylene-d12	15.33	264	343724	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	1044066	134.59	ng	0.00
7) Phenol-d6	6.41	99	1417007	135.40	ng	-0.01
23) Nitrobenzene-d5	7.33	82	788111	92.40	ng	-0.02
41) 2,4,6-Tribromophenol	10.60	330	396240	118.44	ng	-0.01
44) 2-Fluorobiphenyl	9.14	172	1547484	83.47	ng	-0.01
78) Terphenyl-d14	12.89	244	1787923	94.62	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.54	163	307925	14.16	ng	Qvalue # 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102716\
Data File : BF090881.D
Acq On : 27 Oct 2016 21:58
Operator : UM/SJ
Sample : H5423-19
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10 COMP(0-16FEET)

Quant Time: Oct 28 01:34:30 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 27 18:46:43 2016
Response via : Initial Calibration

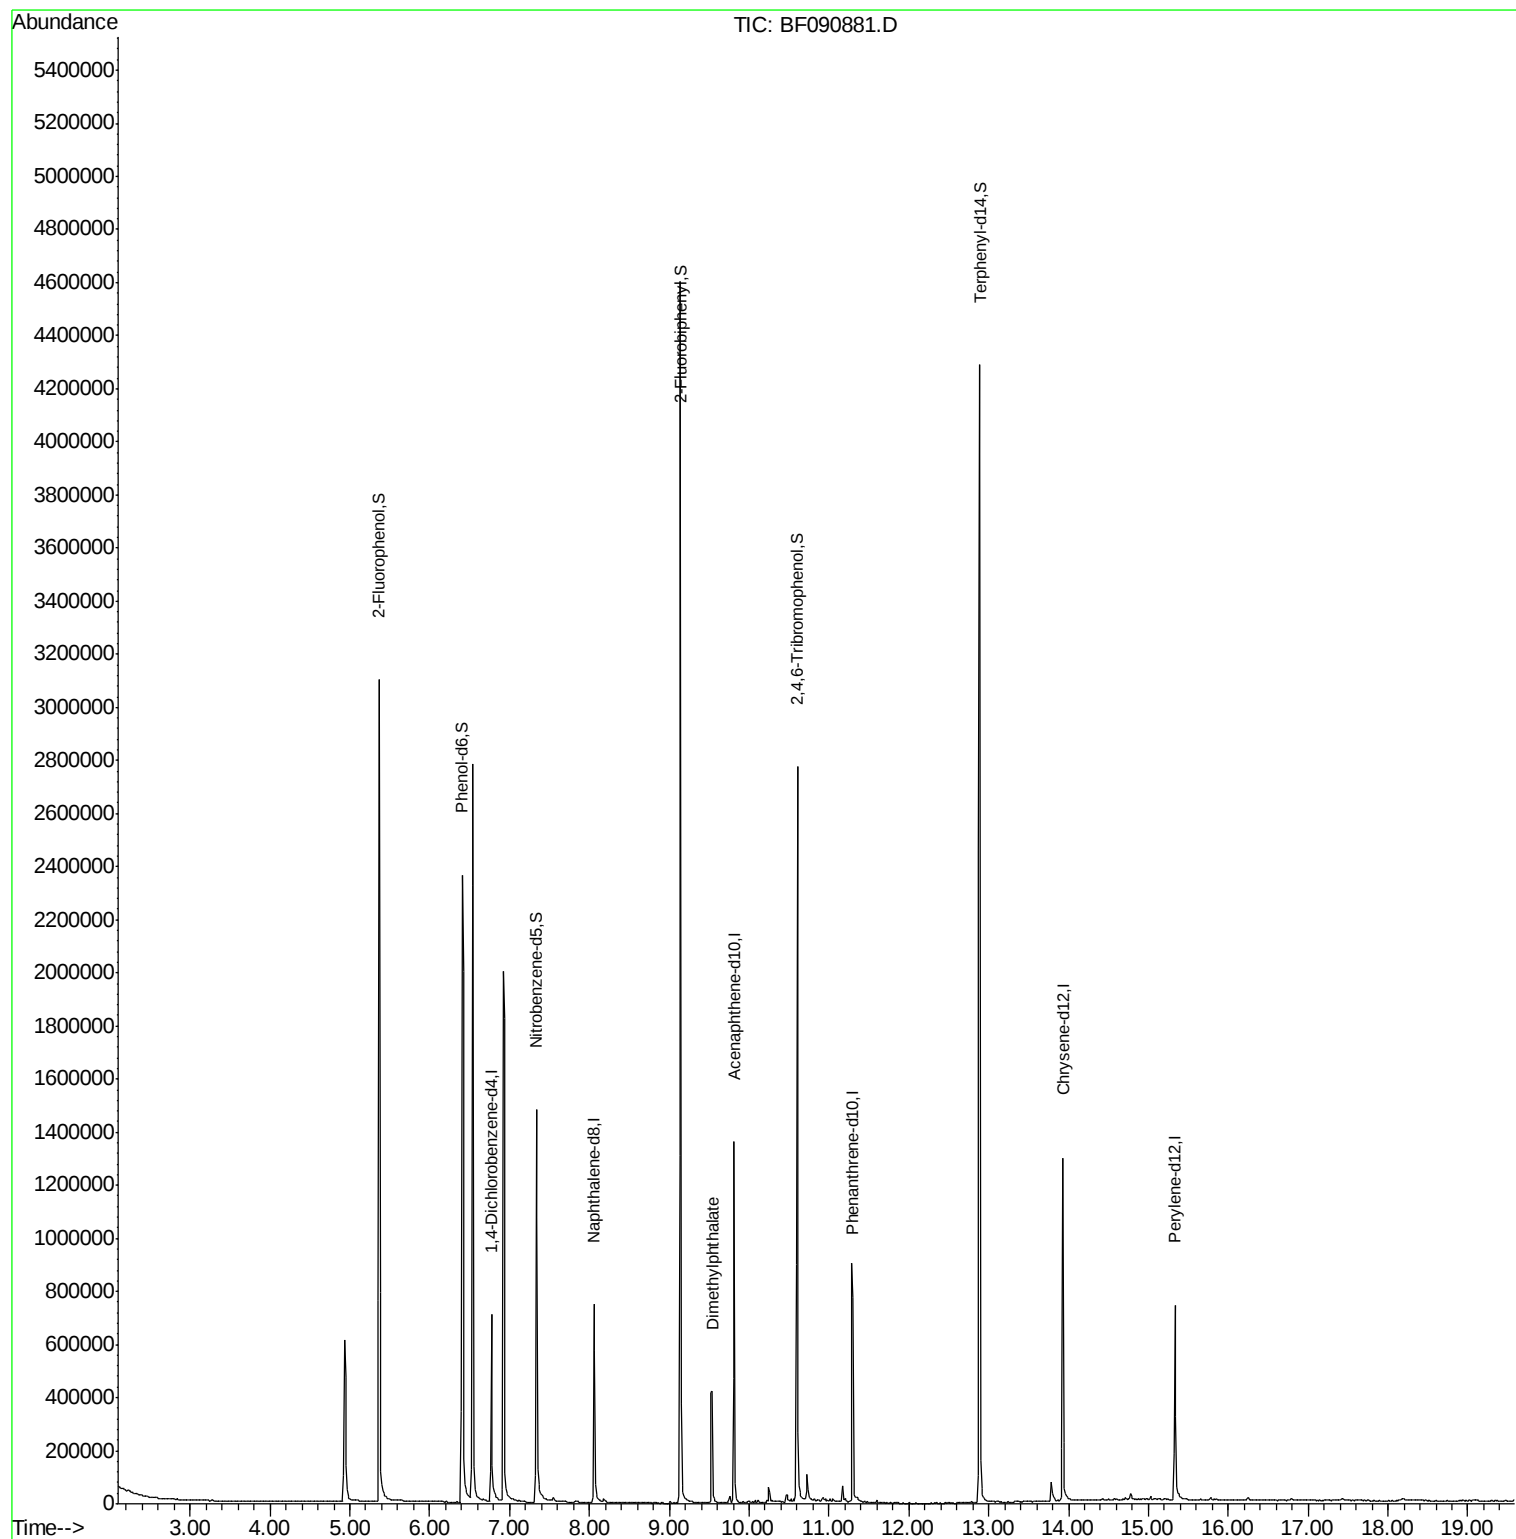







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.77 min Scan# 410
 Delta R.T. 0.00 min
 Lab File: BF090881.D
 Acq: 27 Oct 2016 21:58

Instrument :
 BNA_F
 ClientSampleId :
 SB-10 COMP(0-16FEET)

Tot Ion:152 Resp: 135630
 Ion Ratio Lower Upper
 152 100
 150 158.4 124.7 187.1
 115 57.8 39.0 58.4

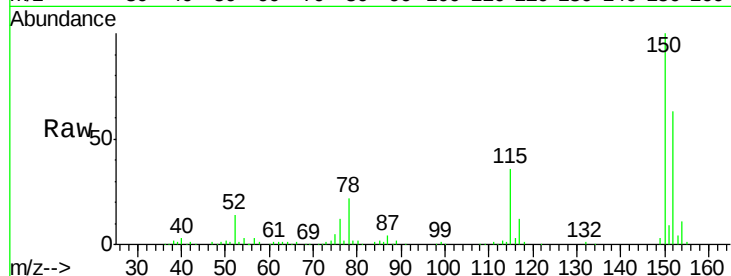


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

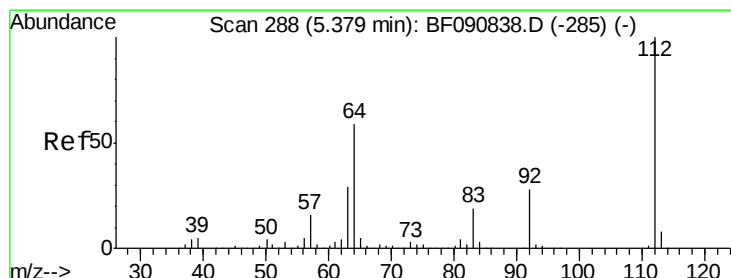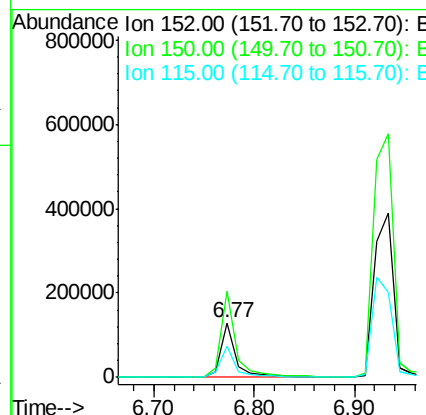
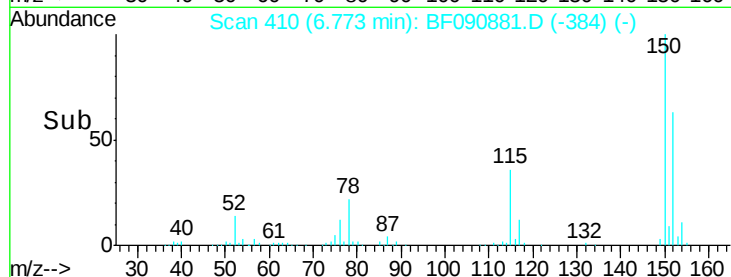



#5
 2-Fluorophenol
 Concen: 134.59 ng
 RT: 5.37 min Scan# 287
 Delta R.T. 0.00 min
 Lab File: BF090881.D
 Acq: 27 Oct 2016 21:58

Tgt Ion:112 Resp: 1044066
 Ion Ratio Lower Upper
 112 100
 64 61.5 39.7 59.5#
 63 30.4 17.4 26.0#

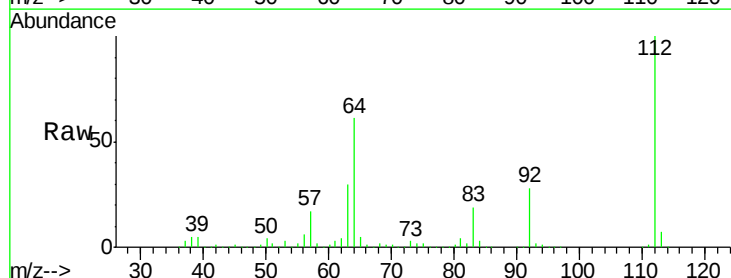

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

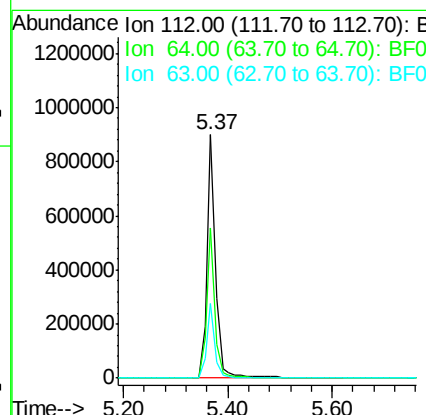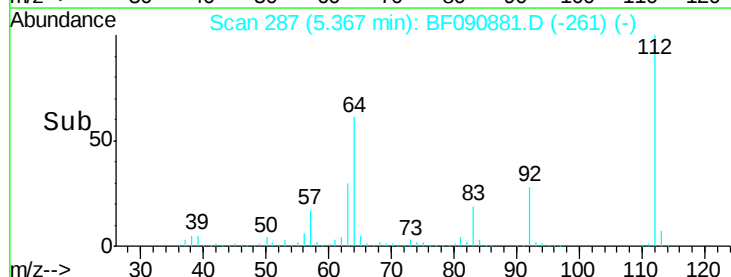

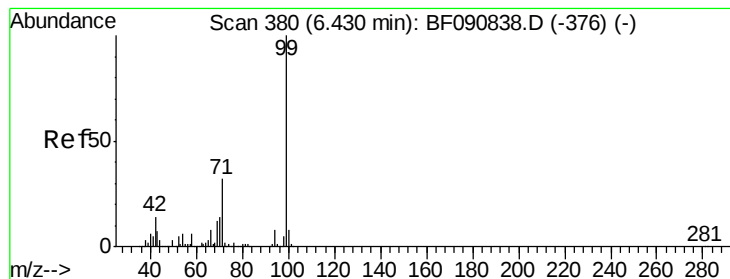

#7

Phenol-d6

Concen: 135.40 ng

RT: 6.41 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF090881.D

Acq: 27 Oct 2016 21:58

Instrument :

BNA_F

ClientSampleId :

SB-10 COMP(0-16FEET)





Tot Ion: 99 Resp: 1417007

Ion Ratio Lower Upper

99 100

42 15.1 13.7 20.5

71 32.2 14.2 21.2#

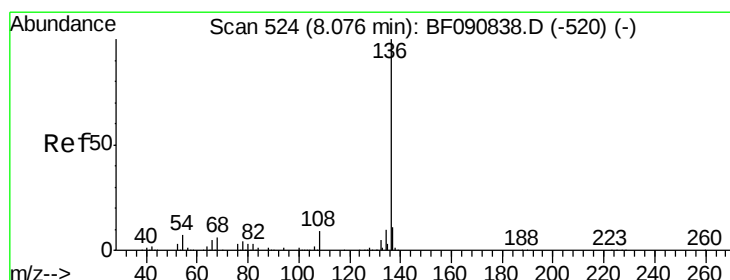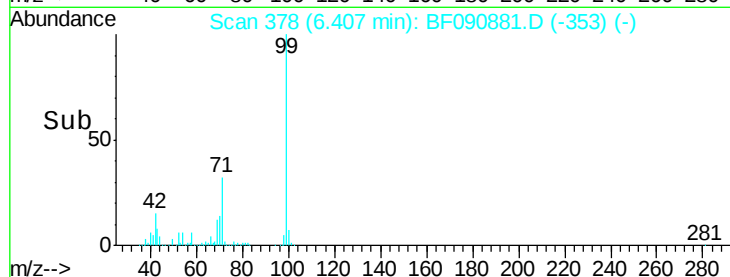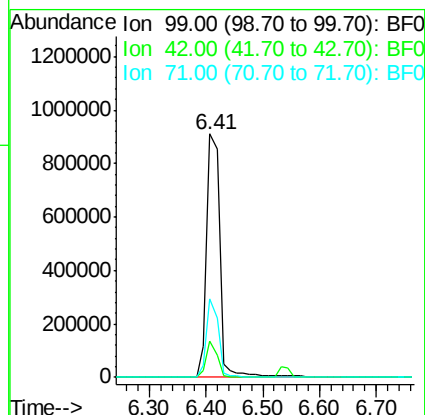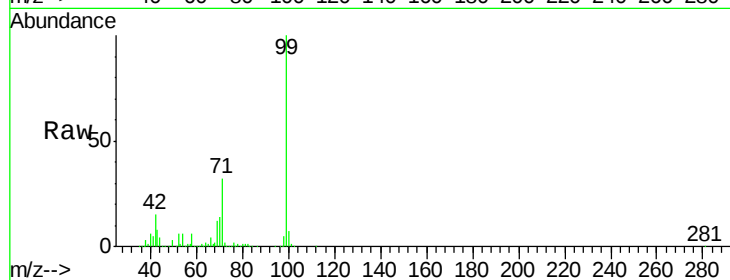

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.05 min Scan# 522

Delta R.T. -0.01 min

Lab File: BF090881.D

Acq: 27 Oct 2016 21:58

Tgt Ion: 136 Resp: 558364




Ion Ratio Lower Upper


136 100

137 11.2 9.0 13.6

54 8.0 8.2 12.2#

68 7.5 5.8 8.6

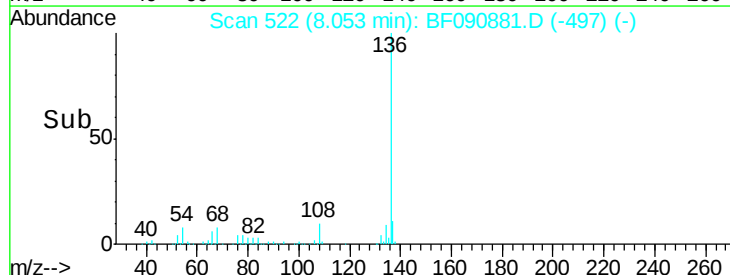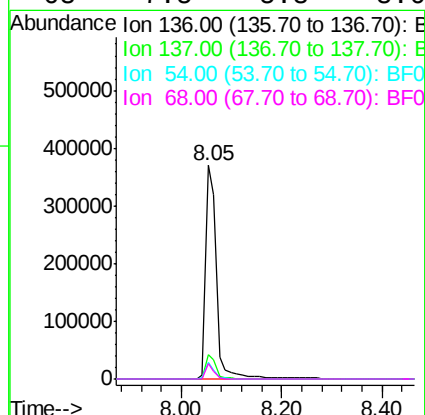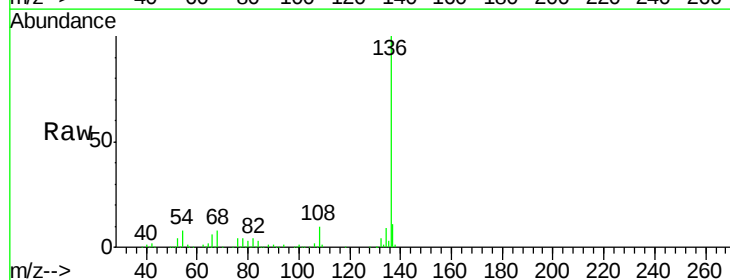


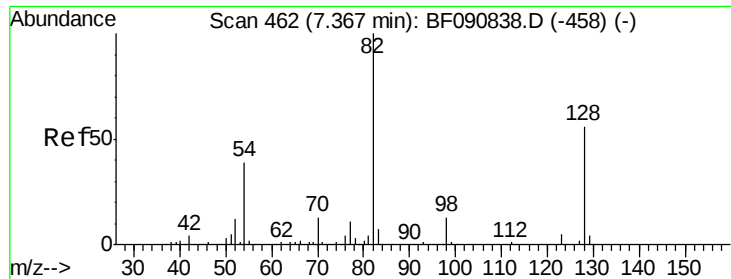




#23
Nitrobenzene-d5
Concen: 92.40 ng
RT: 7.33 min Scan# 459
Delta R.T. -0.02 min
Lab File: BF090881.D
Acq: 27 Oct 2016 21:58

Instrument :
BNA_F
ClientSampleId :
SB-10 COMP(0-16FEET)

Tot Ion: 82 Resp: 788111
Ion Ratio Lower Upper
82 100
128 42.6 51.0 76.6#
54 45.5 47.5 71.3#

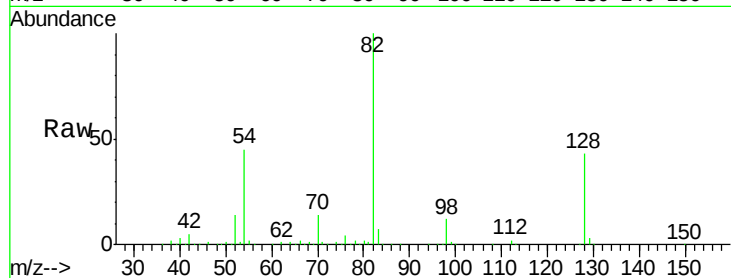


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

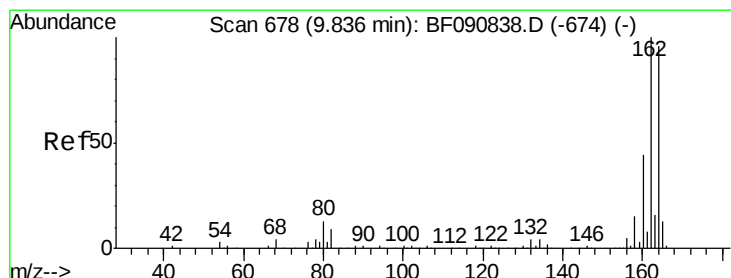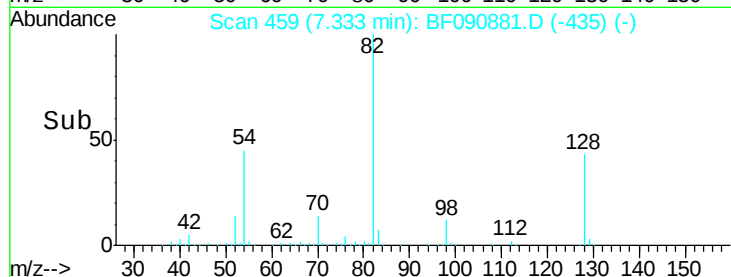
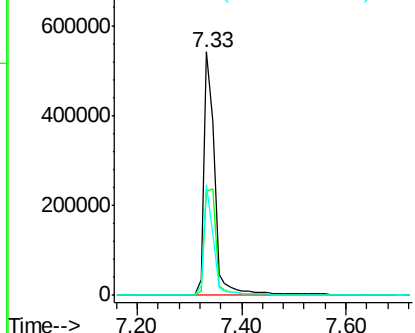



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.81 min Scan# 676
Delta R.T. -0.01 min
Lab File: BF090881.D
Acq: 27 Oct 2016 21:58

Tgt Ion:164 Resp: 325530
Ion Ratio Lower Upper
164 100
162 104.9 75.2 112.8
160 45.4 31.5 47.3

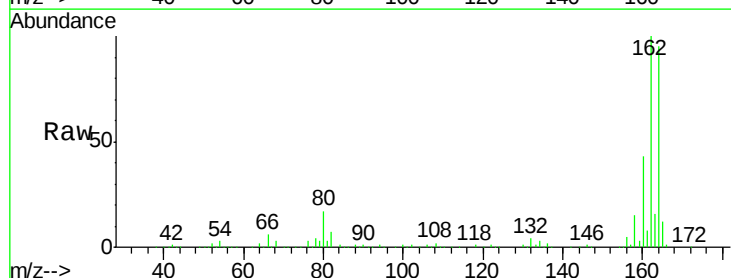

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

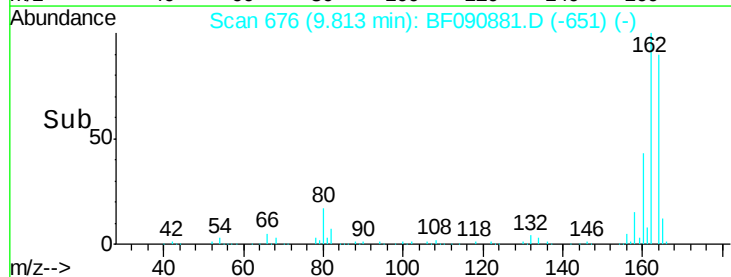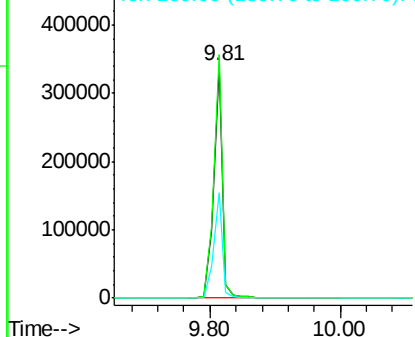


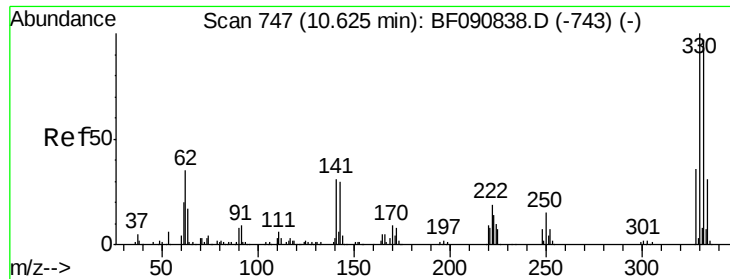




#41
 2,4,6-Tribromophenol
 Concen: 118.44 ng
 RT: 10.60 min Scan# 745
 Delta R.T. -0.01 min
 Lab File: BF090881.D
 Acq: 27 Oct 2016 21:58

Instrument :
 BNA_F
 ClientSampleId :
 SB-10 COMP(0-16FEET)

Tot Ion:330 Resp: 396240
 Ion Ratio Lower Upper
 330 100
 332 95.6 76.6 114.8
 141 32.3 29.7 44.5

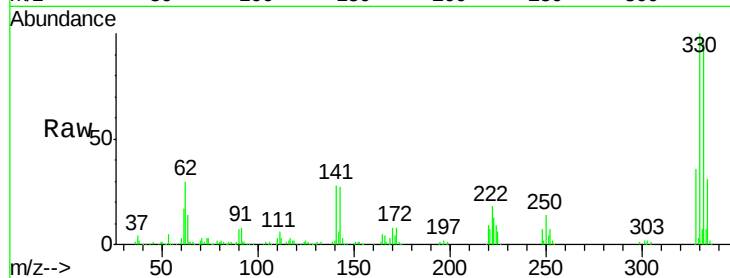


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

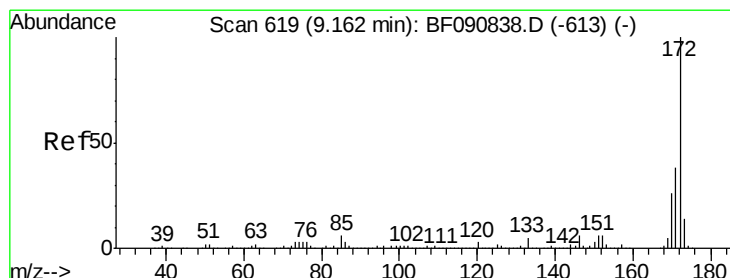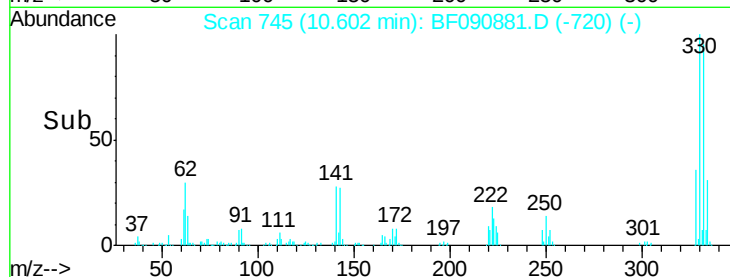
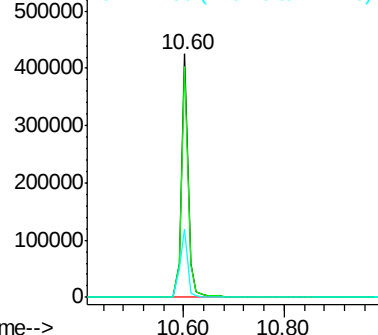



#44
 2-Fluorobiphenyl
 Concen: 83.47 ng
 RT: 9.14 min Scan# 617
 Delta R.T. -0.01 min
 Lab File: BF090881.D
 Acq: 27 Oct 2016 21:58

Tgt Ion:172 Resp: 1547484
 Ion Ratio Lower Upper
 172 100
 171 37.6 26.1 39.1
 170 25.1 17.4 26.2

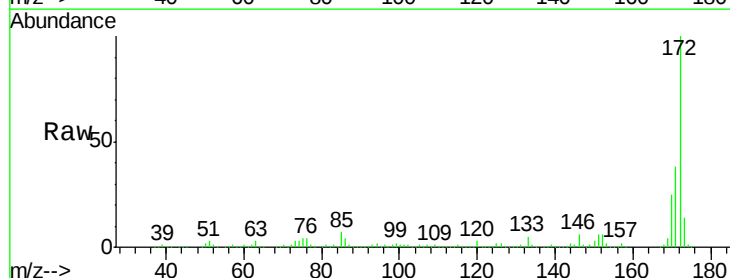

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

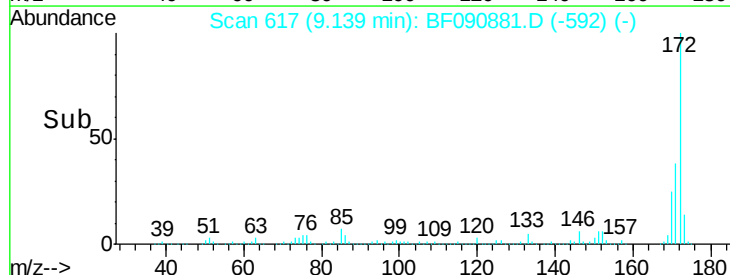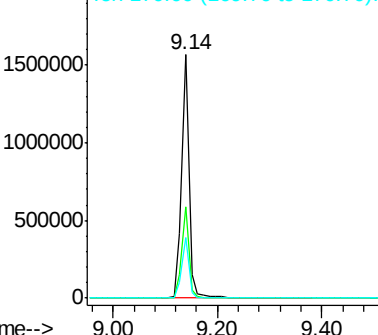

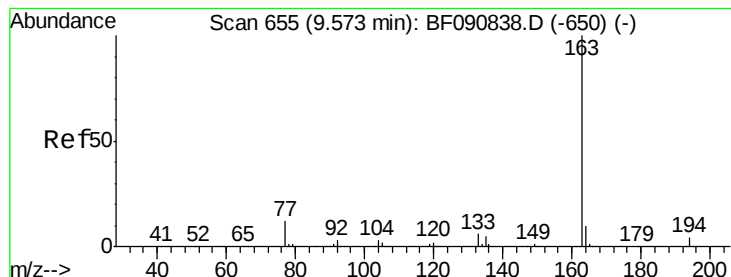

#49

Dimethylphthalate

Concen: 14.16 ng

RT: 9.54 min Scan# 652

Delta R.T. -0.02 min

Lab File: BF090881.D

Acq: 27 Oct 2016 21:58

Instrument :

BNA_F

ClientSampleId :

SB-10 COMP(0-16FEET)


Tot Ion:163 Resp: 307925

Ion Ratio Lower Upper

163 100

194 3.8 4.4 6.6#




164 9.5 8.3 12.5

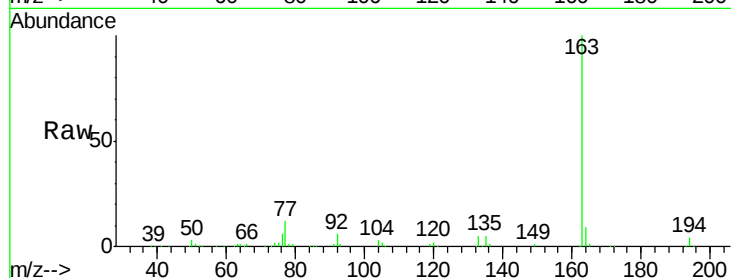

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

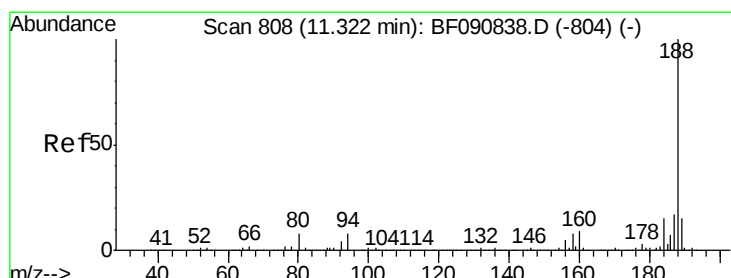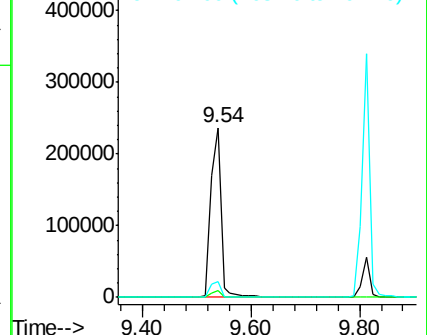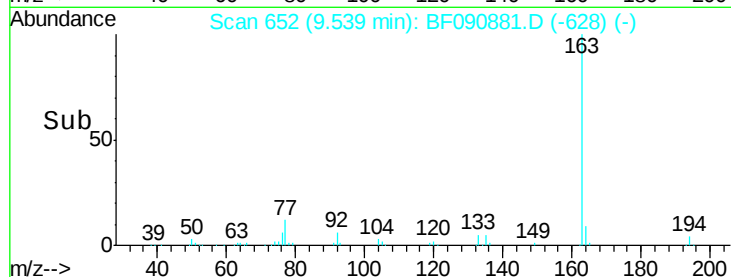

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.30 min Scan# 806

Delta R.T. -0.01 min

Lab File: BF090881.D

Acq: 27 Oct 2016 21:58


Tgt Ion:188 Resp: 539695

Ion Ratio Lower Upper

188 100

94 6.2 11.1 16.7#



80 6.7 11.0 16.4#

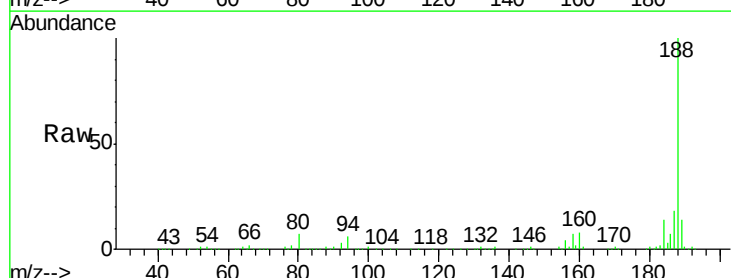


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

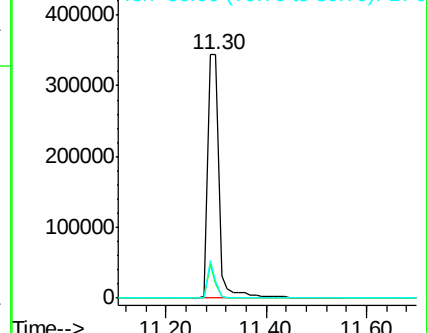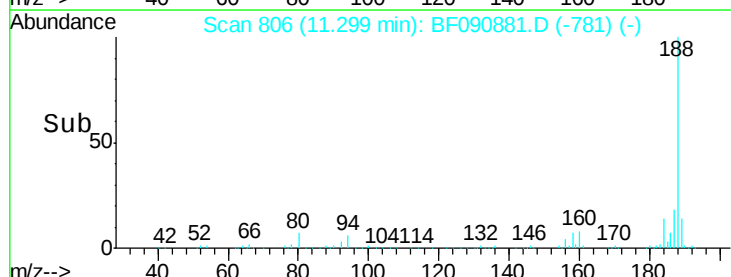

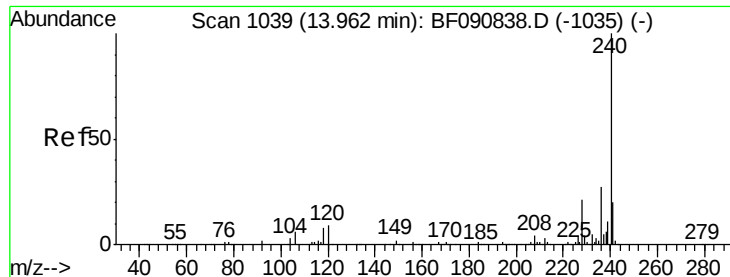

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.93 min Scan# 1036

Delta R.T. -0.02 min

Lab File: BF090881.D

Acq: 27 Oct 2016 21:58

Instrument :

BNA_F

ClientSampleId :

SB-10 COMP(0-16FEET)


Tot Ion:240 Resp: 476082

Ion Ratio Lower Upper

240 100

120 12.1 16.2 24.2#




236 26.7 18.4 27.6

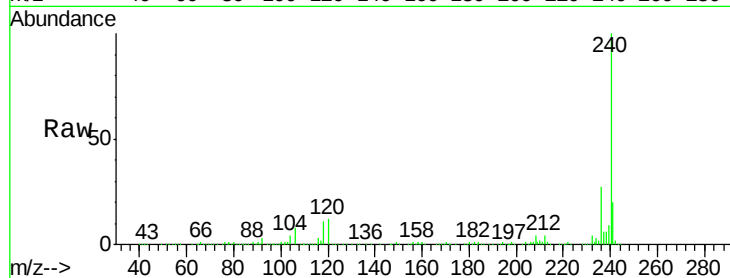

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

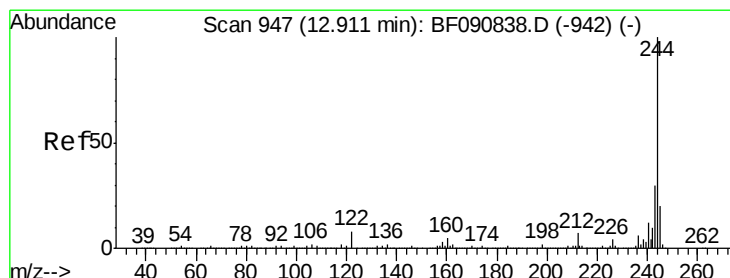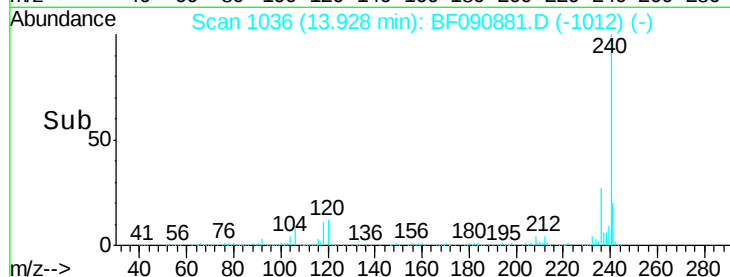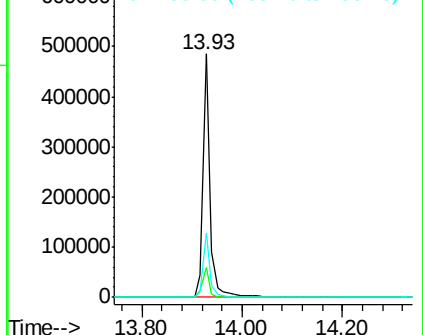

#78

Terphenyl-d14

Concen: 94.62 ng

RT: 12.89 min Scan# 945

Delta R.T. -0.01 min

Lab File: BF090881.D

Acq: 27 Oct 2016 21:58


Tgt Ion:244 Resp: 1787923

Ion Ratio Lower Upper

244 100

212 6.6 4.3 6.5#



122 7.6 17.4 26.2#



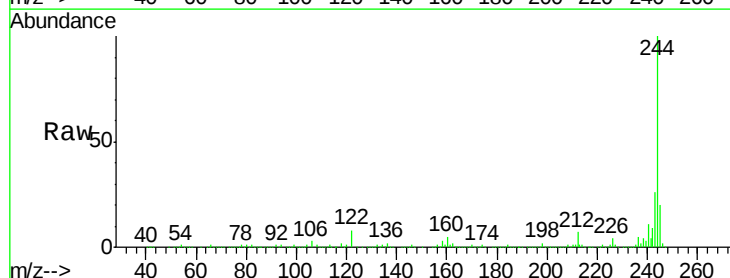


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

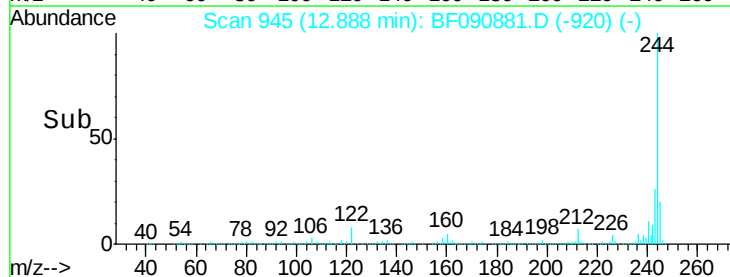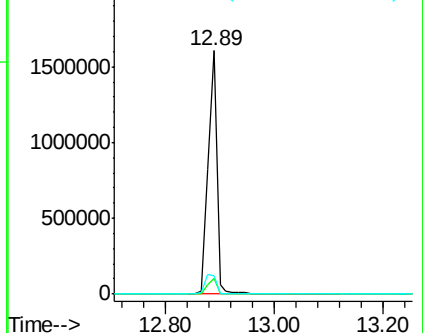

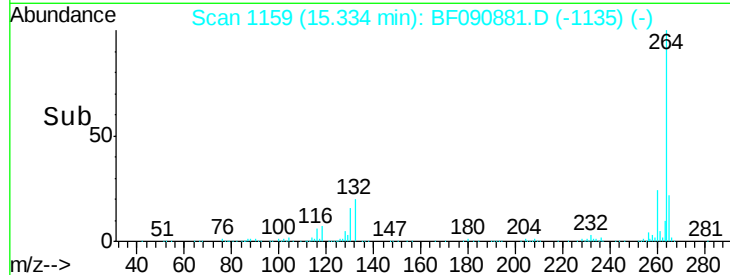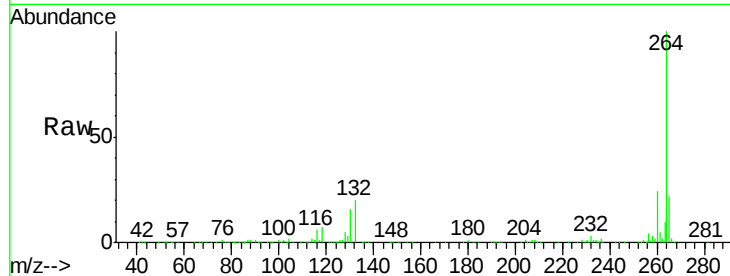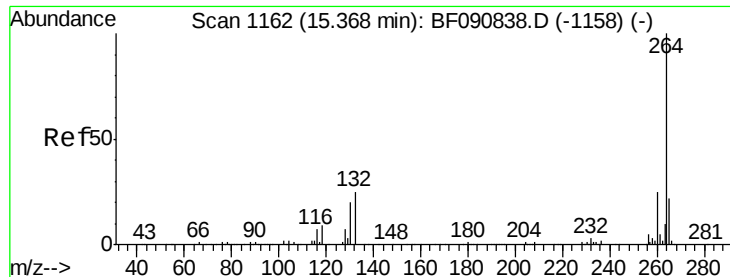

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.33 min Scan# 1159
Delta R.T. -0.02 min
Lab File: BF090881.D
Acq: 27 Oct 2016 21:58

Instrument :
BNA_F
ClientSampleId :
SB-10 COMP(0-16FEET)

Tot Ion:264 Resp: 343724
Ion Ratio Lower Upper
264 100
260 24.2 16.7 25.1
265 21.6 17.2 25.8

