

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
 Data File : BF090869.D
 Acq On : 27 Oct 2016 12:58
 Operator : UM/SJ
 Sample : H5308-25 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-104S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.007	342	343	347	rVB2	20250	32960	1.56%	0.224%
2	6.099	350	351	358	rVB6	8257	23922	1.14%	0.163%
3	6.202	358	360	364	rBV3	17298	31676	1.50%	0.215%
4	6.293	367	368	373	rVB3	16610	27822	1.32%	0.189%
5	6.442	378	381	382	rVV2	16948	28484	1.35%	0.194%
6	6.545	385	390	394	rBV4	24813	67339	3.20%	0.458%
7	6.636	394	398	399	rBV4	11849	21810	1.04%	0.148%
8	6.773	408	410	414	rBV	963971	929102	44.11%	6.314%
9	6.933	422	424	425	rVB2	29016	29121	1.38%	0.198%
10	7.059	432	435	437	rBV	35250	53888	2.56%	0.366%
11	7.219	446	449	450	rBV3	19735	39466	1.87%	0.268%
12	7.310	454	457	459	rVV3	28825	67028	3.18%	0.456%
13	7.379	459	463	465	rVV4	20627	56137	2.67%	0.382%
14	7.425	465	467	469	rVV	46288	69082	3.28%	0.469%
15	7.505	469	474	476	rVV5	19458	57845	2.75%	0.393%
16	7.539	476	477	479	rVV2	25468	44399	2.11%	0.302%
17	7.585	479	481	483	rVB2	65639	74996	3.56%	0.510%
18	7.699	490	491	494	rVB3	37676	36632	1.74%	0.249%
19	7.813	500	501	503	rBV2	18088	25257	1.20%	0.172%
20	7.893	505	508	510	rVB3	25702	45268	2.15%	0.308%
21	7.950	510	513	516	rBV4	21959	47816	2.27%	0.325%
22	8.019	516	519	520	rBV2	16074	31346	1.49%	0.213%
23	8.065	520	523	525	rBV	1654470	1624341	77.12%	11.039%
24	8.133	528	529	530	rVB	66478	46963	2.23%	0.319%
25	8.236	535	538	539	rBV	26134	44800	2.13%	0.304%
26	8.270	539	541	543	rVB2	38434	34961	1.66%	0.238%
27	8.362	547	549	550	rBV2	24319	28254	1.34%	0.192%
28	8.419	552	554	556	rBV2	82240	77685	3.69%	0.528%
29	8.499	558	561	566	rBV3	54724	125562	5.96%	0.853%
30	8.613	568	571	573	rBV3	26852	56349	2.68%	0.383%
31	8.682	575	577	578	rBV2	18728	30409	1.44%	0.207%
32	8.762	582	584	585	rVB	50715	64941	3.08%	0.441%
33	8.819	587	589	590	rBV2	14869	26081	1.24%	0.177%
34	8.888	592	595	599	rVB3	46285	97696	4.64%	0.664%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
 Data File : BF090869.D
 Acq On : 27 Oct 2016 12:58
 Operator : UM/SJ
 Sample : H5308-25 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-104S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.945	599	600	601 rBV	23839	23703	1.13%	0.161%
36	8.979	601	603	605 rBV3	18918	34809	1.65%	0.237%
37	9.093	611	613	616 rBV4	80778	111821	5.31%	0.760%
38	9.219	622	624	627 rVB4	50396	78927	3.75%	0.536%
39	9.276	627	629	633 rVB5	37741	89826	4.26%	0.610%
40	9.345	633	635	637 rBV2	60934	61799	2.93%	0.420%
41	9.413	637	641	643 rBV3	40018	69386	3.29%	0.472%
42	9.482	644	647	648 rVV3	42231	58899	2.80%	0.400%
43	9.551	650	653	654 rVB2	89442	114536	5.44%	0.778%
44	9.688	663	665	667 rBV3	31952	73667	3.50%	0.501%
45	9.733	667	669	671 rVV	113455	146428	6.95%	0.995%
46	9.813	674	676	678 rVV	1940618	1912111	90.79%	12.995%
47	9.848	678	679	681 rVV2	63148	85638	4.07%	0.582%
48	9.928	684	686	688 rVB	59438	79018	3.75%	0.537%
49	9.973	688	690	691 rBV2	23125	37768	1.79%	0.257%
50	10.019	692	694	696 rVV2	67378	74475	3.54%	0.506%
51	10.065	696	698	699 rVV	21299	27524	1.31%	0.187%
52	10.133	702	704	706 rBV	66357	94315	4.48%	0.641%
53	10.225	710	712	715 rVB4	57374	99977	4.75%	0.679%
54	10.305	715	719	722 rBV5	37207	109082	5.18%	0.741%
55	10.362	722	724	725 rBV2	21381	23496	1.12%	0.160%
56	10.476	733	734	736 rVB	74352	70713	3.36%	0.481%
57	10.522	736	738	740 rVB3	26549	42450	2.02%	0.288%
58	10.591	740	744	747 rBV6	48335	112655	5.35%	0.766%
59	10.705	752	754	755 rBV2	20301	30714	1.46%	0.209%
60	10.739	755	757	760 rBV2	93311	130110	6.18%	0.884%
61	10.796	760	762	763 rBV	67967	92063	4.37%	0.626%
62	10.831	763	765	766 rVB2	48322	61705	2.93%	0.419%
63	10.865	766	768	771 rBV3	33025	71508	3.40%	0.486%
64	11.002	779	780	783 rVB	23597	21528	1.02%	0.146%
65	11.208	795	798	801 rVB3	83741	125898	5.98%	0.856%
66	11.299	804	806	812 rBV	2074238	1991404	94.55%	13.533%
67	11.802	848	850	851 rBV2	39143	60090	2.85%	0.408%
68	11.905	857	859	865 rVB6	48169	134473	6.38%	0.914%
69	12.351	896	898	900 rBV2	41203	62778	2.98%	0.427%
70	12.511	910	912	914 rBV	57556	73117	3.47%	0.497%
71	12.739	930	932	934 rBV	66294	82324	3.91%	0.559%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102716\
Data File : BF090869.D
Acq On : 27 Oct 2016 12:58
Operator : UM/SJ
Sample : H5308-25 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104S

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.888	943	945	949	rBV	81000	154814	7.35%	1.052%
73	13.562	1003	1004	1006	rVB	94420	101660	4.83%	0.691%
74	13.940	1034	1037	1039	rBV	1983441	2106171	100.00%	14.313%
75	14.477	1083	1084	1086	rVB	95677	81407	3.87%	0.553%
76	15.345	1158	1160	1163	rBV	976087	1415352	67.20%	9.619%
77	15.997	1215	1217	1226	rVB3	42295	115111	5.47%	0.782%
78	16.397	1250	1252	1258	rVB4	32075	69960	3.32%	0.475%


Sum of corrected areas: 14714648

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data File : BF090869.D
Acq On : 27 Oct 2016 12:58
Operator : UM/SJ
Sample : H5308-25 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-104S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

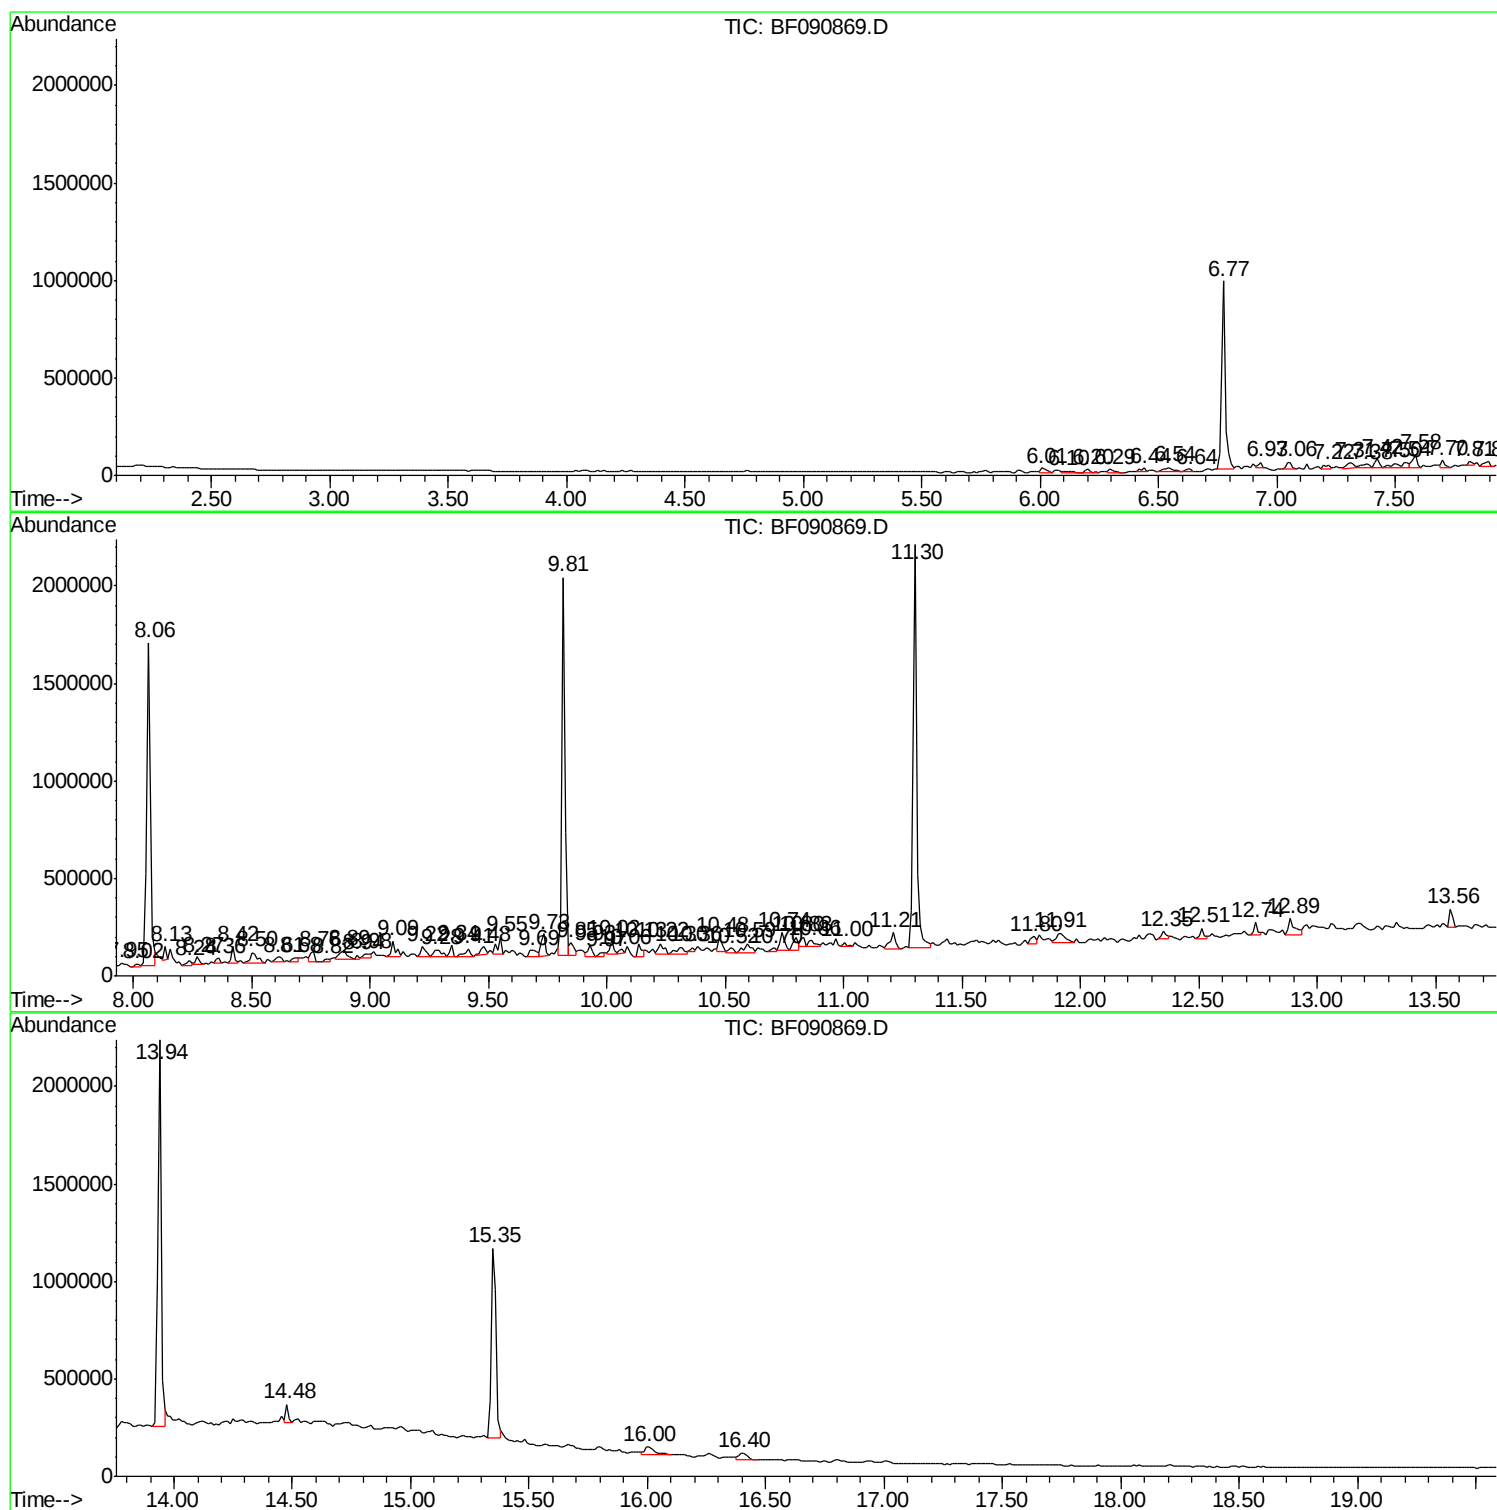

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data_File : BF090869.D
Acq_On : 27 Oct 2016 12:588
Operator : UM/SJJ
Sample : H5308-25-10XX
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
MW-104S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
