

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102716\
 Data File : BF090870.D
 Acq On : 27 Oct 2016 13:25
 Operator : UM/SJ
 Sample : PB94264BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94264BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.921	246	248	253	rBV	66271	74583	5.79%	0.752%
2	5.367	285	287	304	rBV	167902	319829	24.83%	3.227%
3	6.407	376	378	388	rBV	262148	348339	27.05%	3.514%
4	6.533	388	389	397	rVV	263624	395078	30.68%	3.986%
5	6.773	408	410	421	rBV	774145	793787	61.63%	8.008%
6	6.933	421	424	426	rBV	283763	337456	26.20%	3.404%
7	7.345	457	460	469	rBV	116051	216148	16.78%	2.181%
8	8.065	520	523	525	rBV	988504	960198	74.55%	9.687%
9	9.139	615	617	628	rVB	612519	565879	43.94%	5.709%
10	9.722	663	668	674	rBV	21322	48125	3.74%	0.486%
11	9.813	674	676	679	rBV	1319950	1216316	94.44%	12.271%
12	10.602	743	745	755	rVB	275363	275385	21.38%	2.778%
13	11.299	803	806	808	rBV	1467691	1287945	100.00%	12.993%
14	12.888	942	945	947	rBV	562242	563184	43.73%	5.682%
15	13.939	1034	1037	1039	rBV	1076481	1202683	93.38%	12.133%
16	14.534	1085	1089	1096	rBV8	4511	23233	1.80%	0.234%
17	14.717	1103	1105	1109	rVB	13972	17375	1.35%	0.175%
18	15.037	1130	1133	1136	rVB	19887	27143	2.11%	0.274%
19	15.345	1157	1160	1163	rBV	852476	1016905	78.96%	10.259%
20	15.391	1163	1164	1167	rVB	39577	38936	3.02%	0.393%
21	15.791	1196	1199	1203	rVB	30438	44433	3.45%	0.448%
22	16.260	1237	1240	1246	rVB	26862	51315	3.98%	0.518%
23	16.808	1285	1288	1292	rVB	10097	22182	1.72%	0.224%
24	17.448	1340	1344	1350	rVB2	11910	35841	2.78%	0.362%
25	17.734	1367	1369	1372	rBV4	5018	14895	1.16%	0.150%
26	18.203	1407	1410	1414	rBV5	5959	15264	1.19%	0.154%


Sum of corrected areas: 9912457

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data File : BF090870.D
Acq On : 27 Oct 2016 13:25
Operator : UM/SJ
Sample : PB94264BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94264BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

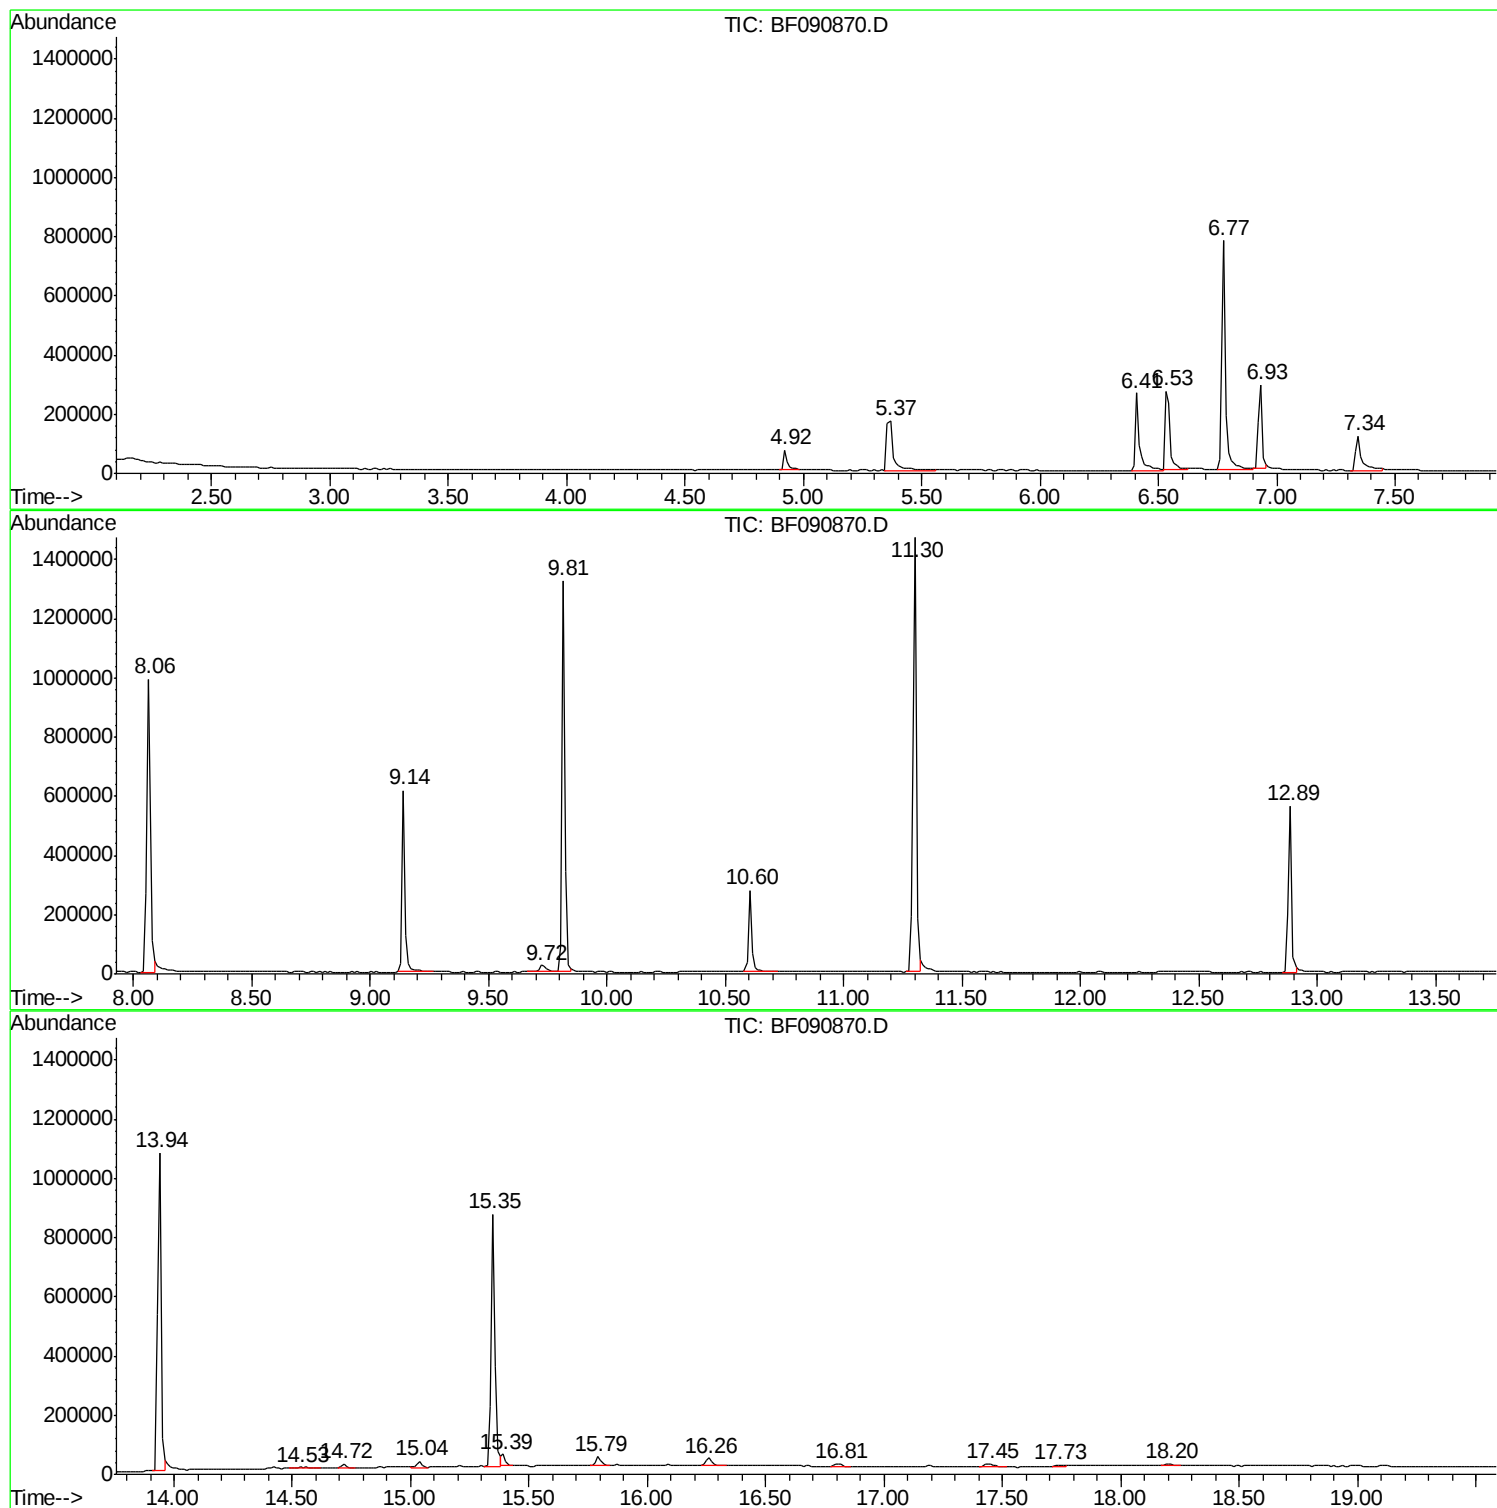

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
Data_File : BF090870.D
Acq_On : 27 Oct 2016 13:255
Operator : UM/SJJ
Sample : PB94264BLL
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB94264BL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
