


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
 Data File : BF090866.D
 Acq On : 27 Oct 2016 11:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 28 15:18:12 2016

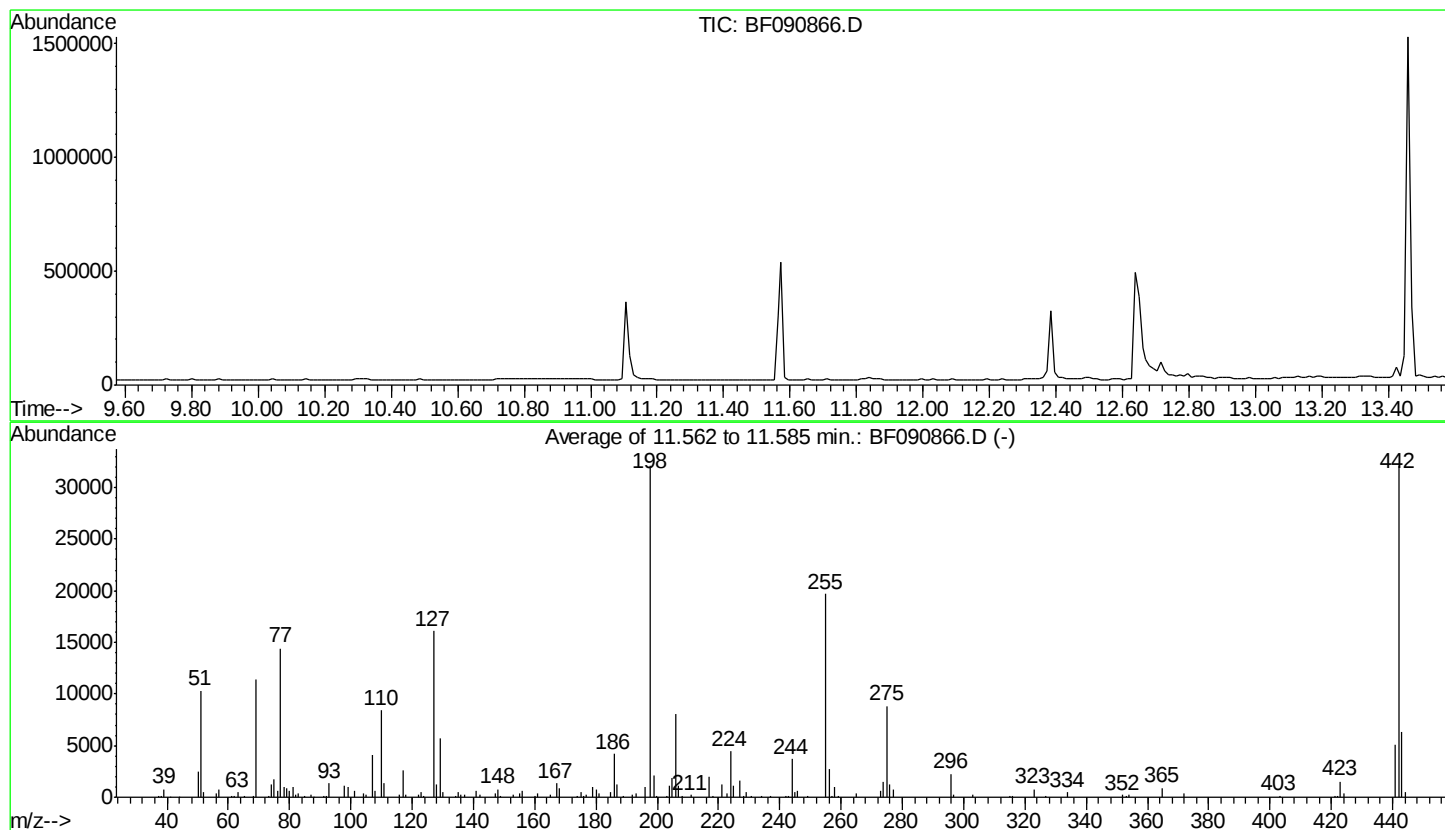

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	10315	PASS
68	69	0.00	2	1.3	146	PASS
69	198	0.00	100	35.5	11396	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	16061	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32112	PASS
199	198	5	9	6.7	2163	PASS
275	198	10	60	27.5	8823	PASS
365	198	1	100	2.8	911	PASS
441	442	0.01	24	15.8	5070	PASS
442	198	50	100	99.9	32067	PASS
443	442	15	24	19.6	6274	PASS