


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102716\
 Data File : BF090873.D
 Acq On : 27 Oct 2016 16:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 28 15:18:12 2016

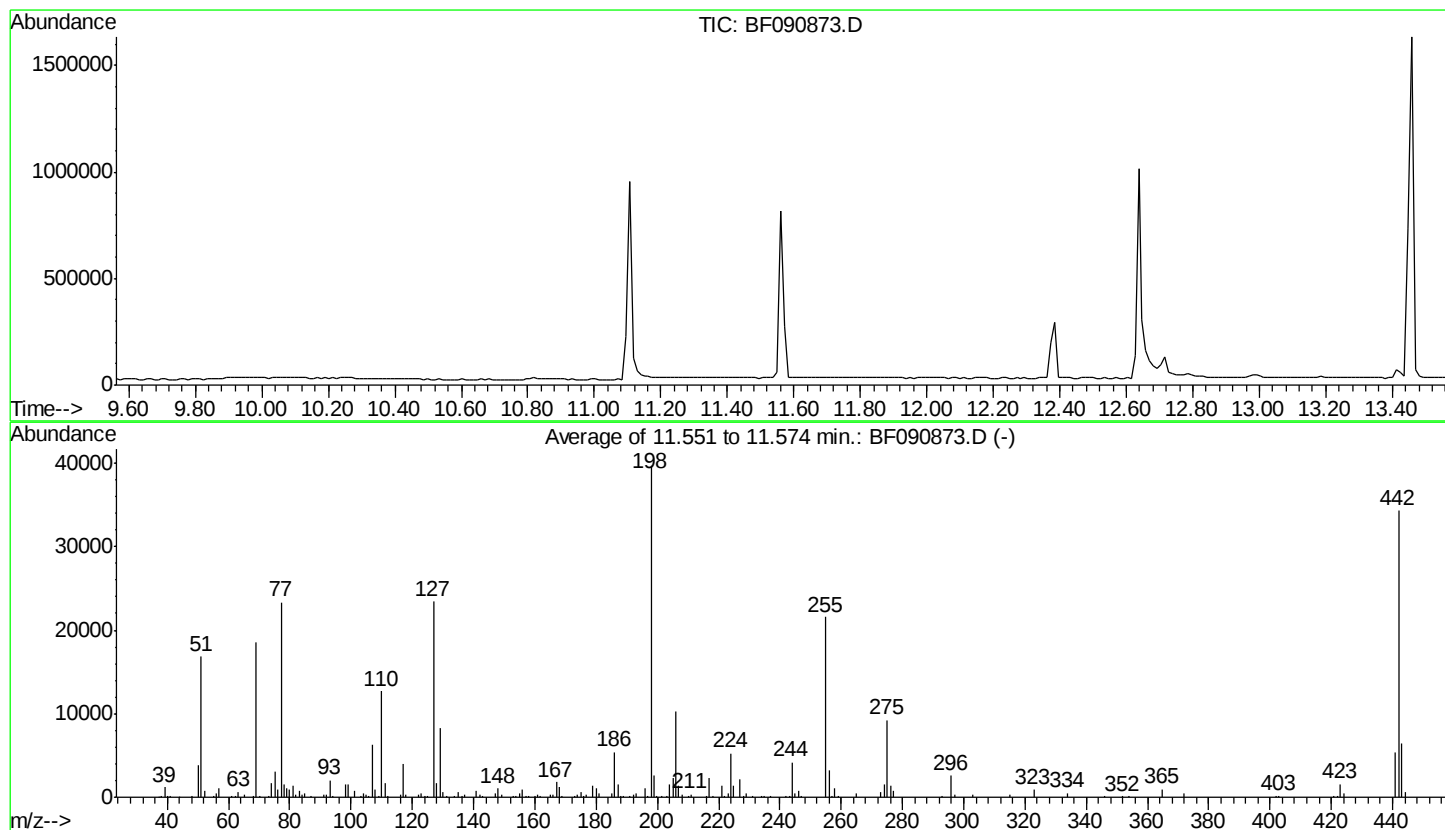

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	16844	PASS
68	69	0.00	2	1.2	231	PASS
69	198	0.00	100	46.8	18575	PASS
70	69	0.00	2	0.6	110	PASS
127	198	10	80	58.9	23399	PASS
197	198	0.00	2	0.3	116	PASS
198	198	100	100	100.0	39703	PASS
199	198	5	9	6.7	2657	PASS
275	198	10	60	23.3	9251	PASS
365	198	1	100	2.5	1000	PASS
441	442	0.01	24	15.5	5313	PASS
442	198	50	100	86.4	34322	PASS
443	442	15	24	18.9	6499	PASS