


Data Path : Z:\HPCHEM1\BNA F\Data\BF102717\
 Data File : BF099874.D
 Acq On : 27 Oct 2017 13:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

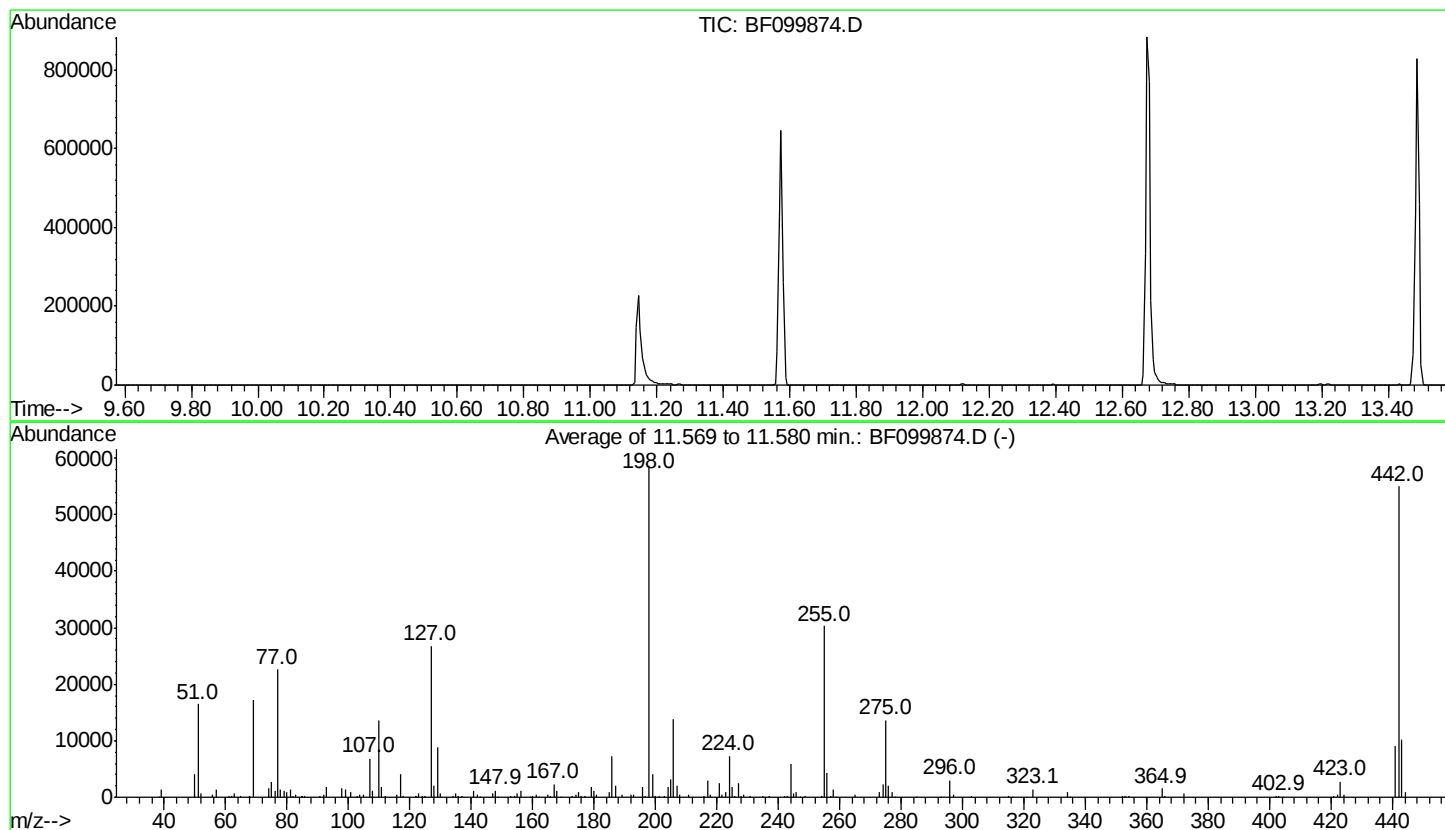

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	16509	PASS
68	69	0.00	2	1.8	304	PASS
69	198	0.00	100	29.2	17116	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	26765	PASS
197	198	0.00	2	0.3	189	PASS
198	198	100	100	100.0	58674	PASS
199	198	5	9	6.9	4048	PASS
275	198	10	60	23.3	13677	PASS
365	198	1	100	2.6	1522	PASS
441	443	0.01	100	87.6	9002	PASS
442	198	50	100	93.7	54984	PASS
443	442	15	24	18.7	10278	PASS