


Data Path : Z:\HPCHEM1\BNA_F\Data\BF102717\
 Data File : BF099885.D
 Acq On : 27 Oct 2017 18:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

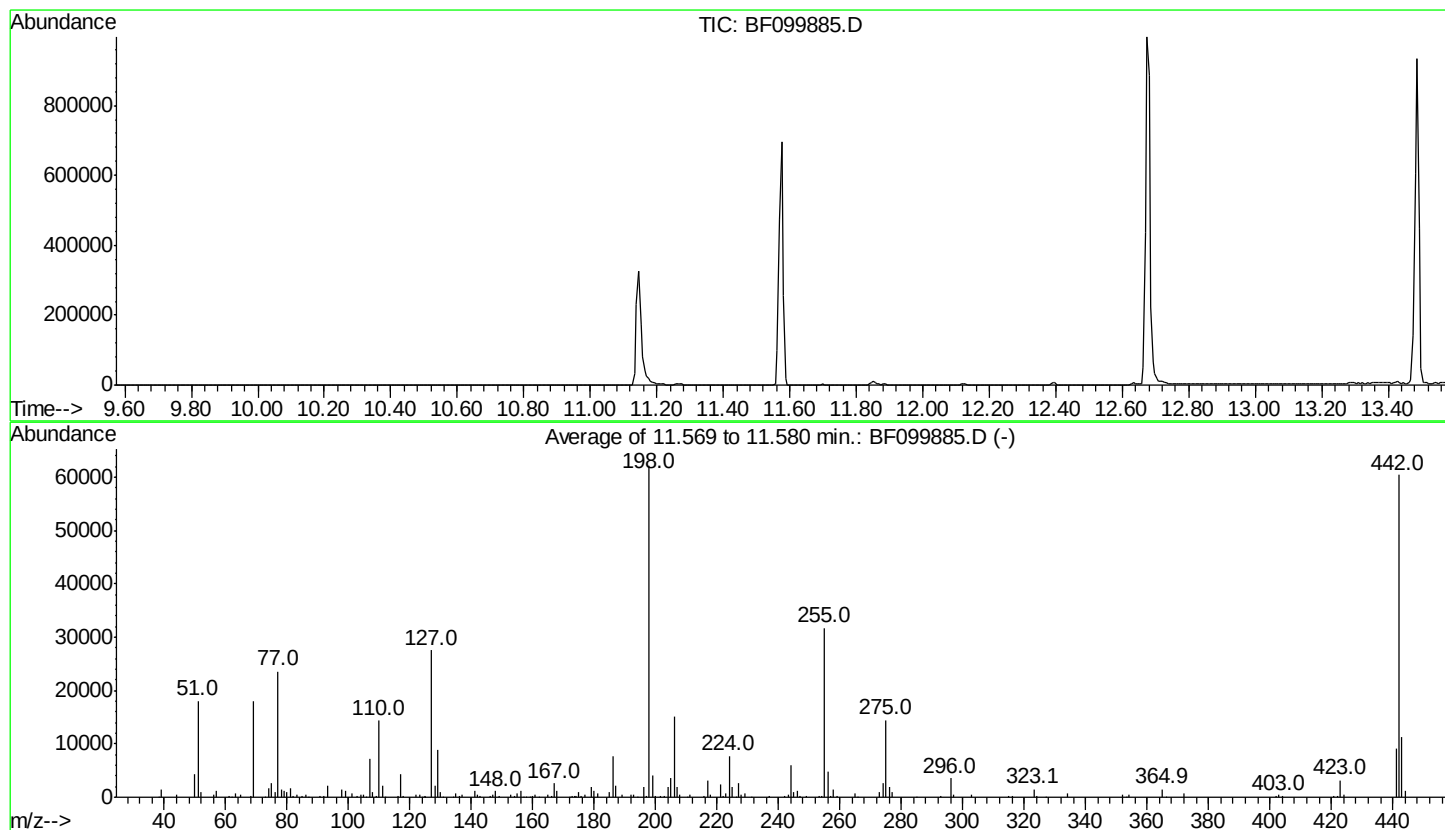

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	18018	PASS
68	69	0.00	2	1.7	311	PASS
69	198	0.00	100	28.8	17923	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.3	27537	PASS
197	198	0.00	2	0.4	261	PASS
198	198	100	100	100.0	62136	PASS
199	198	5	9	6.5	4054	PASS
275	198	10	60	23.3	14451	PASS
365	198	1	100	2.4	1503	PASS
441	443	0.01	100	81.6	9232	PASS
442	198	50	100	97.2	60392	PASS
443	442	15	24	18.7	11320	PASS