
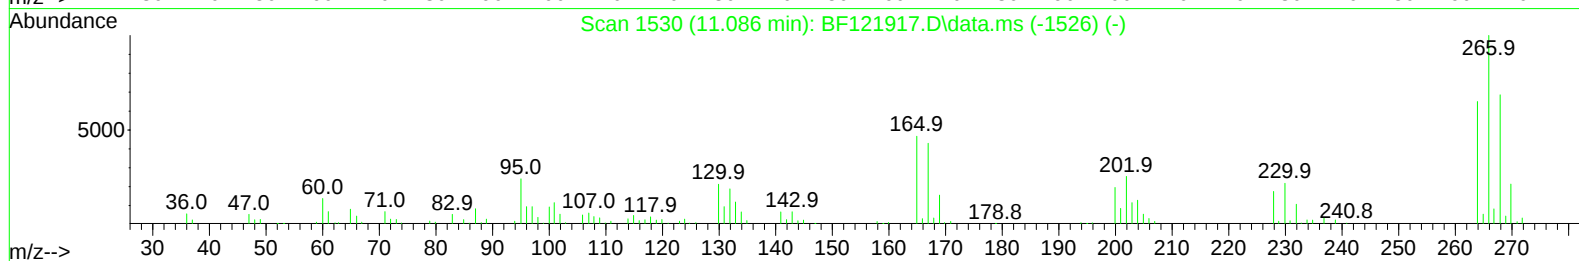
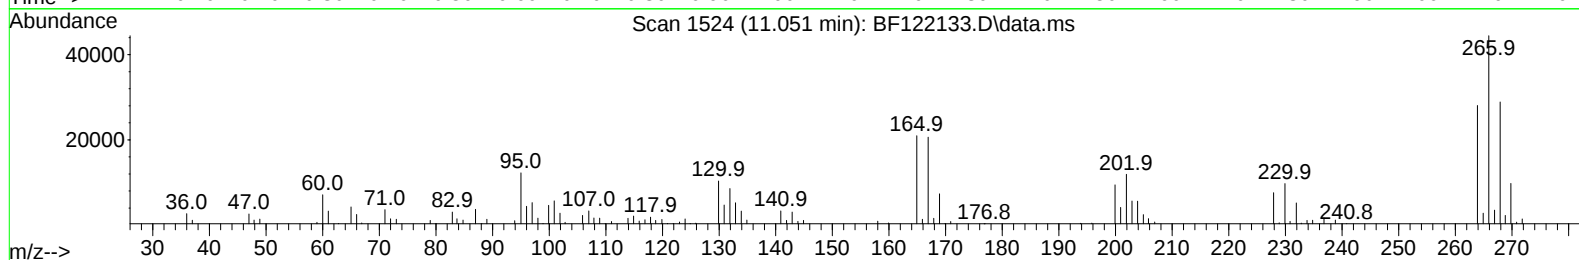


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102720\
Data File : BF122133.D
Acq On : 27 Oct 2020 8:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:51:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

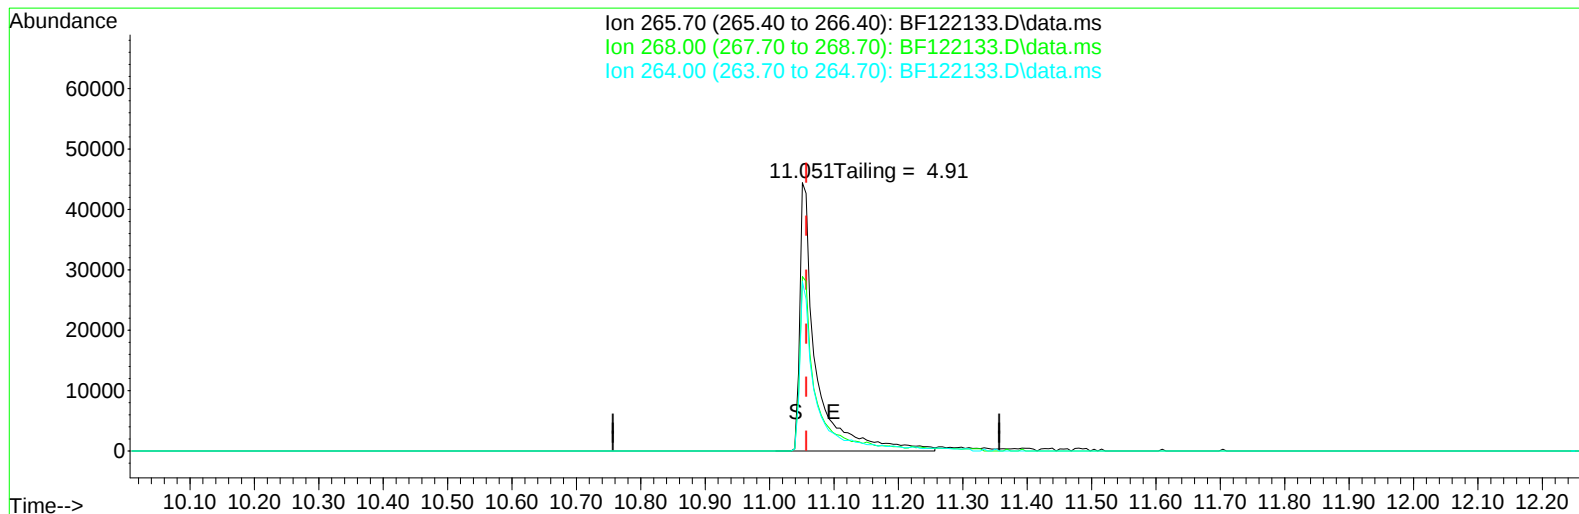

TIC: BF122133.D\data.ms

(70) Pentachlorophenol (C)




11.051min (-0.006) 102072.14 ng

response 78072

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.98
264.00	62.40	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102720\
Data File : BF122133.D
Acq On : 27 Oct 2020 8:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:51:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

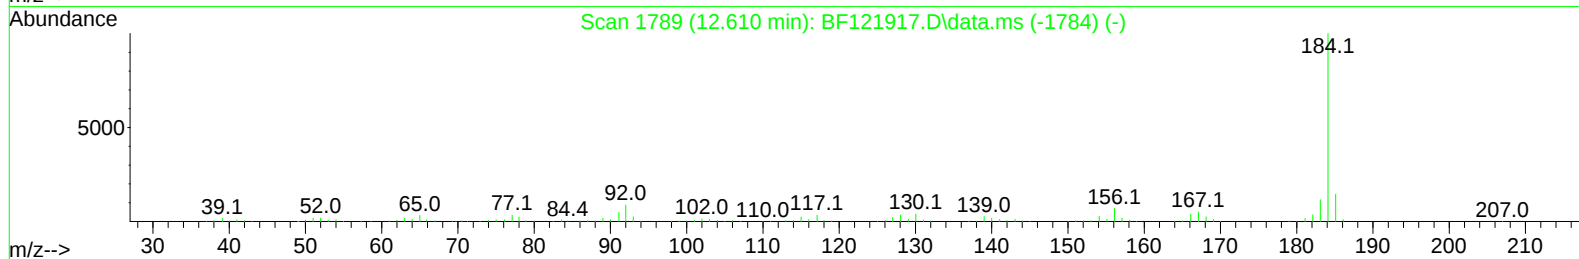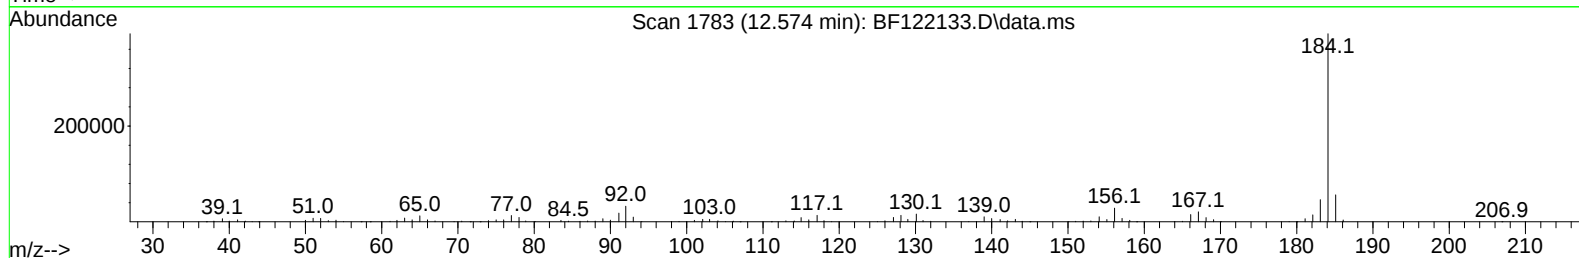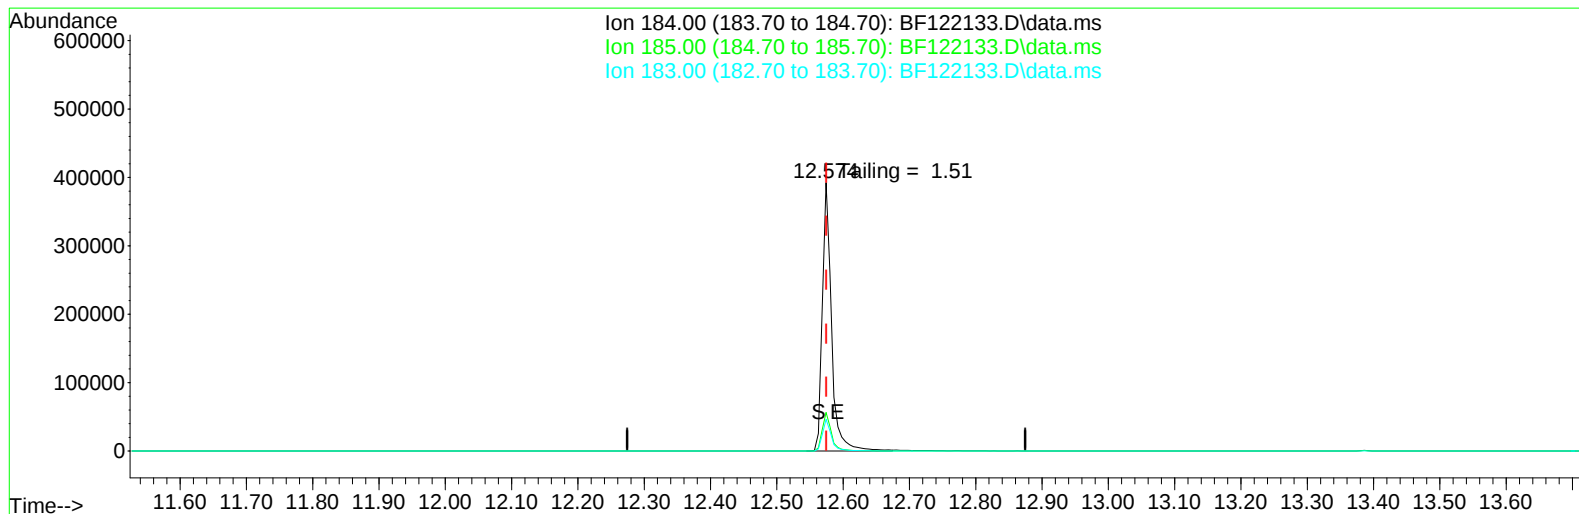

TIC: BF122133.D\data.ms

(77) Benzidine

12.574min (-0.000) 0.00 ng

response 383334

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.39
183.00	11.70	11.84
0.00	0.00	0.00