
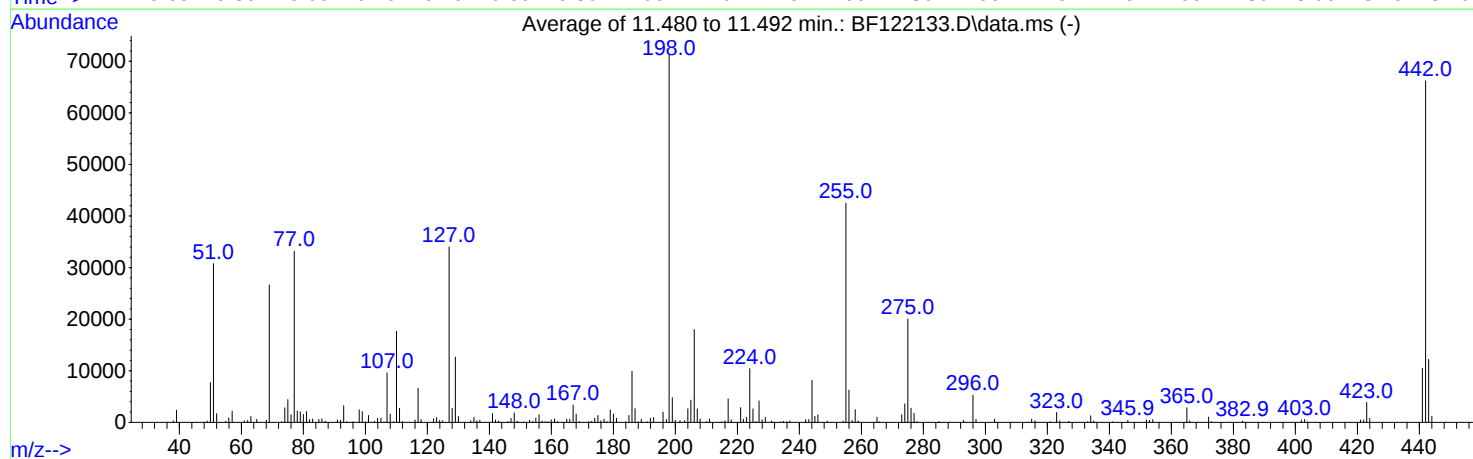


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102720\
 Data File : BF122133.D
 Acq On : 27 Oct 2020 8:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 26 17:27:32 2020

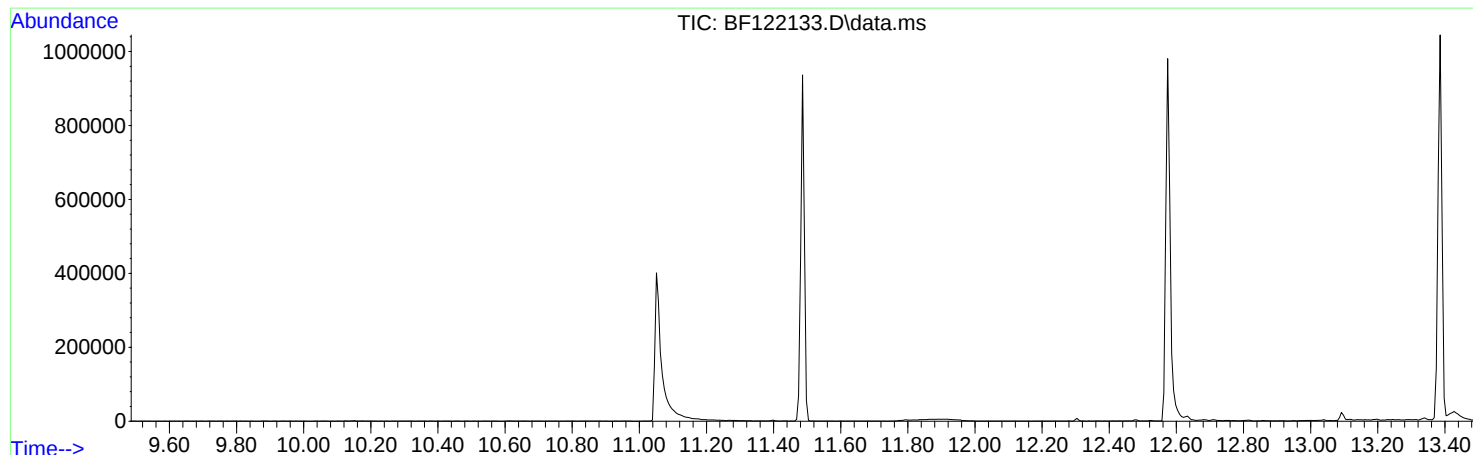

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	30768	PASS
68	69	0.00	2	1.7	440	PASS
69	198	0.00	100	37.4	26655	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	34019	PASS
197	198	0.00	2	0.8	575	PASS
198	198	100	100	100.0	71307	PASS
199	198	5	9	6.7	4771	PASS
275	198	10	60	28.1	20040	PASS
365	198	1	100	4.0	2817	PASS
441	198	0.01	100	14.7	10454	PASS
442	198	50	100	92.8	66179	PASS
443	442	15	24	18.4	12207	PASS