
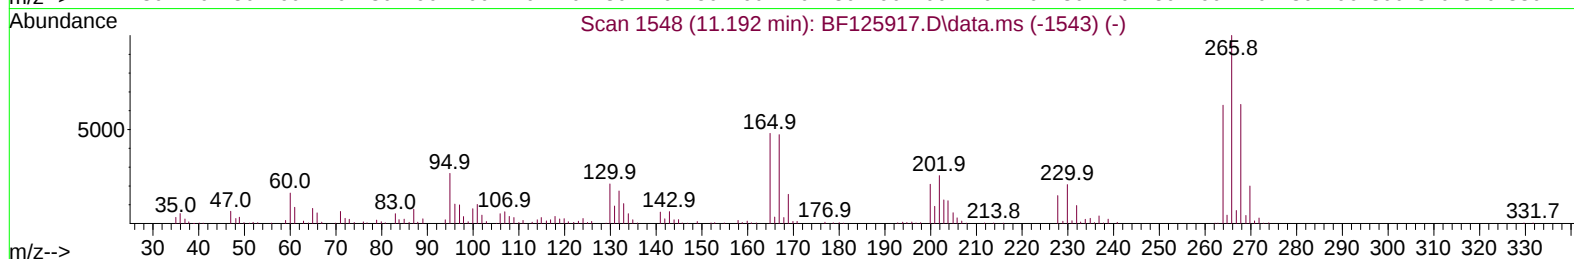
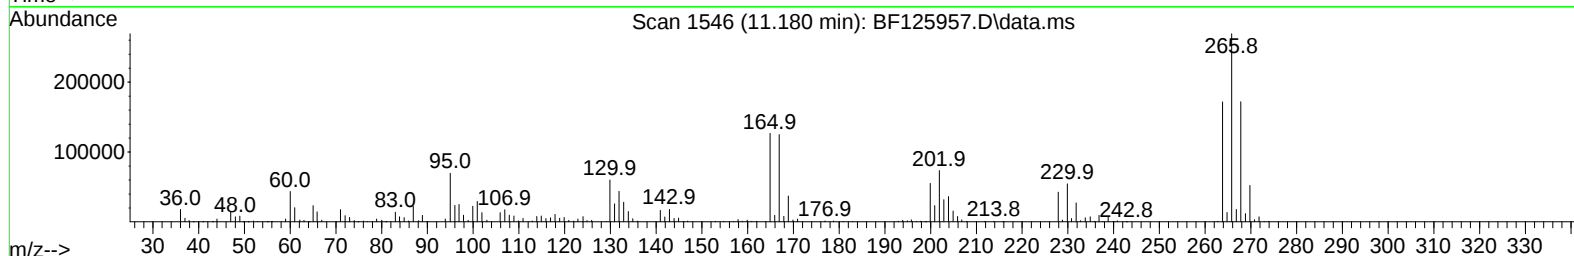


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102721\
Data File : BF125957.D
Acq On : 27 Oct 2021 11:29
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 13:10:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 18:49:16 2021
Response via : Initial Calibration

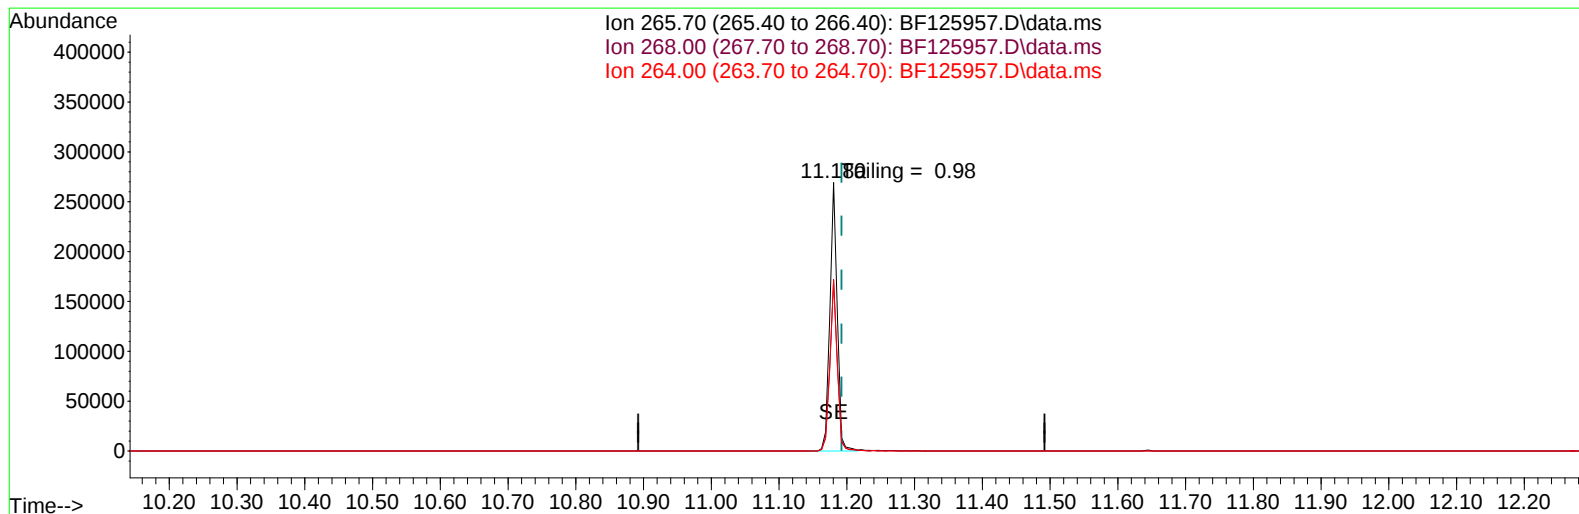

TIC: BF125957.D\data.ms

(70) Pentachlorophenol (C)




11.180min (-0.012) 31467.22 ng

response 204869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.86
264.00	69.90	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102721\
 Data File : BF125957.D
 Acq On : 27 Oct 2021 11:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 13:10:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 18:49:16 2021
 Response via : Initial Calibration

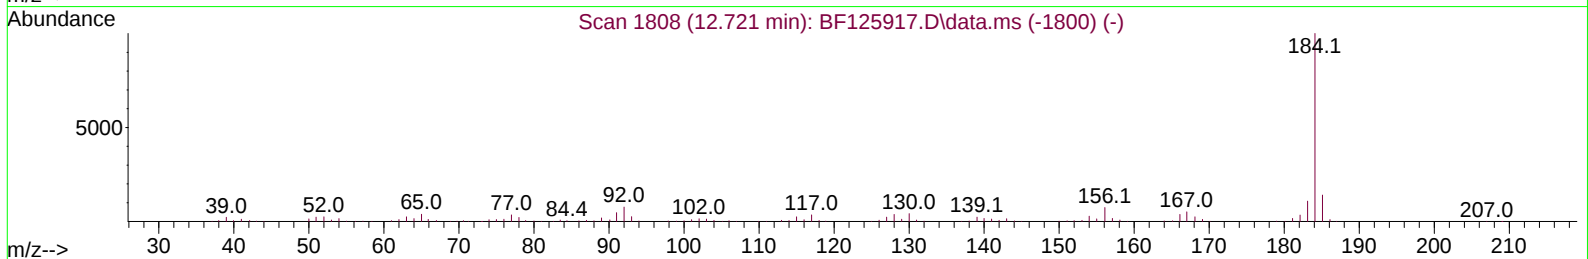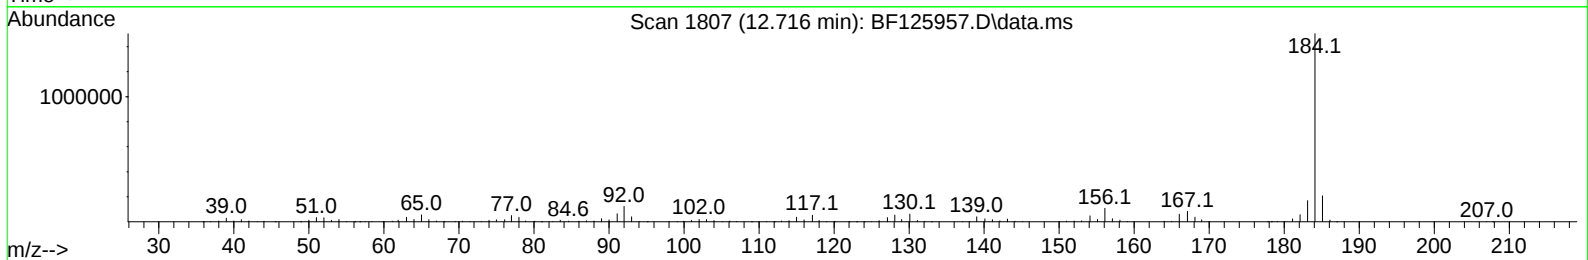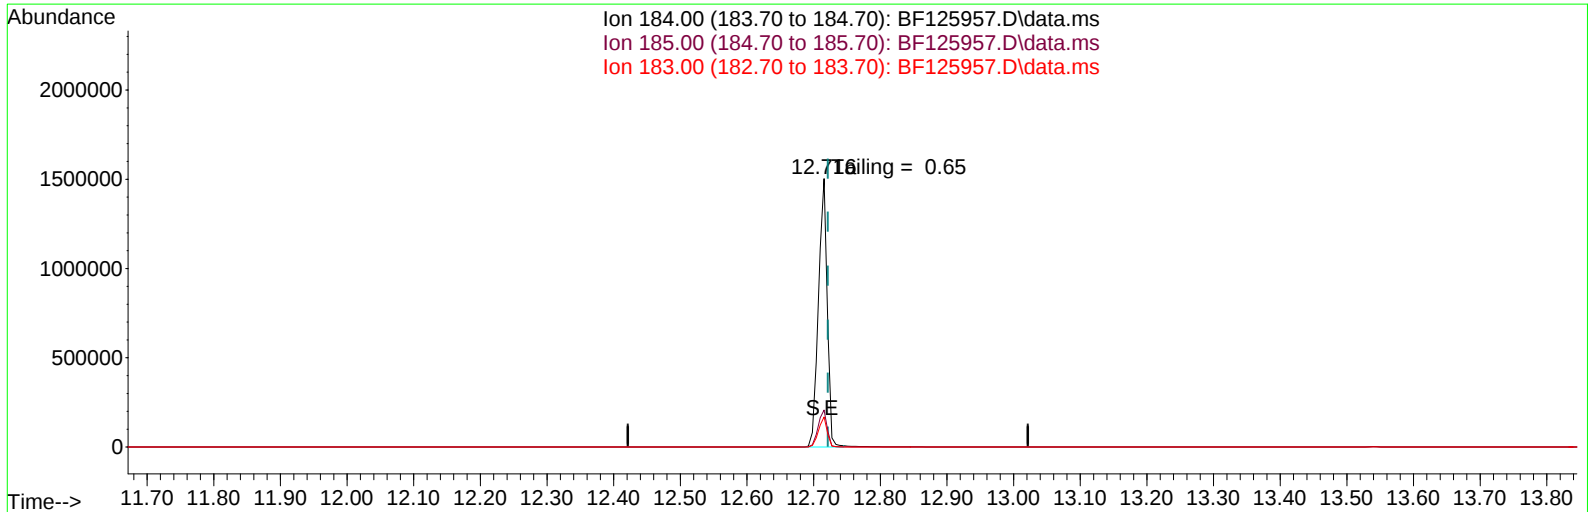

TIC: BF125957.D\data.ms

(77) Benzidine

12.716min (-0.006) 0.00 ng

response 1387748

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.80
183.00	10.10	11.22
0.00	0.00	0.00