


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF102721\  
 Data File : BF125957.D  
 Acq On : 27 Oct 2021 11:29  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF102521.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Oct 28 12:01:54 2021

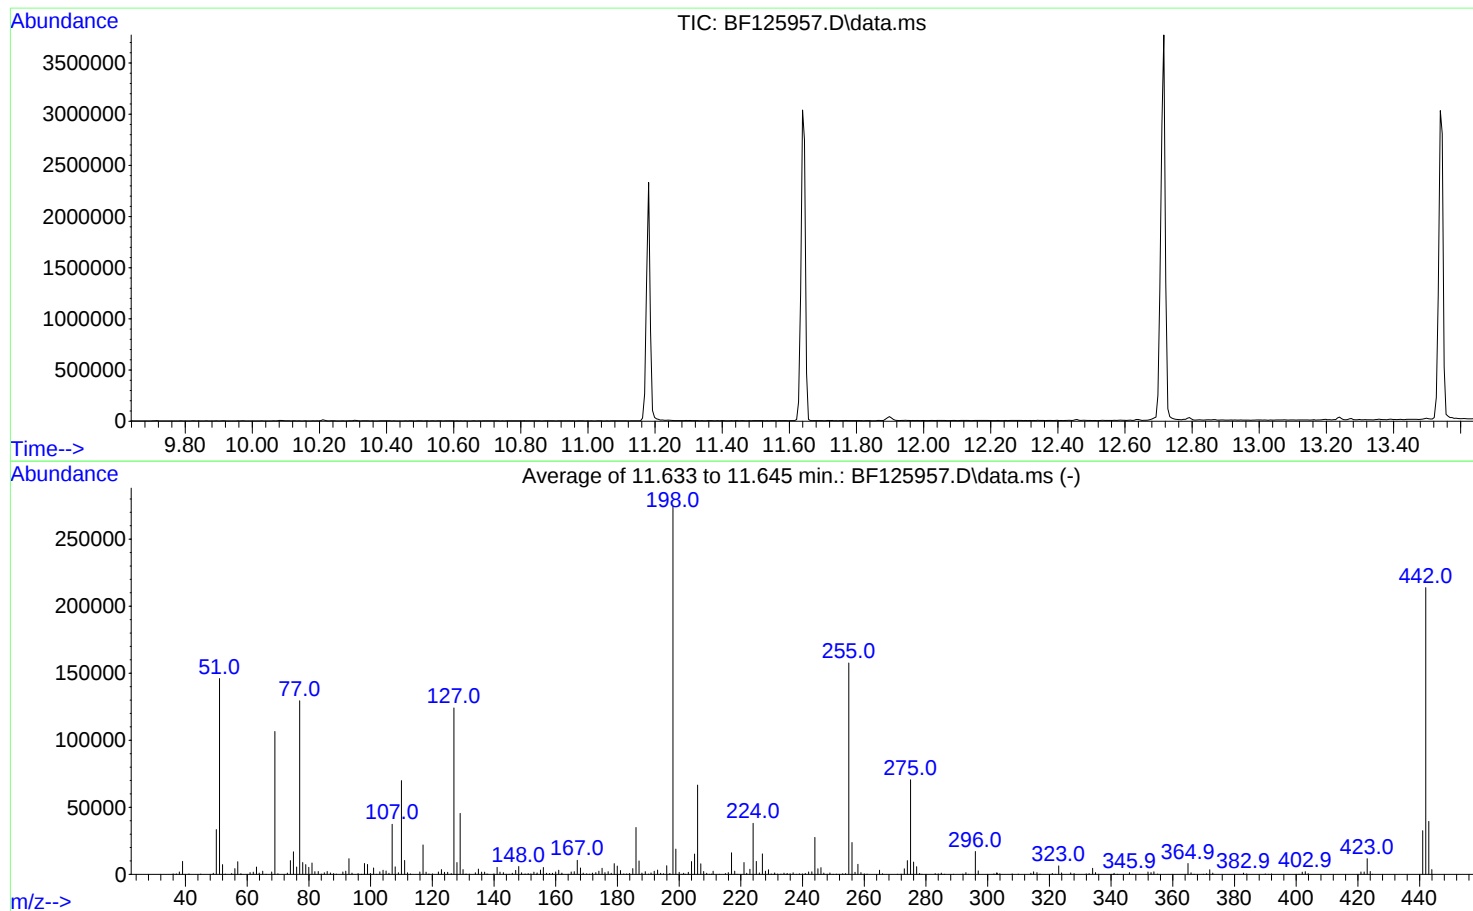

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618




| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 53.2         | 146053     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 1748       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.8         | 106549     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 468        | PASS                |
| 127            | 198             | 10              | 80              | 45.2         | 124120     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 589        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 274347     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 18855      | PASS                |
| 275            | 198             | 10              | 60              | 25.7         | 70576      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 8162       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.9         | 32604      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 213837     | PASS                |
| 443            | 442             | 15              | 24              | 18.5         | 39549      | PASS                |



Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF102721\  
Data File : BF125957.D  
Acq On : 27 Oct 2021 11:29  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Oct 27 13:10:08 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF102521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 25 18:49:16 2021  
Response via : Initial Calibration

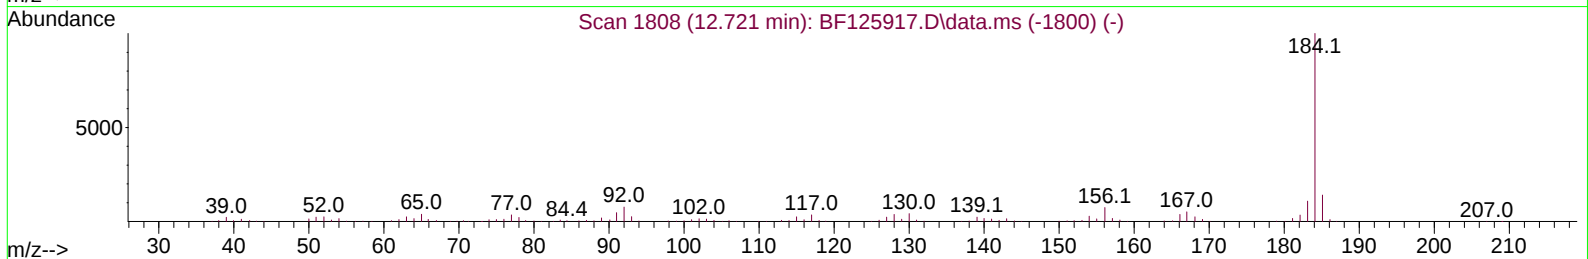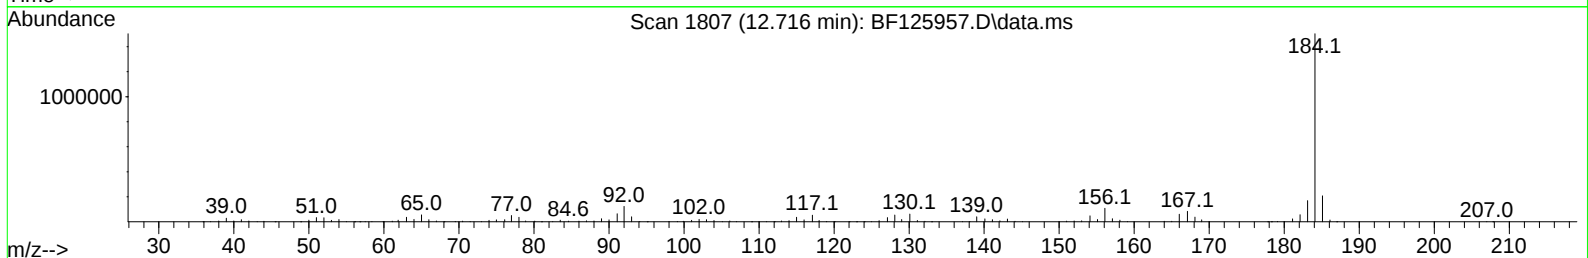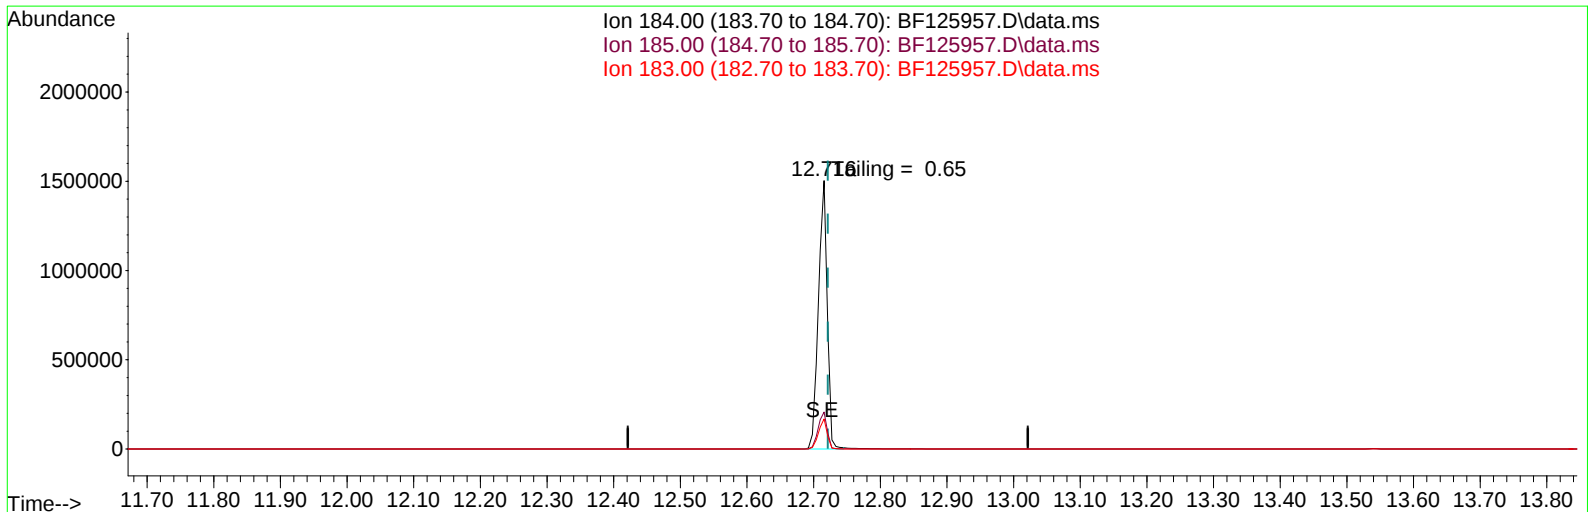

TIC: BF125957.D\data.ms

(77) Benzidine

12.716min (-0.006) 0.00 ng

response 1387748

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 13.80  |
| 183.00 | 10.10  | 11.22  |
| 0.00   | 0.00   | 0.00   |

DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/27/2021    | BNA_F            | BF125957.D         |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 487198           | 13.54              |
| DDD           | 5127             | 13.23              |
| DDE           | 0                | 12.91              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 5127          | 492325           | 1.04               |
|               |                  |                    |