
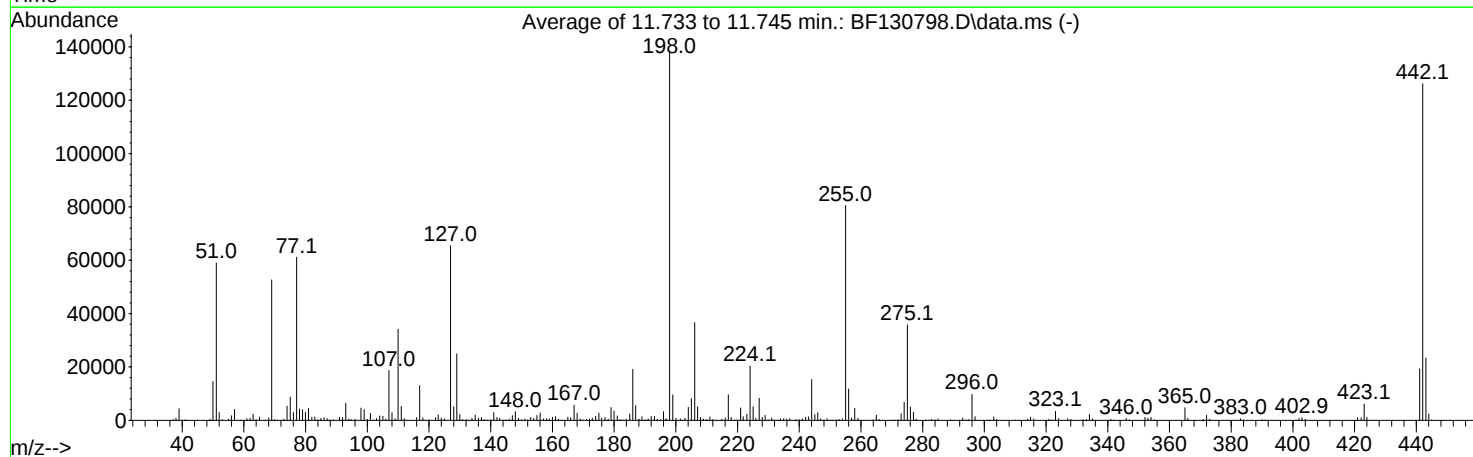


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102722\
 Data File : BF130798.D
 Acq On : 27 Oct 2022 14:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 28 04:00:21 2022

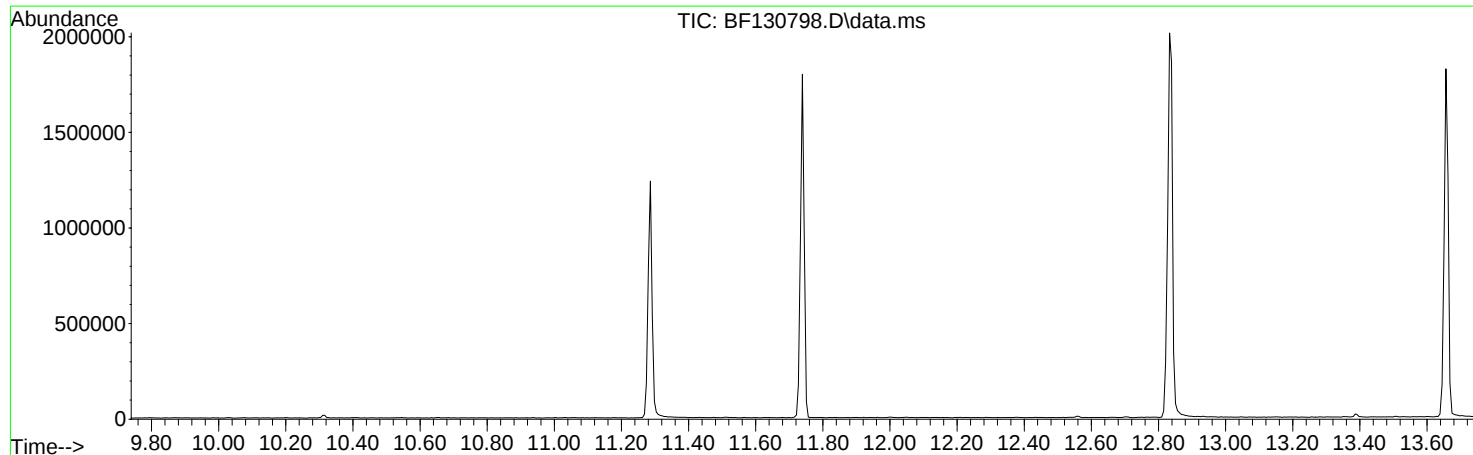




AutoFind: Scans 1674, 1675, 1676; Background Corrected with Scan 1669

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	58952	PASS
68	69	0.00	2	1.7	907	PASS
69	198	0.00	100	38.2	52632	PASS
70	69	0.00	2	0.6	326	PASS
127	198	10	80	47.5	65472	PASS
197	198	0.00	2	0.4	558	PASS
198	198	100	100	100.0	137920	PASS
199	198	5	9	6.9	9539	PASS
275	198	10	60	25.9	35776	PASS
365	198	1	100	3.4	4729	PASS
441	198	0.01	100	13.9	19203	PASS
442	442	50	100	100.0	126200	PASS
443	442	15	24	18.5	23386	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102722\
Data File : BF130798.D
Acq On : 27 Oct 2022 14:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 06:30:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 28 04:00:21 2022
Response via : Initial Calibration

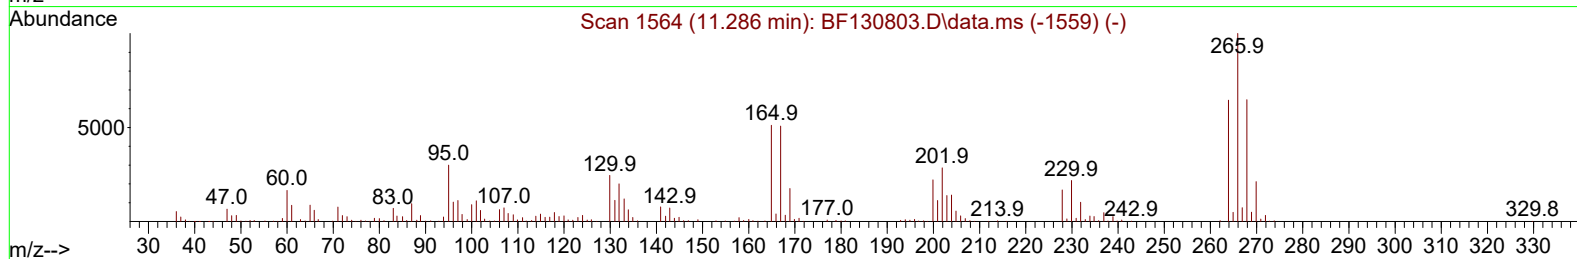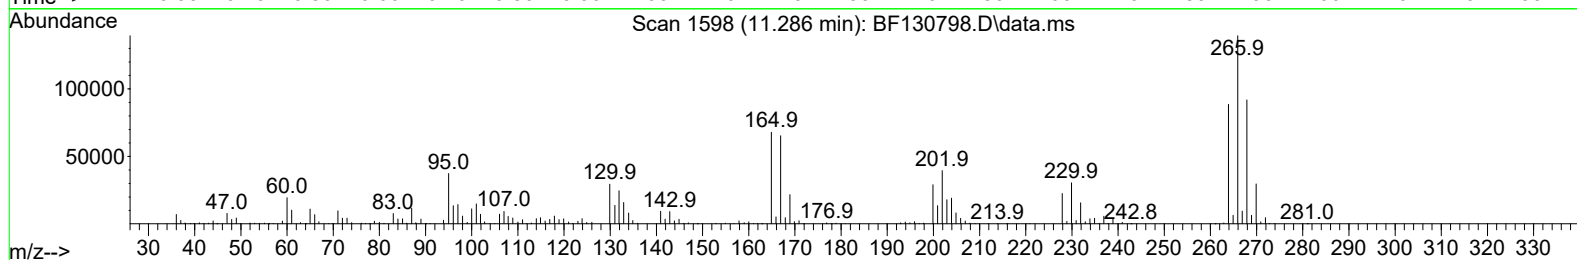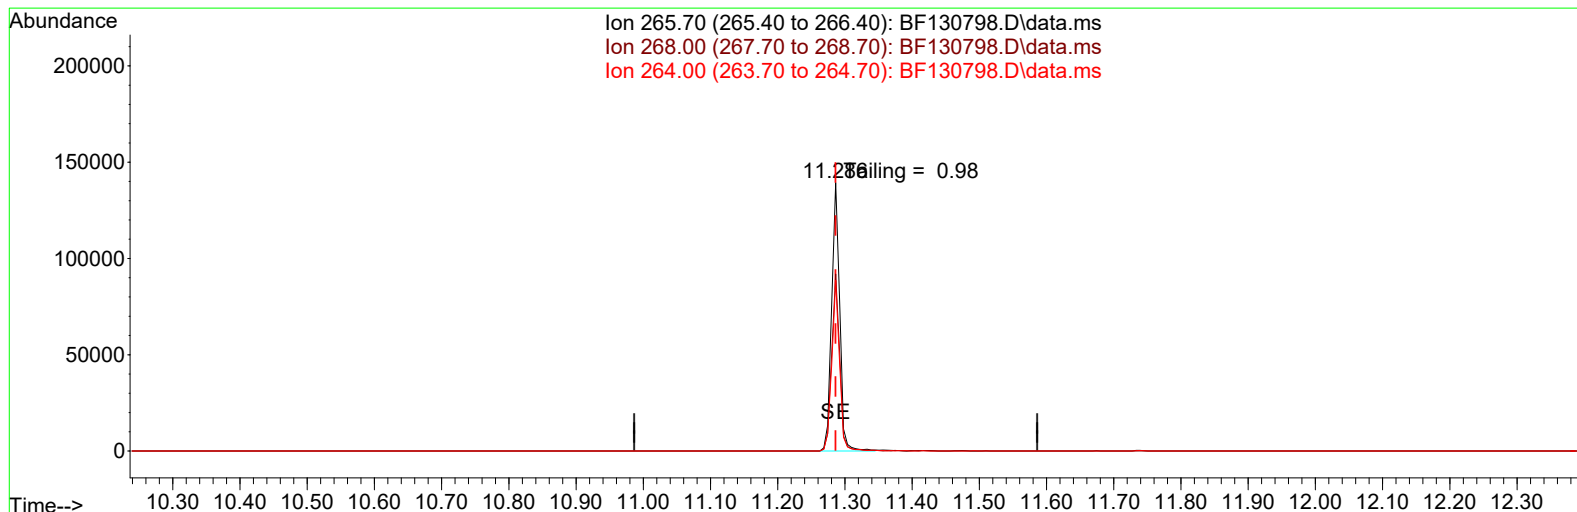

TIC: BF130798.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.000) 29425.83 ng




response 117026

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	65.93
264.00	64.50	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102722\
Data File : BF130798.D
Acq On : 27 Oct 2022 14:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 06:30:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 28 04:00:21 2022
Response via : Initial Calibration

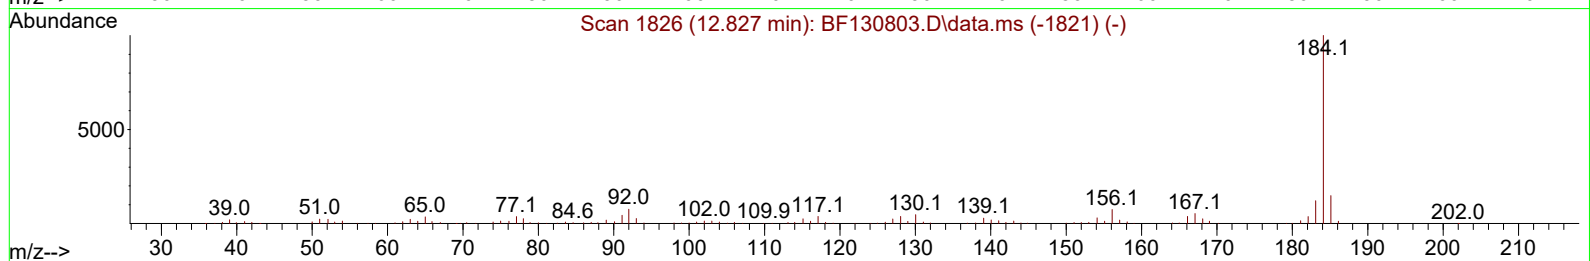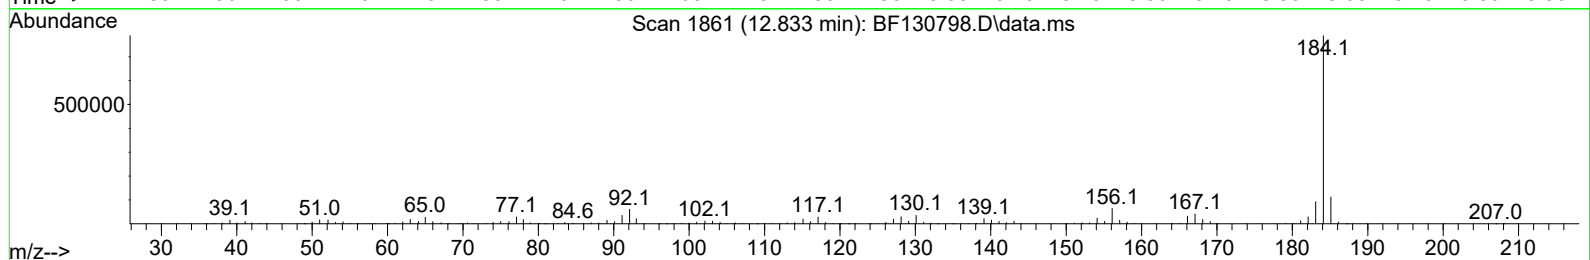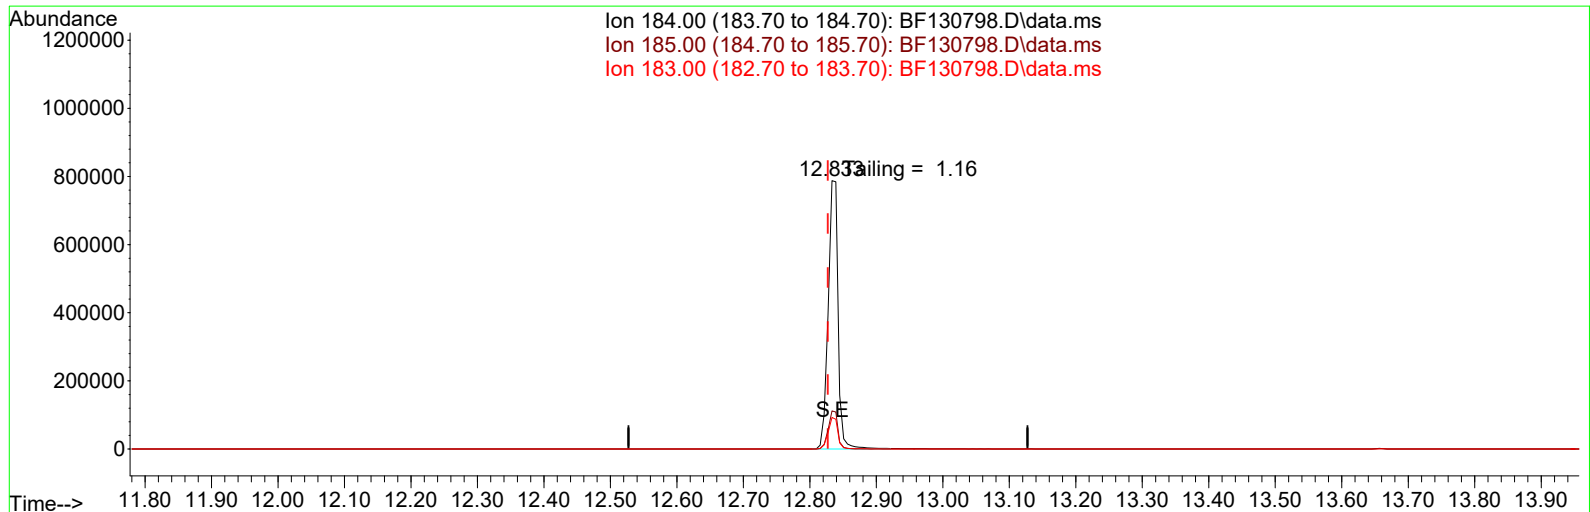

TIC: BF130798.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 0.00 ng

response 823559

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.21
183.00	12.10	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/27/2022	BNA_F	<u>BF130798.D</u>
Compound Name	Response	Retention Time
DDT	145664	13.657
DDD	2463	13.386
DDE	0	12.996
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2463	148127	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP