
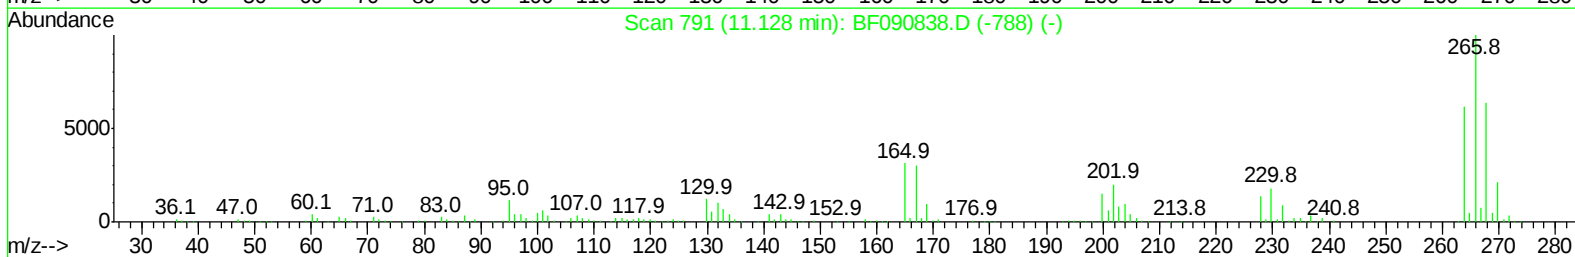
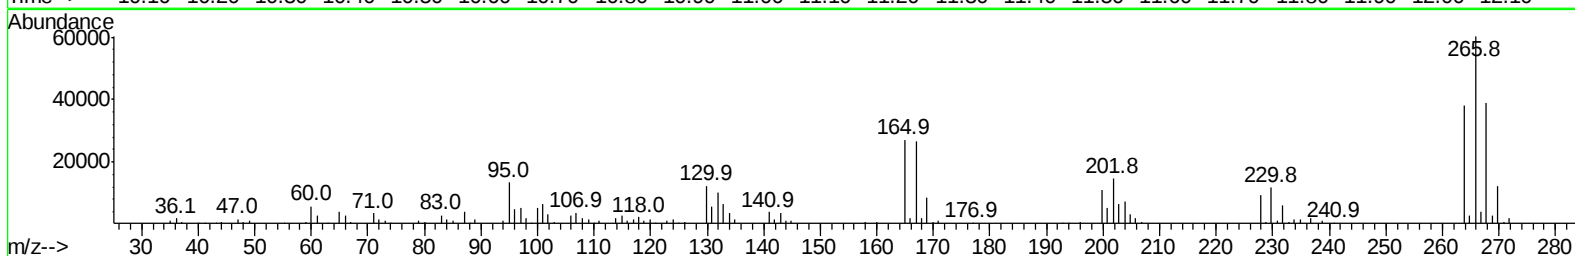


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102816\
Data File : BF090898.D
Acq On : 28 Oct 2016 9:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 19:11:50 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 28 15:18:12 2016
Response via : Initial Calibration

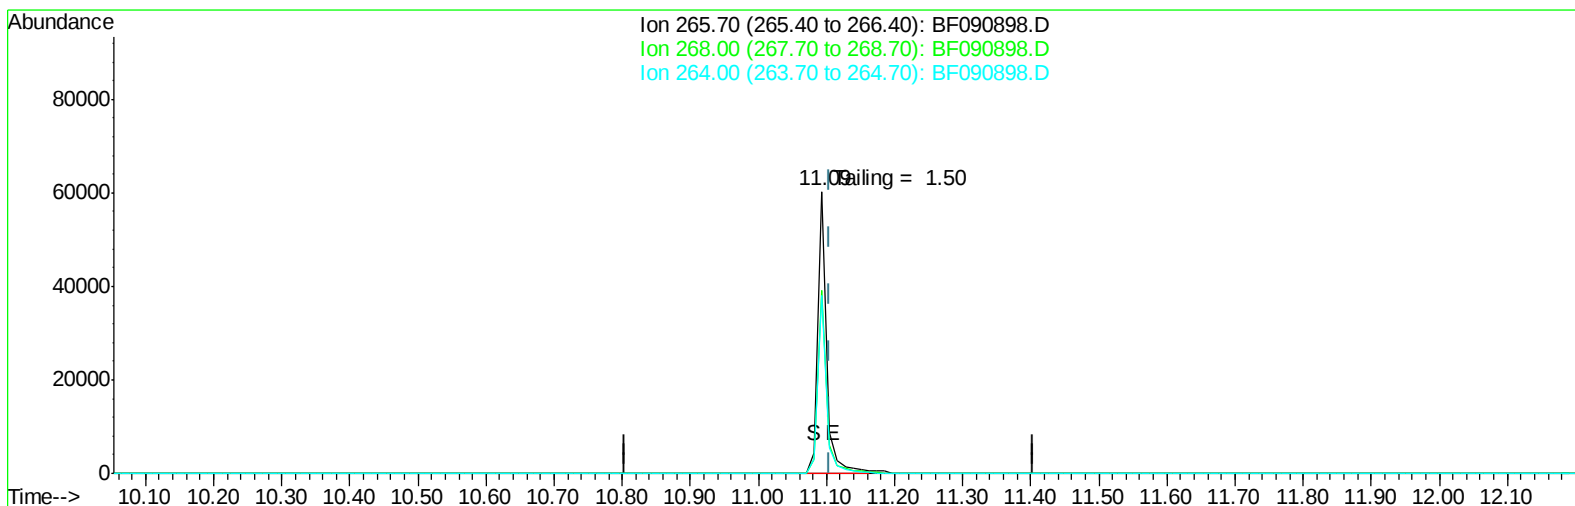

TIC: BF090898.D

(69) Pentachlorophenol (C)




11.093min (-0.011) 0.00ng

response 55500

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.82
264.00	62.70	63.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102816\
Data File : BF090898.D
Acq On : 28 Oct 2016 9:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 19:11:50 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 28 15:18:12 2016
Response via : Initial Calibration

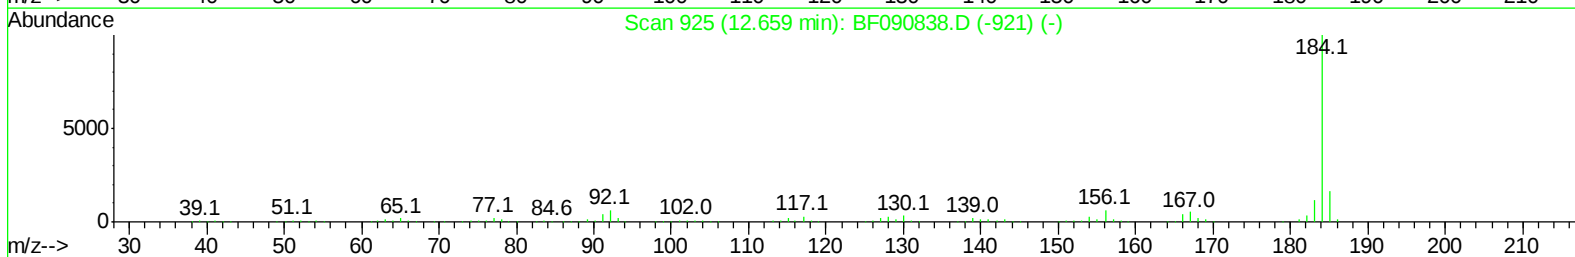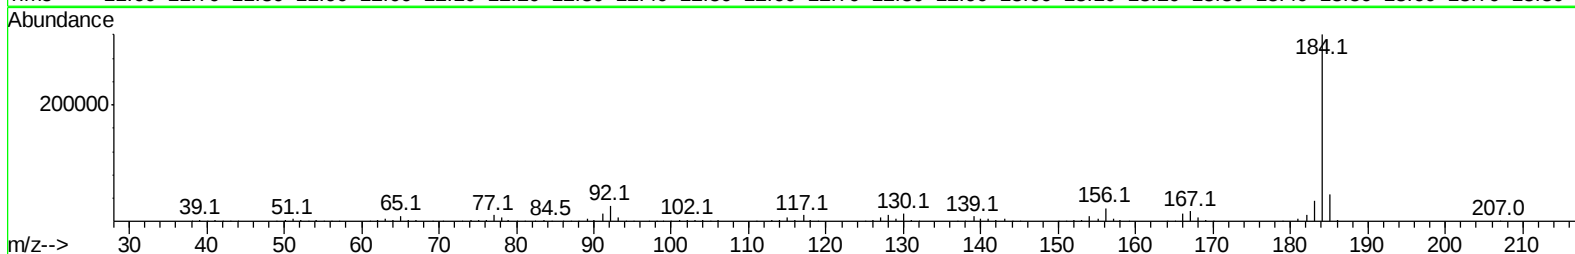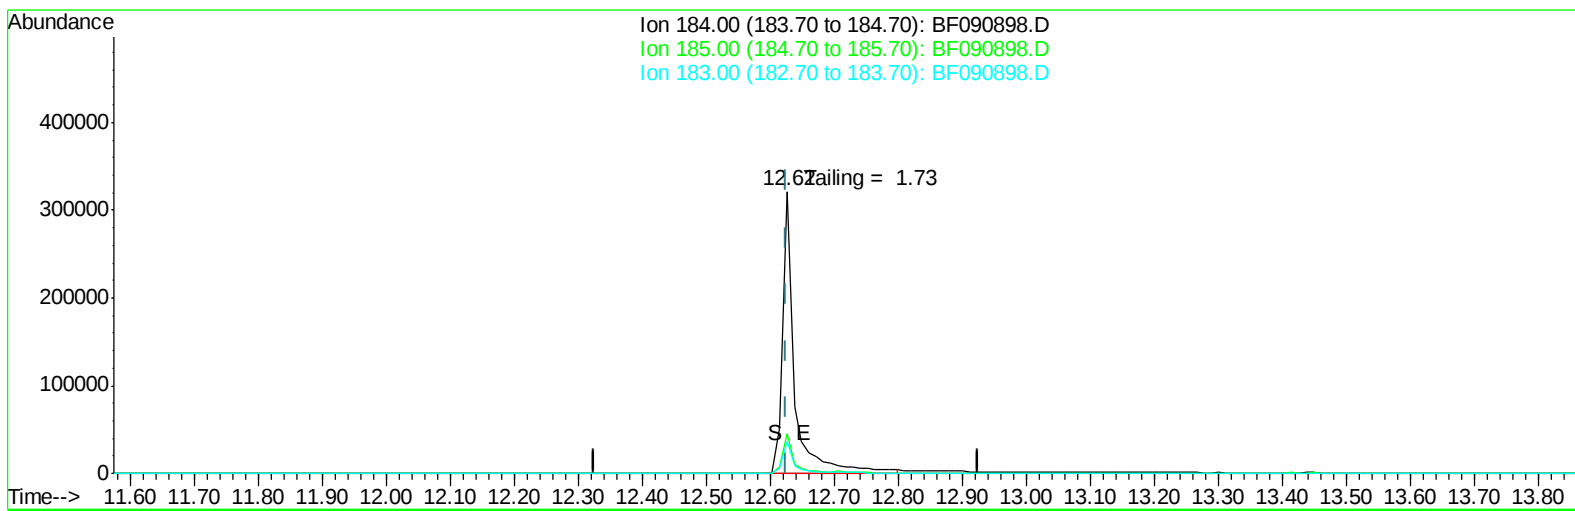

TIC: BF090898.D

(76) Benzidine

12.625min (+0.000) 41551.56ng

response 427325

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.28
183.00	9.50	11.25
0.00	0.00	0.00