


Data Path : Z:\HPCHEM1\BNA_F\Data\BF102816\
 Data File : BF090898.D
 Acq On : 28 Oct 2016 9:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 01 11:53:50 2016

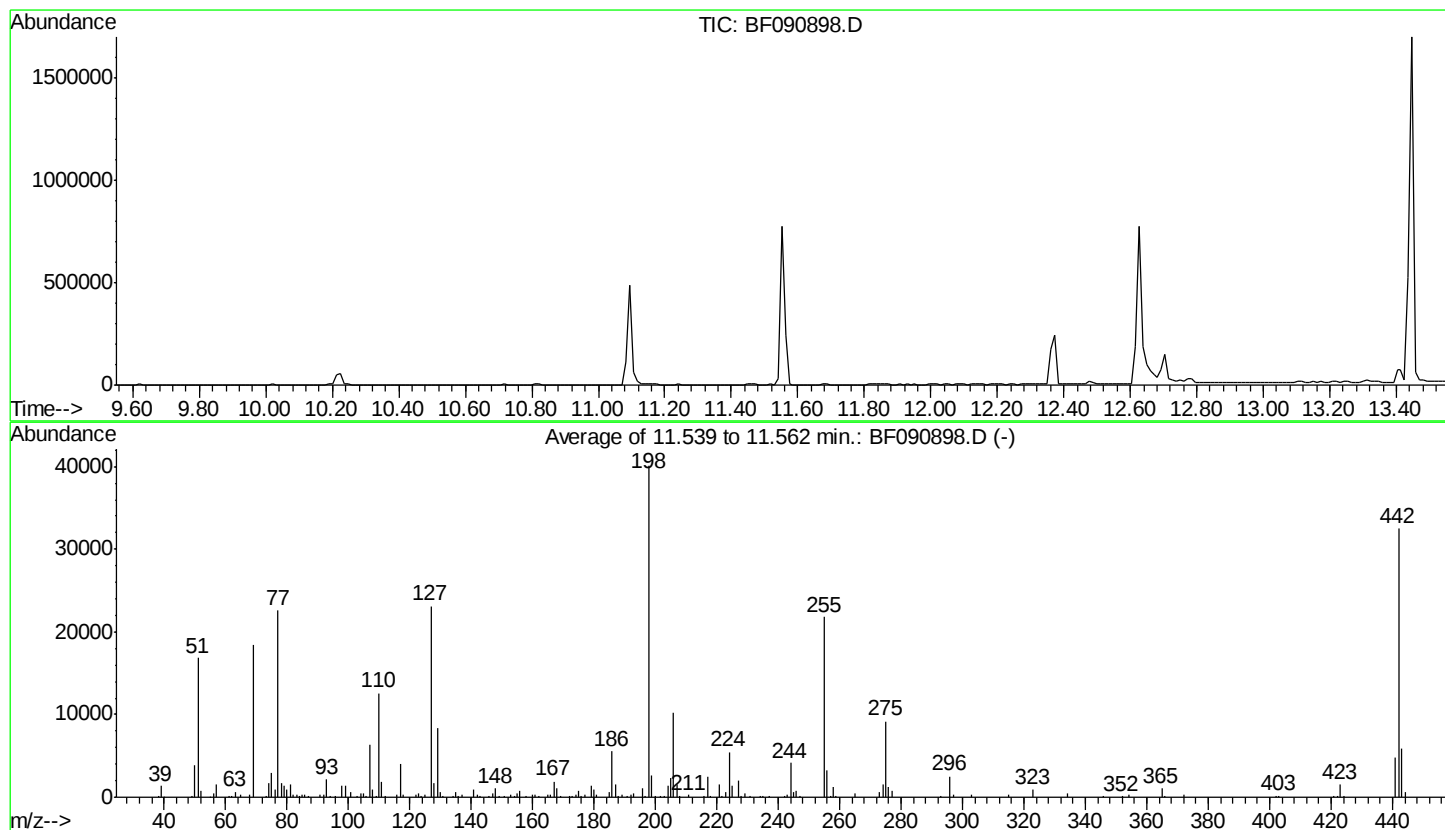

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	16843	PASS
68	69	0.00	2	1.4	256	PASS
69	198	0.00	100	46.1	18494	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.6	23104	PASS
197	198	0.00	2	0.3	120	PASS
198	198	100	100	100.0	40115	PASS
199	198	5	9	6.6	2633	PASS
275	198	10	60	22.8	9151	PASS
365	198	1	100	2.7	1079	PASS
441	442	0.01	24	14.9	4829	PASS
442	198	50	100	81.0	32485	PASS
443	442	15	24	17.9	5812	PASS