

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102817\
 Data File : BF099918.D
 Acq On : 28 Oct 2017 15:39
 Operator : SJ/JU
 Sample : I6071-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EPE-P-5A(10-12)

Quant Time: Oct 30 02:51:54 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 27 15:58:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	92598	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	385790	20.00	ng	-0.01
38) Acenaphthene-d10	9.82	164	173017	20.00	ng	-0.02
63) Phenanthrene-d10	11.32	188	274587	20.00	ng	-0.02
75) Chrysene-d12	13.96	240	171230	20.00	ng	-0.03
86) Perylene-d12	15.43	264	174319	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	552137	93.61	ng	0.00
7) Phenol-d6	6.43	99	658429	94.15	ng	0.00
23) Nitrobenzene-d5	7.36	82	383543	64.01	ng	-0.01
41) 2,4,6-Tribromophenol	10.62	330	123124	78.09	ng	-0.02
44) 2-Fluorobiphenyl	9.14	172	809601	72.19	ng	-0.02
78) Terphenyl-d14	12.90	244	556873	71.07	ng	-0.02
Target Compounds						
10) Phenol	6.45	94	17224	2.243	ng	80
49) Dimethylphthalate	9.54	163	120362	8.785	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102817\
Data File : BF099918.D
Acq On : 28 Oct 2017 15:39
Operator : SJ/JU
Sample : I6071-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EPE-P-5A(10-12)

Quant Time: Oct 30 02:51:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 27 15:58:57 2017
Response via : Initial Calibration

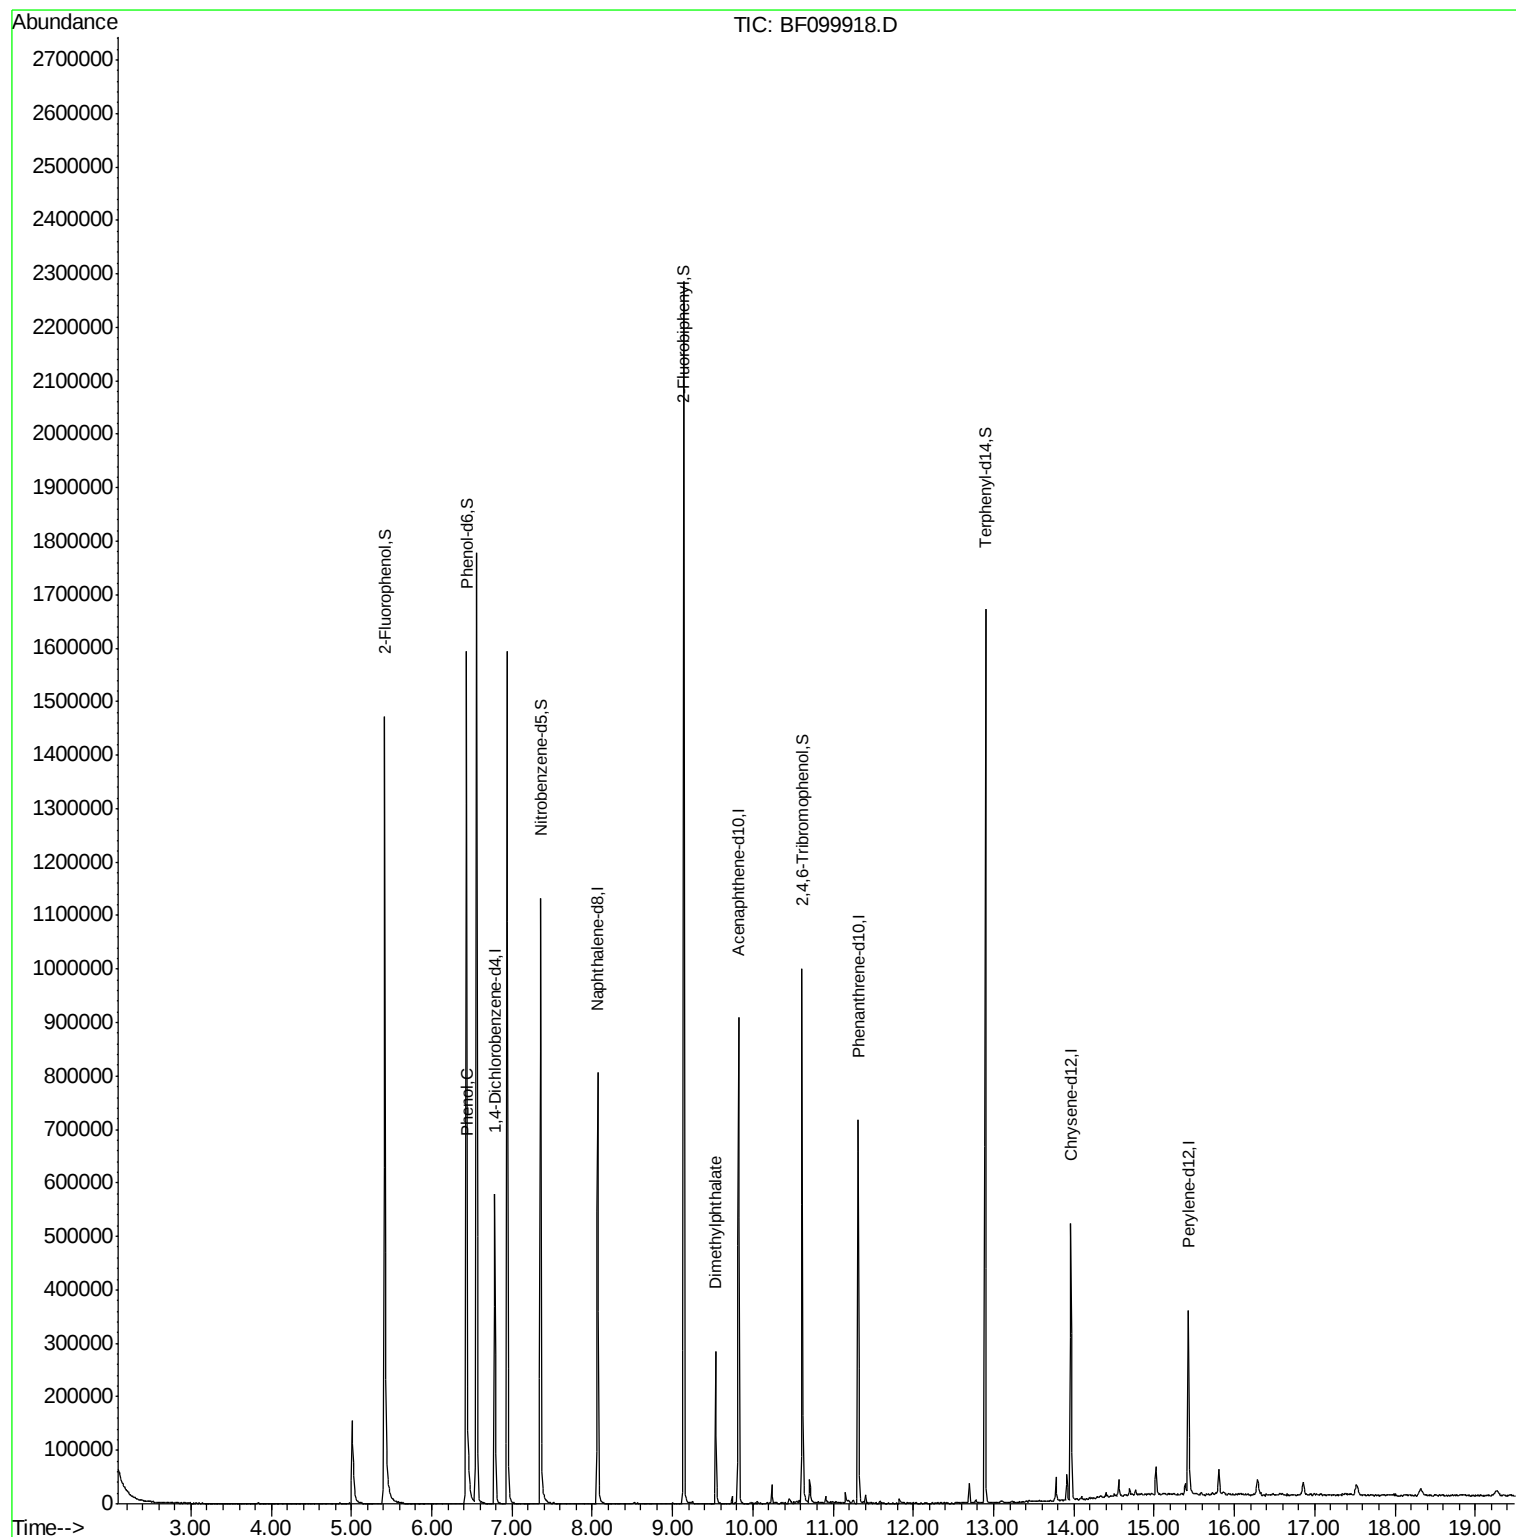

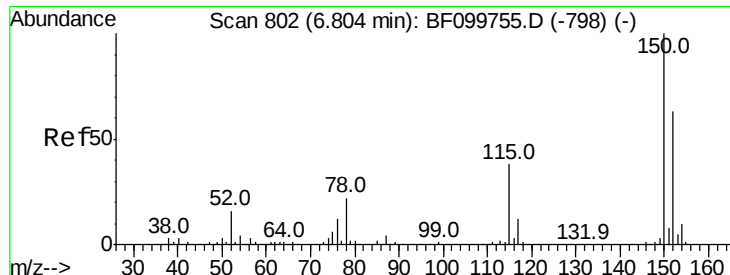


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. -0.01 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Instrument :
BNA_F
ClientSampleId :
EPE-P-5A(10-12)

Tot Ion:152 Resp: 92598
Ion Ratio Lower Upper
152 100
150 157.8 124.6 186.8
115 57.6 50.1 75.1

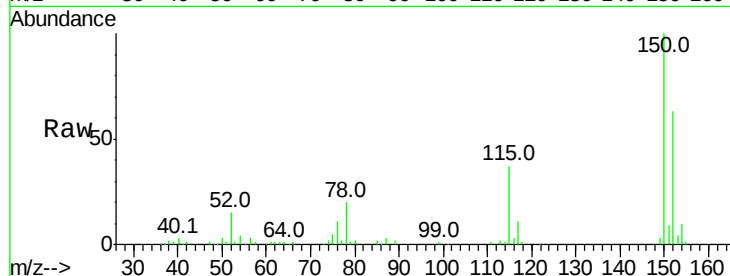


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

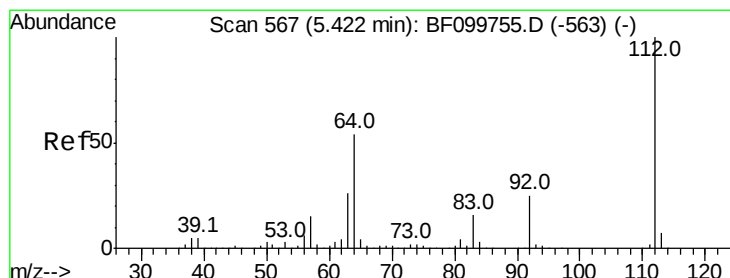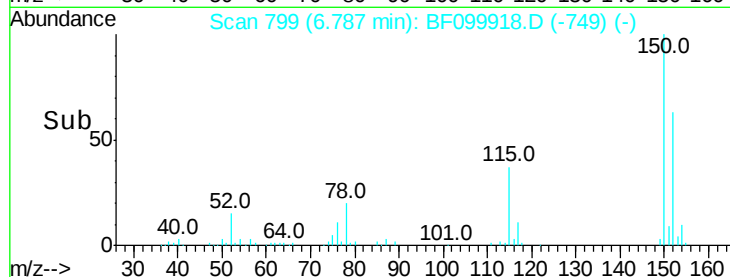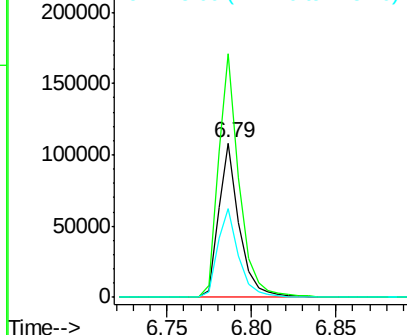



#5


2-Fluorophenol
Concen: 93.613 ng
RT: 5.41 min Scan# 565
Delta R.T. -0.01 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Tgt Ion:112 Resp: 552137
Ion Ratio Lower Upper
112 100
64 52.0 47.9 71.9
63 24.6 23.7 35.5

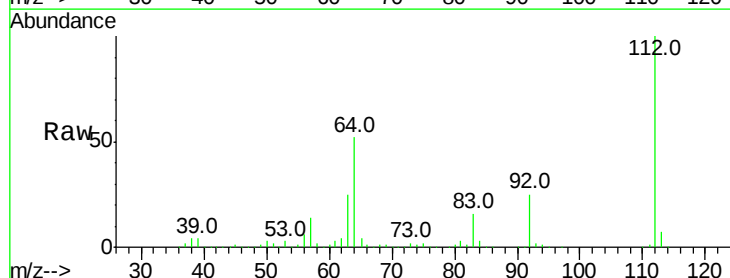

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

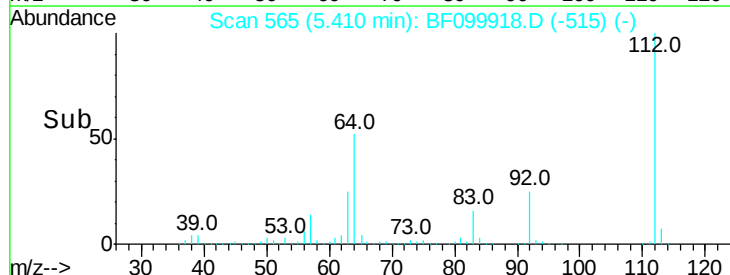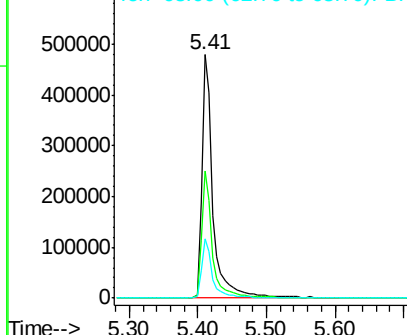

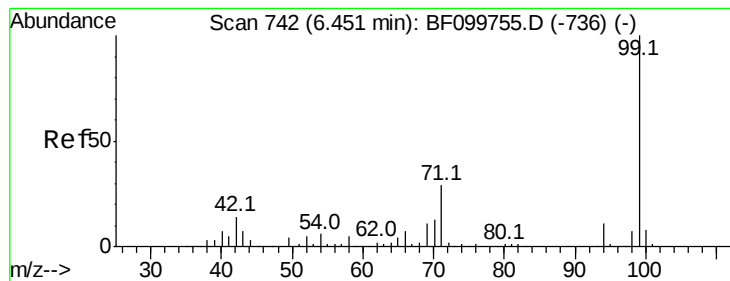

#7

Phenol-d6

Concen: 94.149 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF099918.D

Acq: 28 Oct 2017 15:39

Instrument :

BNA_F

ClientSampleId :

EPE-P-5A(10-12)


Tot Ion: 99 Resp: 658429

Ion Ratio Lower Upper

99 100

42 13.3 14.5 21.7#


71 28.4 25.4 38.0

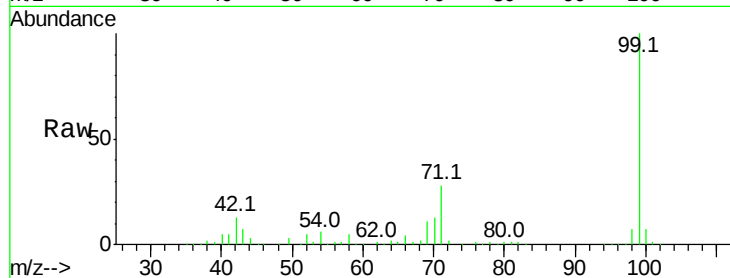



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

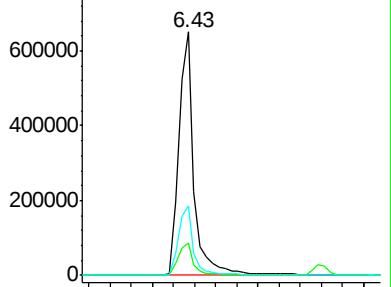

Time-->

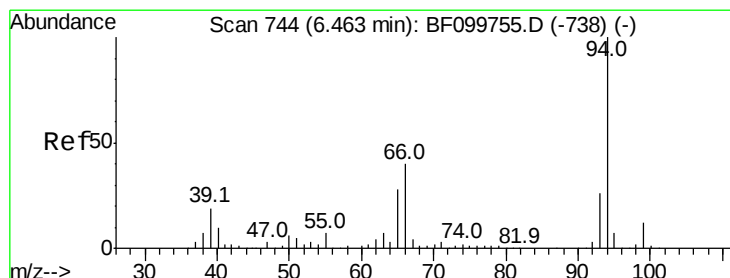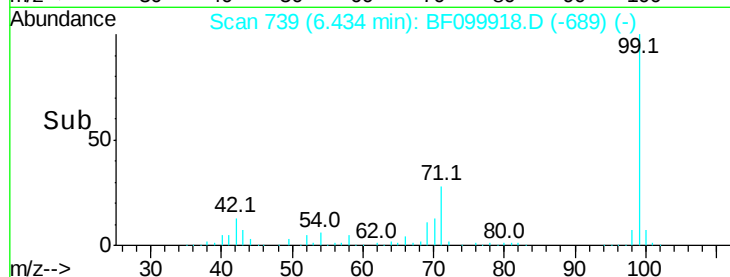

#10

Phenol

Concen: 2.243 ng

RT: 6.45 min Scan# 741

Delta R.T. -0.01 min

Lab File: BF099918.D

Acq: 28 Oct 2017 15:39


Tgt Ion: 94 Resp: 17224

Ion Ratio Lower Upper

94 100

65 25.0 7.9 47.9


66 55.1 16.2 56.2

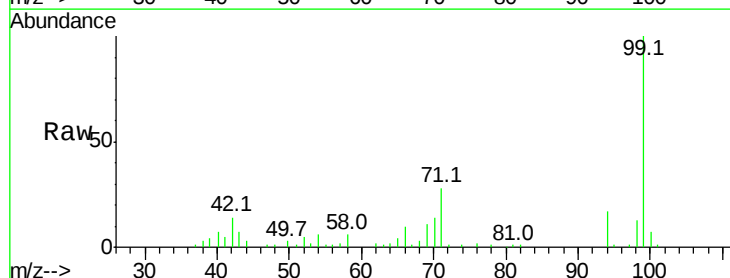


Abundance Ion 94.00 (93.70 to 94.70): BF0


Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

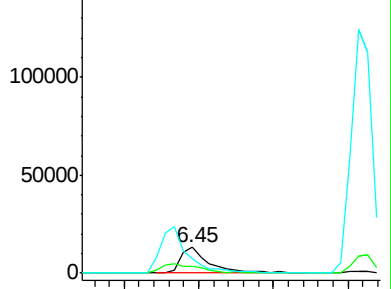

Time-->

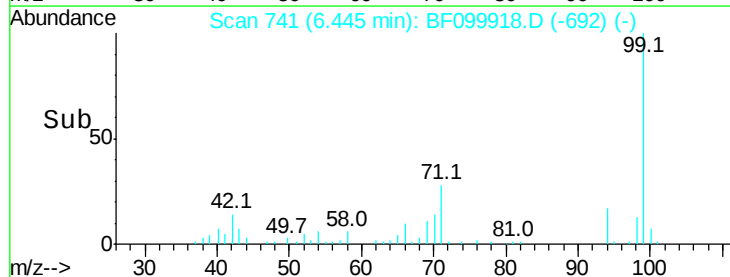


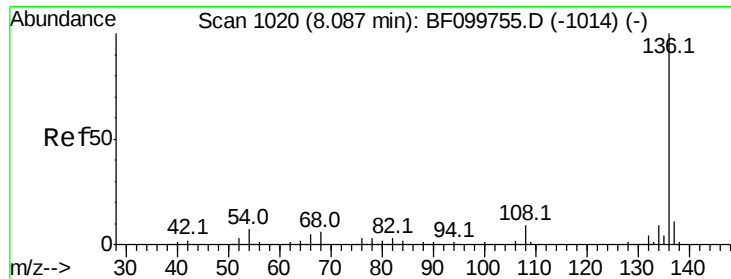




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.07 min Scan# 1017
Delta R.T. -0.01 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Instrument :
BNA_F
ClientSampleId :
EPE-P-5A(10-12)

Tot Ion:	136	Resp:	385790
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	6.3	6.6	9.8#
68	5.4	5.0	7.4

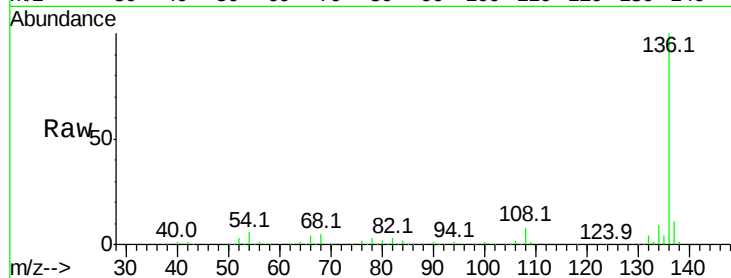


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

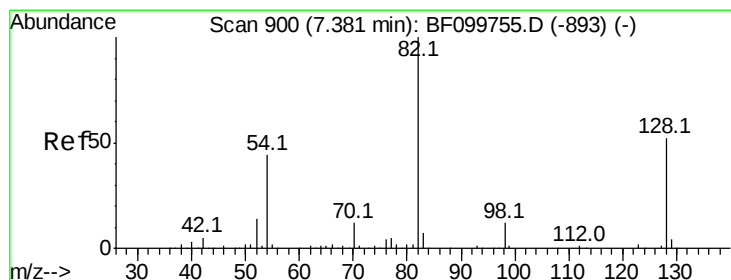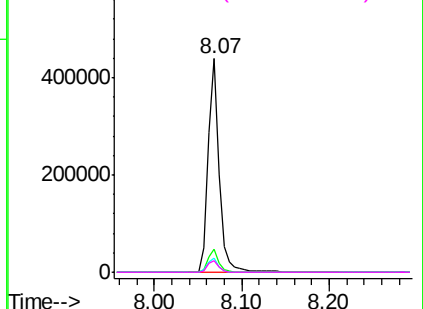
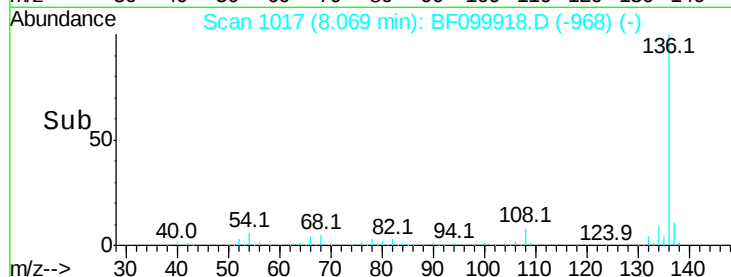



#23
Nitrobenzene-d5
Concen: 64.006 ng
RT: 7.36 min Scan# 896
Delta R.T. -0.01 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Tgt Ion:	82	Resp:	383543
Ion	Ratio	Lower	Upper
82	100		
128	51.2	36.1	54.1
54	43.4	41.4	62.2

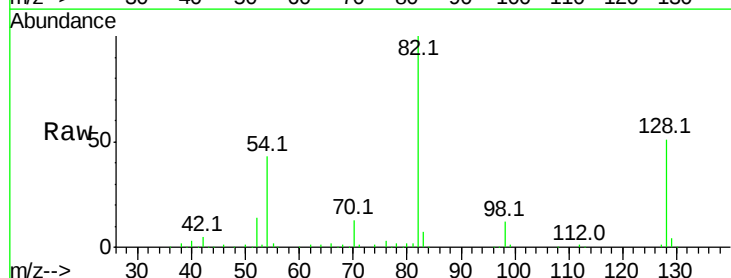

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0



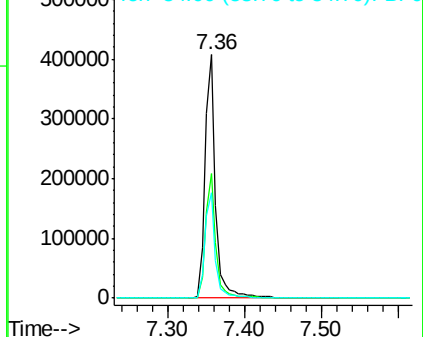
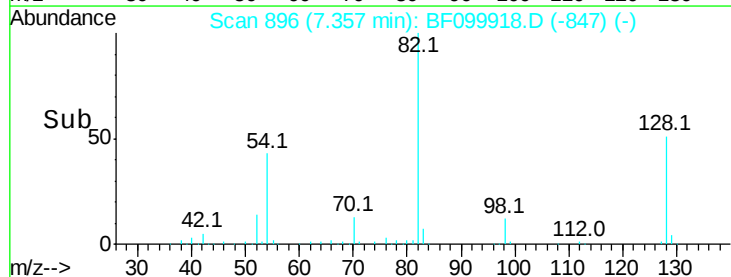


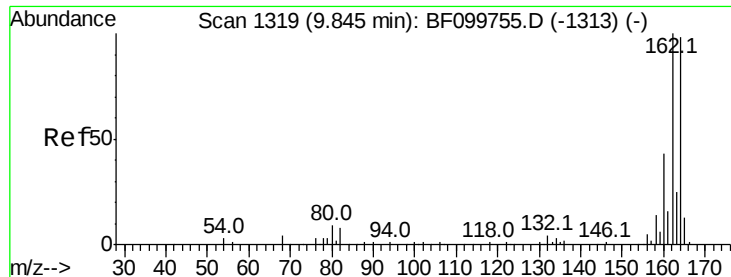

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.82 min Scan# 1315
Delta R.T. -0.02 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39




Instrument :
BNA_F
ClientSampleId :
EPE-P-5A(10-12)


Tot Ion	Ratio	Lower	Upper
164	100		
162	102.0	86.1	129.1
160	45.4	38.3	57.5

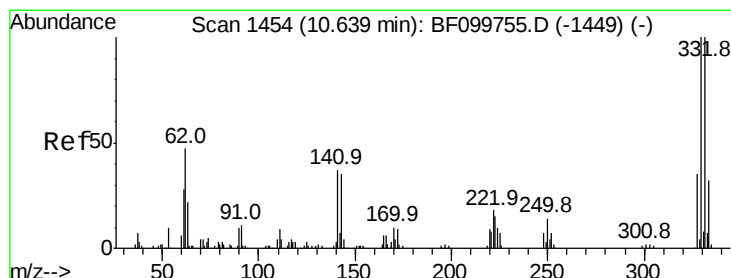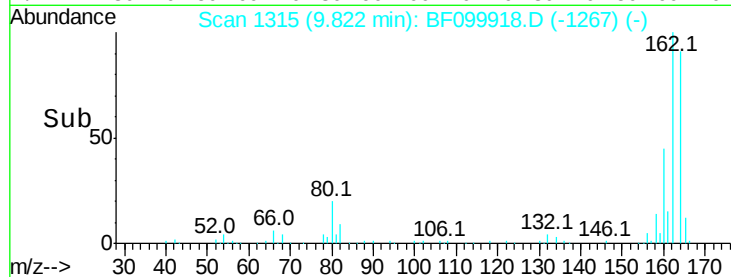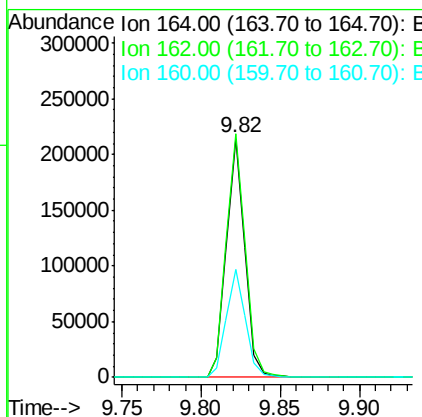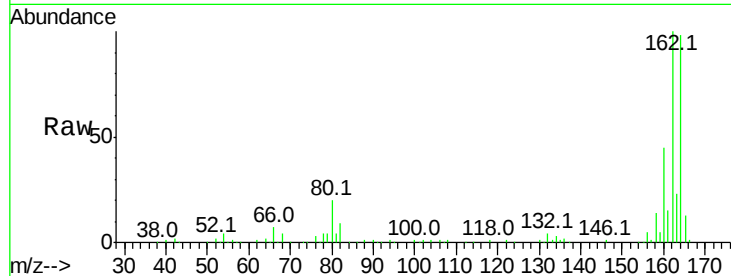

#41
2,4,6-Tribromophenol
Concen: 78.088 ng
RT: 10.62 min Scan# 1450
Delta R.T. -0.02 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.0	115.6
141	35.1	29.9	44.9


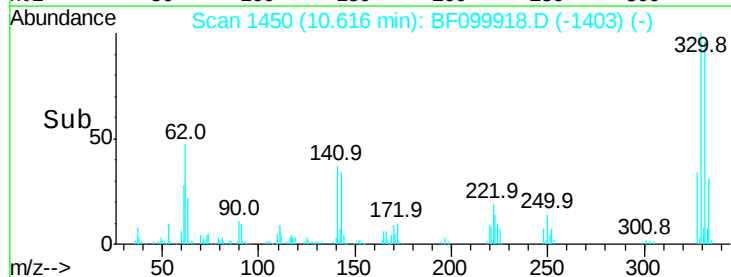
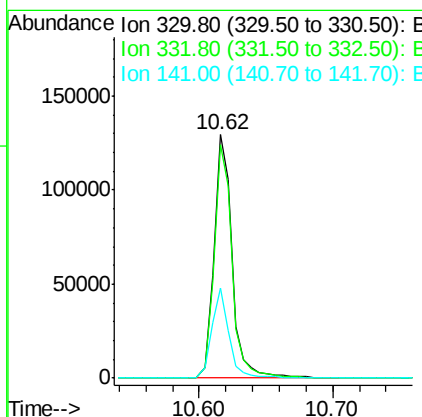
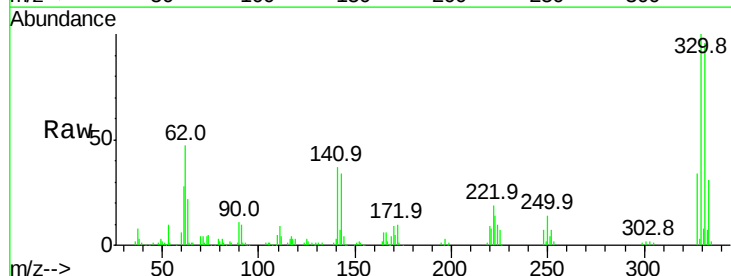


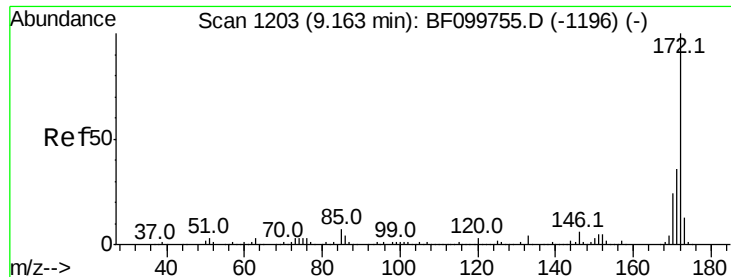

#44
2-Fluorobiphenyl
Concen: 72.194 ng
RT: 9.14 min Scan# 1199
Delta R.T. -0.02 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39




Instrument :
BNA_F
ClientSampleId :
EPE-P-5A(10-12)


Tot Ion:172 Resp: 809601
Ion Ratio Lower Upper
172 100
171 36.1 29.7 44.5
170 23.3 19.6 29.4

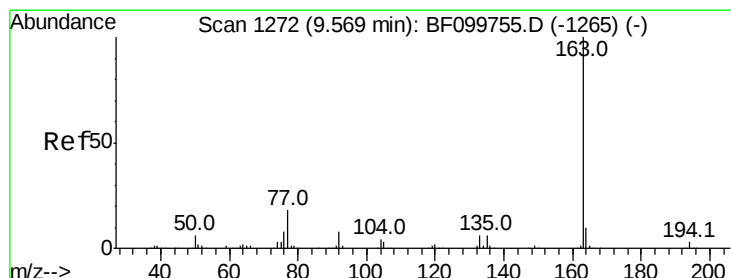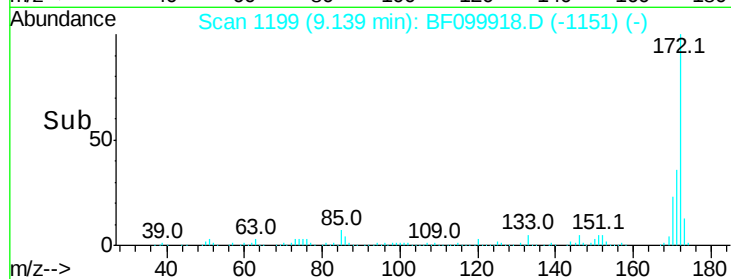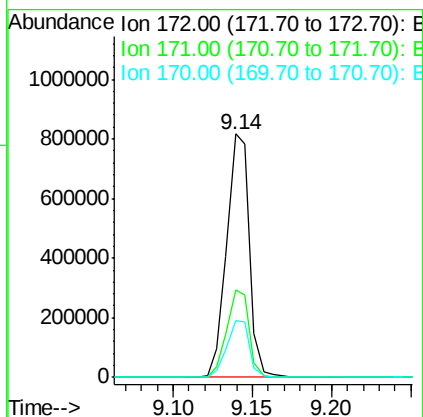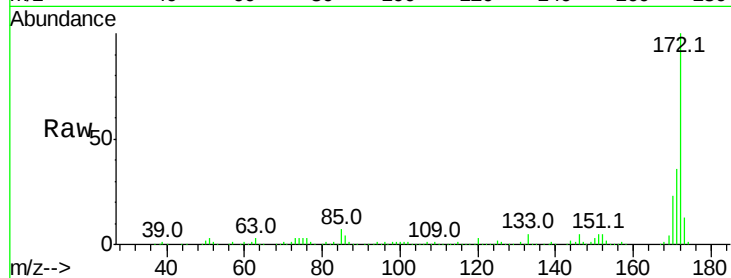

#49
Dimethylphthalate
Concen: 8.785 ng
RT: 9.54 min Scan# 1267
Delta R.T. -0.02 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Tgt Ion:163 Resp: 120362
Ion Ratio Lower Upper
163 100
194 3.5 2.7 4.1
164 10.0 8.2 12.2


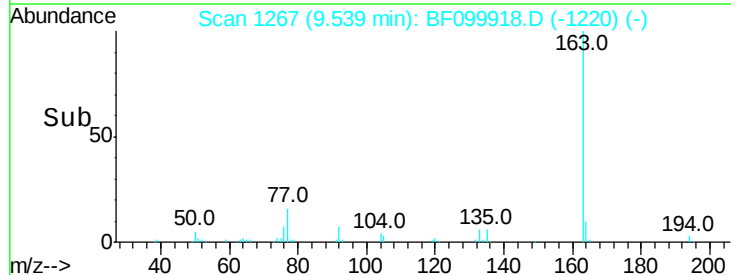
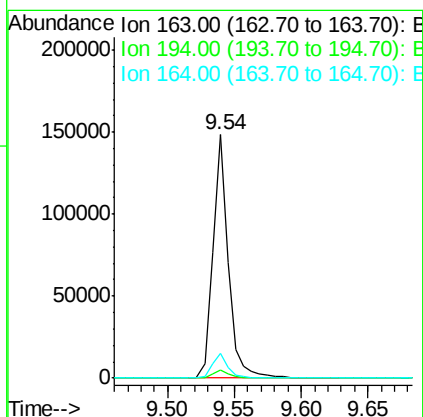
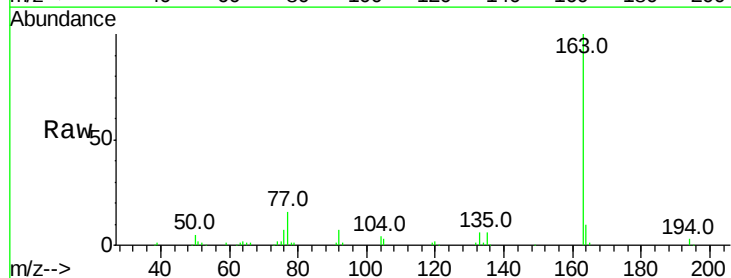


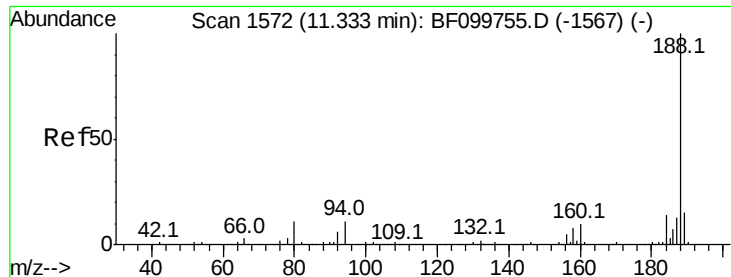

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.32 min Scan# 1569
Delta R.T. -0.02 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39




Instrument :
BNA_F
ClientSampleId :
EPE-P-5A(10-12)


Tot Ion	Ratio	Lower	Upper
188	100		
94	9.8	8.5	12.7
80	10.1	9.2	13.8

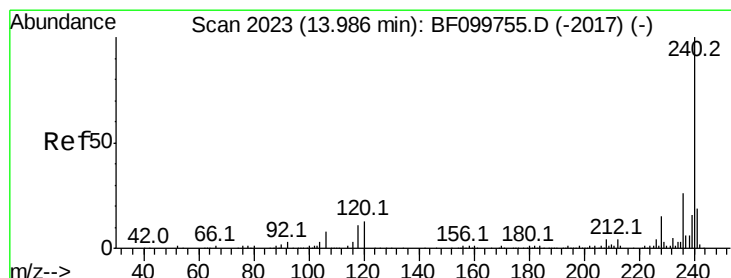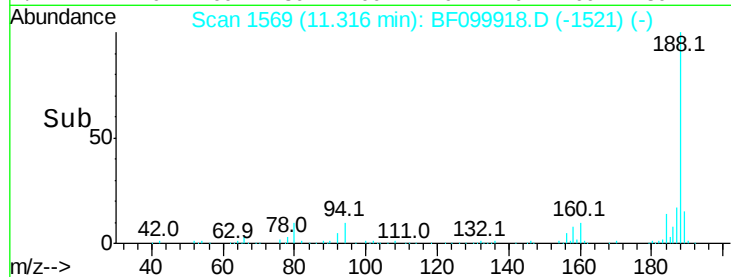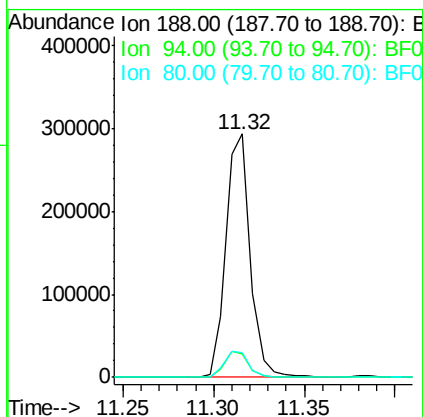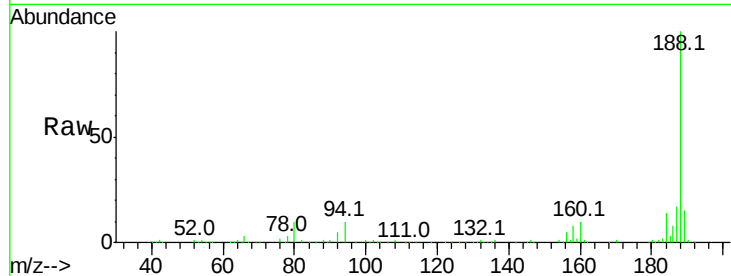

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.96 min Scan# 2019
Delta R.T. -0.03 min
Lab File: BF099918.D
Acq: 28 Oct 2017 15:39

Tgt Ion	Ratio	Lower	Upper
240	100		
120	13.2	9.5	14.3
236	25.2	20.7	31.1

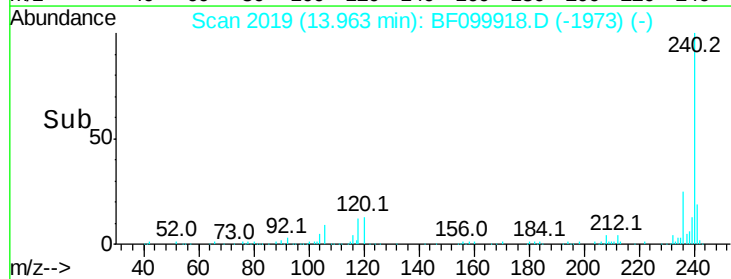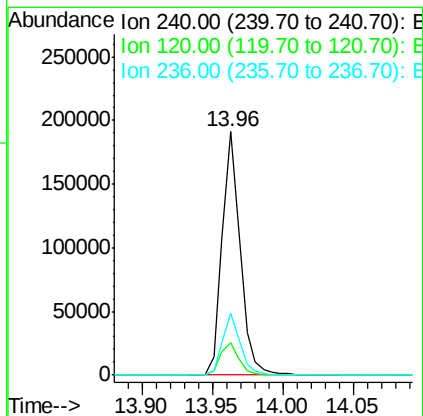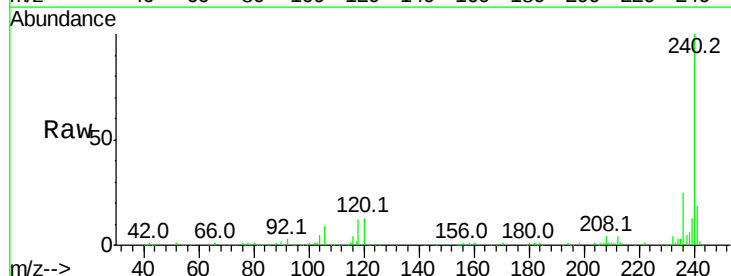

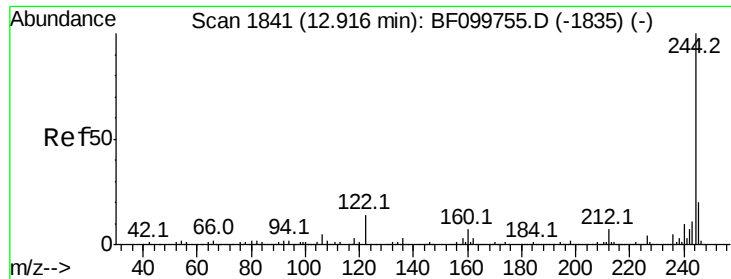

#78

Terphenyl-d14

Concen: 71.072 ng

RT: 12.90 min Scan# 1838

Delta R.T. -0.02 min

Lab File: BF099918.D

Acq: 28 Oct 2017 15:39

Instrument :

BNA_F

ClientSampleId :

EPE-P-5A(10-12)


Tot Ion:244 Resp: 556873

Ion Ratio Lower Upper

244 100

212 6.5 5.4 8.0




122 11.8 11.0 16.4

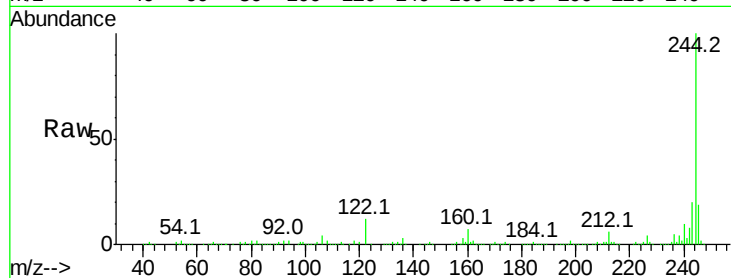

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

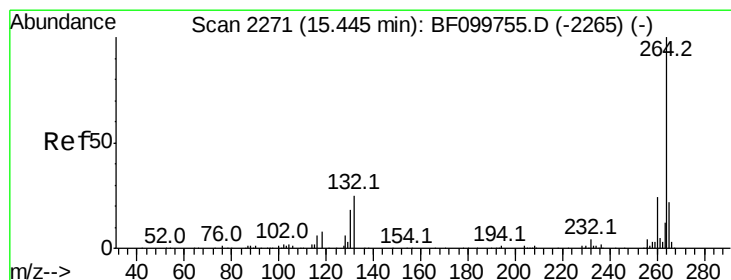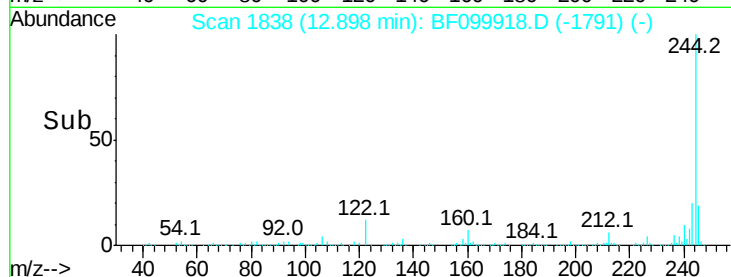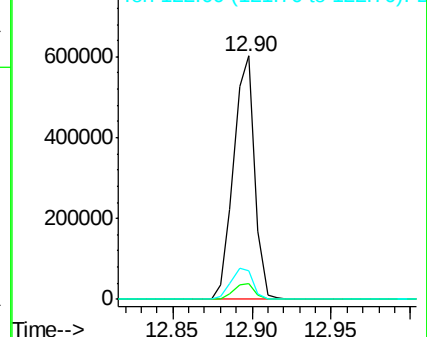

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.43 min Scan# 2268

Delta R.T. -0.03 min

Lab File: BF099918.D

Acq: 28 Oct 2017 15:39


Tgt Ion:264 Resp: 174319

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 21.1 17.5 26.3

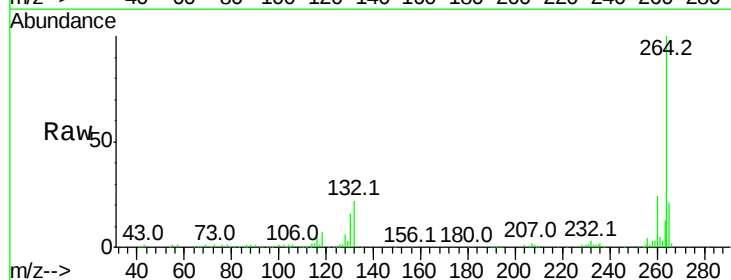

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

