


Data Path : Z:\HPCHEM1\BNA F\Data\BF102817\
 Data File : BF099909.D
 Acq On : 28 Oct 2017 11:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

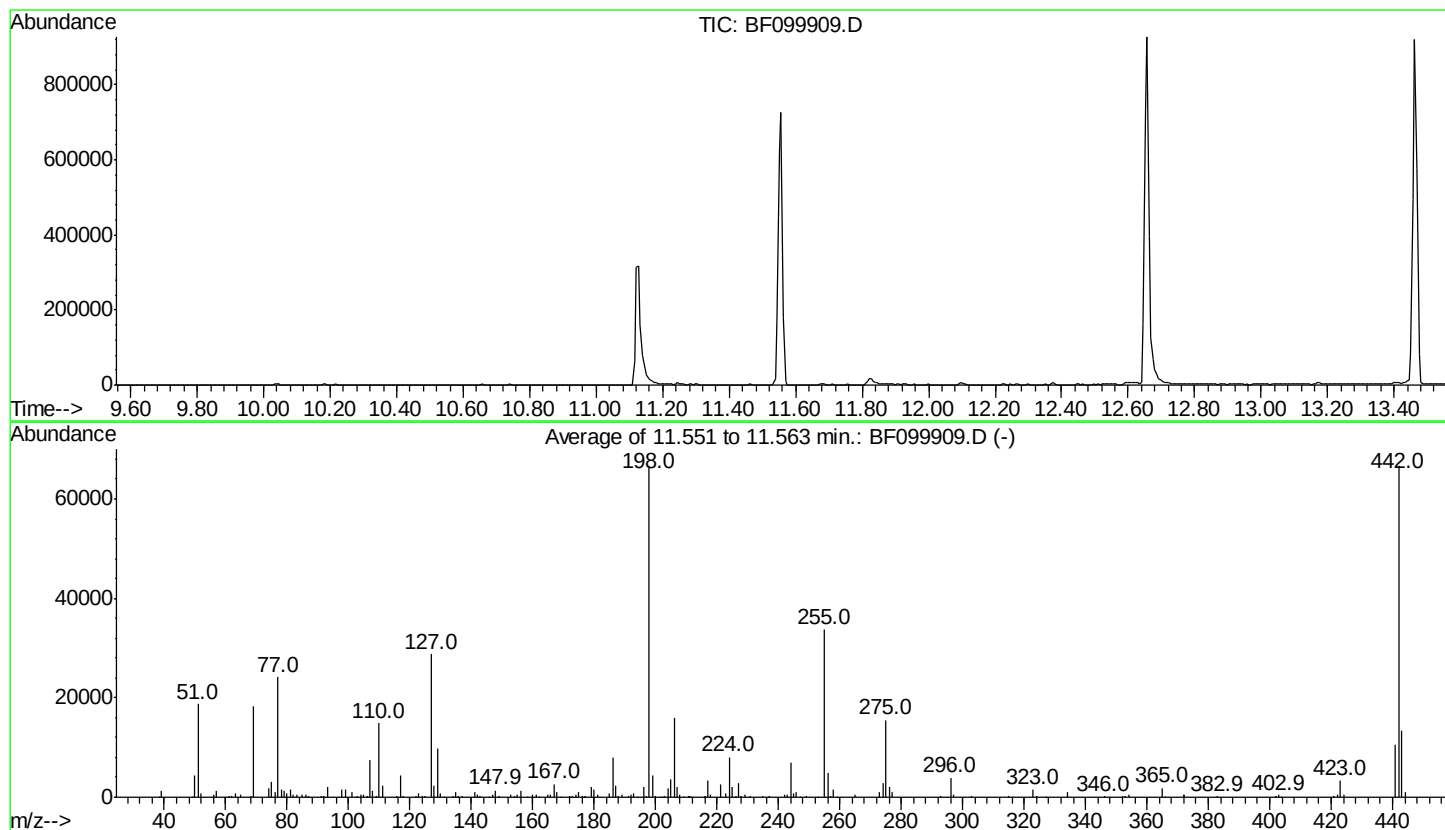

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	18792	PASS
68	69	0.00	2	1.8	324	PASS
69	198	0.00	100	27.4	18308	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	28821	PASS
197	198	0.00	2	0.5	366	PASS
198	198	100	100	100.0	66698	PASS
199	198	5	9	6.8	4504	PASS
275	198	10	60	23.3	15555	PASS
365	198	1	100	2.8	1853	PASS
441	443	0.01	100	78.5	10470	PASS
442	198	50	100	99.8	66594	PASS
443	442	15	24	20.0	13339	PASS