


Data Path : Z:\HPCHEM1\BNA F\Data\BF102817\
 Data File : BF099935.D
 Acq On : 29 Oct 2017 00:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 27 15:58:57 2017

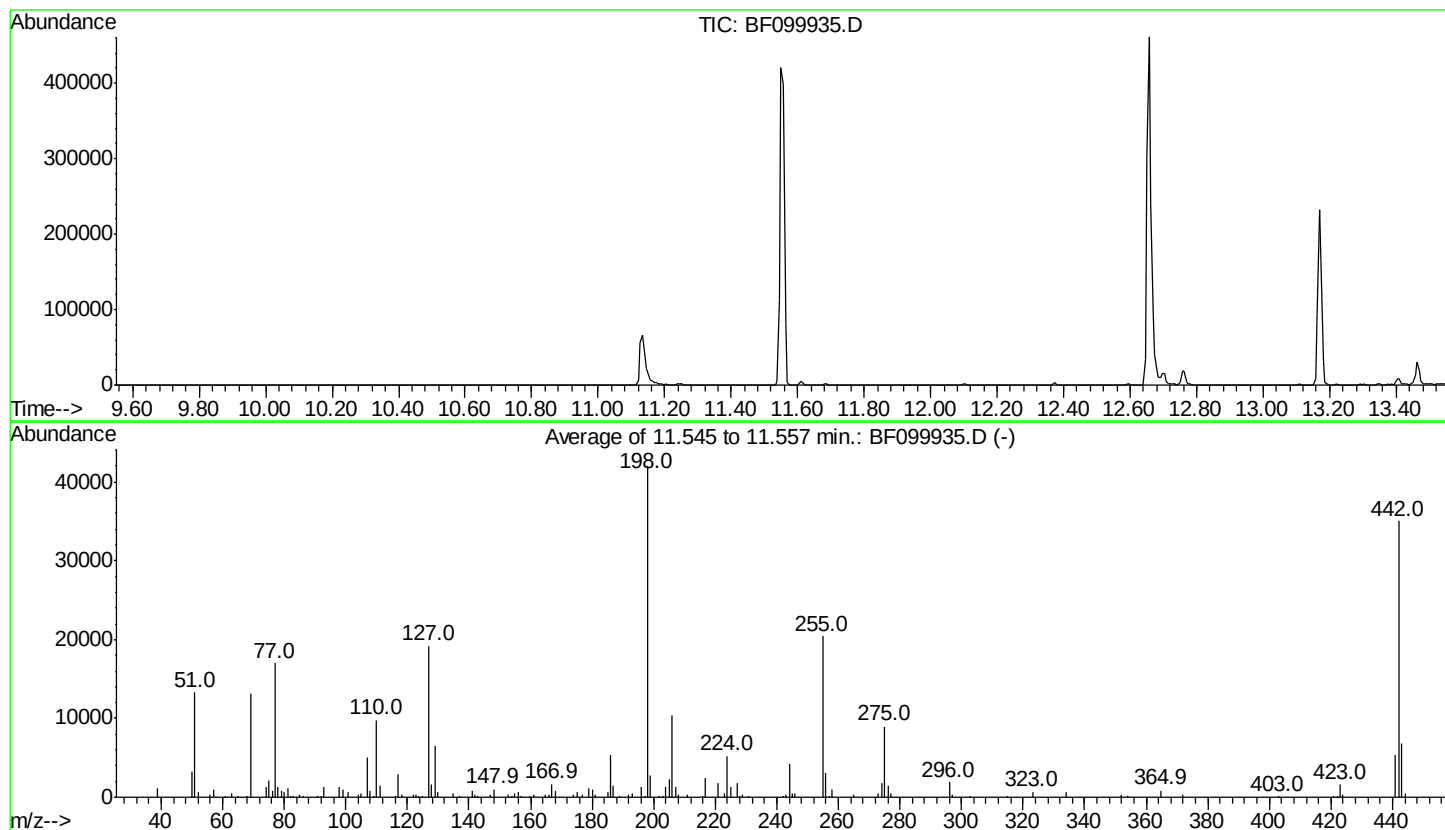

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	13267	PASS
68	69	0.00	2	0.8	109	PASS
69	198	0.00	100	31.3	13171	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	19212	PASS
197	198	0.00	2	0.5	219	PASS
198	198	100	100	100.0	42074	PASS
199	198	5	9	6.7	2805	PASS
275	198	10	60	21.3	8953	PASS
365	198	1	100	2.1	888	PASS
441	443	0.01	100	78.2	5387	PASS
442	198	50	100	83.3	35057	PASS
443	442	15	24	19.6	6887	PASS