

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102819\
 Data File : BF117557.D
 Acq On : 28 Oct 2019 13:23
 Operator : JU
 Sample : K5502-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 180-34-(0-2.1)

Quant Time: Oct 29 15:24:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	41113	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	167425	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	85631	20.00	ng	-0.01
64) Phenanthrene-d10	11.24	188	139353	20.00	ng	0.00
76) Chrysene-d12	13.89	240	88661	20.00	ng	0.00
87) Perylene-d12	15.33	264	72193	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	231566	83.79	ng	0.00
7) Phenol-d6	6.38	99	334637	90.16	ng	0.00
23) Nitrobenzene-d5	7.29	82	201984	59.56	ng	-0.01
42) 2,4,6-Tribromophenol	10.56	330	61575	83.11	ng	0.00
45) 2-Fluorobiphenyl	9.08	172	304543	50.11	ng	-0.01
79) Terphenyl-d14	12.83	244	267731	49.26	ng	0.00
Target Compounds						
10) Phenol	6.39	94	8237	2.174	ng	89
50) Dimethylphthalate	9.48	163	43075	7.056	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102819\
Data File : BF117557.D
Acq On : 28 Oct 2019 13:23
Operator : JU
Sample : K5502-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
180-34-(0-2.1)

Quant Time: Oct 29 15:24:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

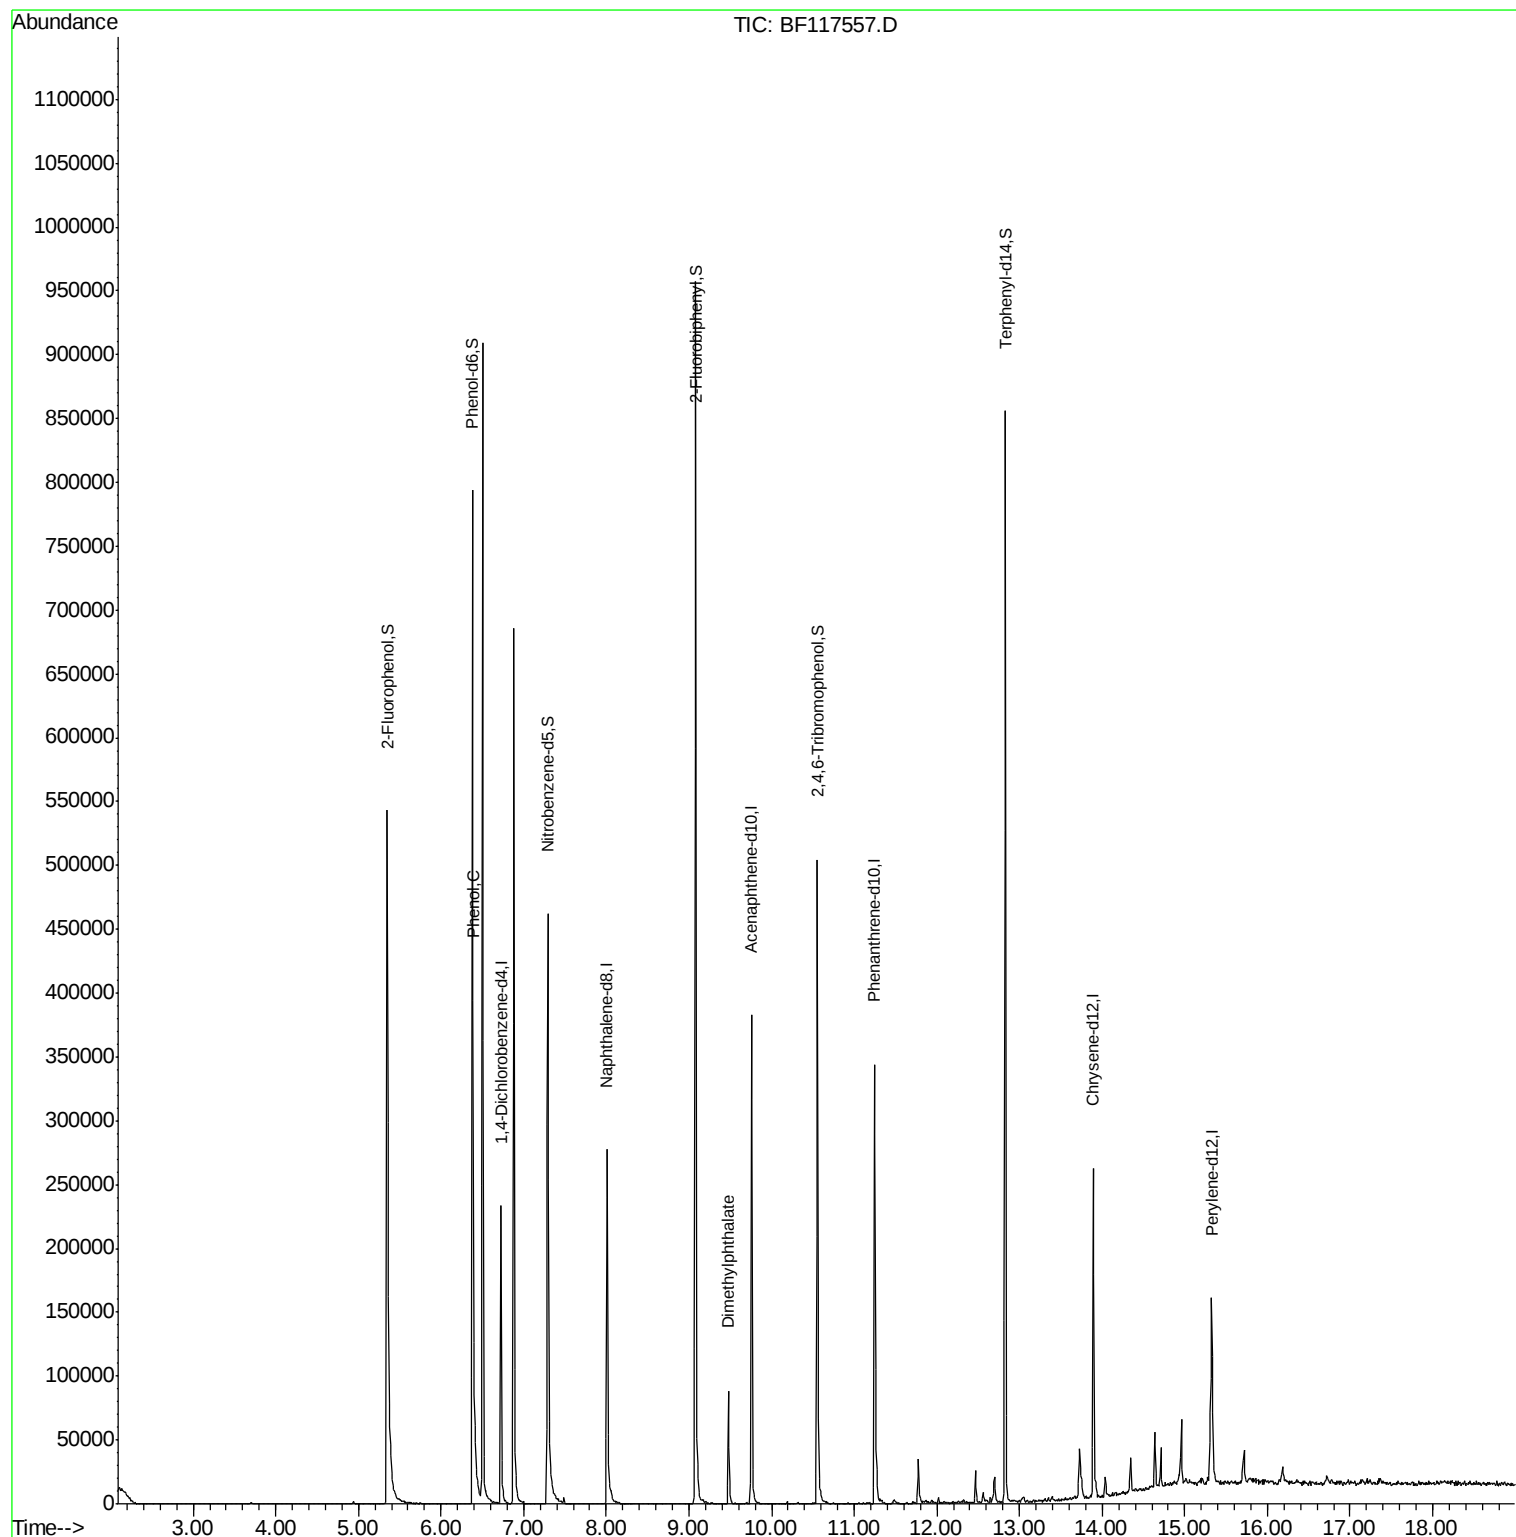

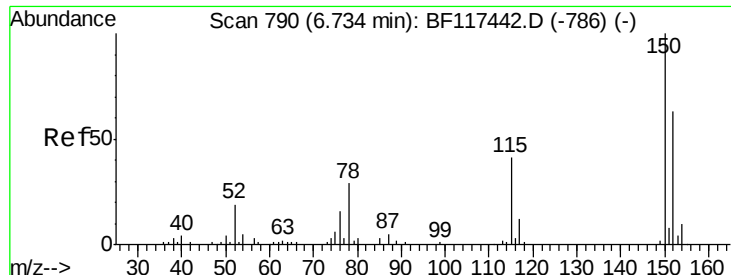


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23

Instrument :
BNA_F
ClientSampleId :
180-34-(0-2.1)

Tot Ion:152 Resp: 41113
Ion Ratio Lower Upper
152 100
150 160.8 126.8 190.2
115 63.9 51.6 77.4

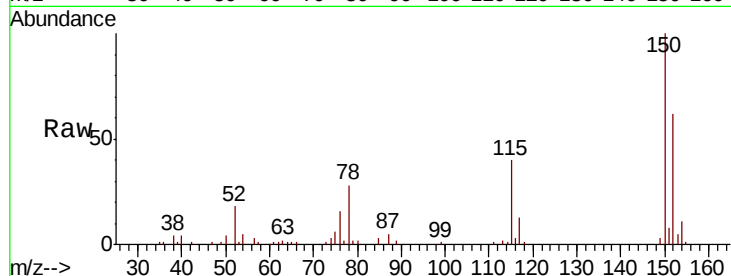


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

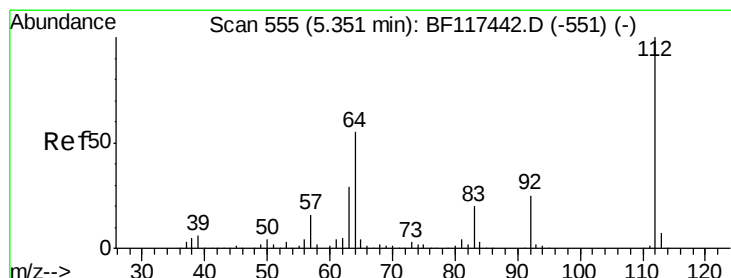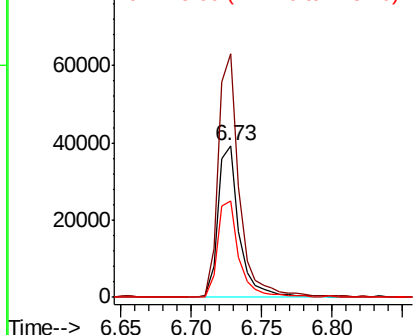



#5


2-Fluorophenol
Concen: 83.794 ng
RT: 5.35 min Scan# 555
Delta R.T. -0.00 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23

Tgt Ion:112 Resp: 231566
Ion Ratio Lower Upper
112 100
64 54.1 44.1 66.1
63 28.9 23.4 35.2

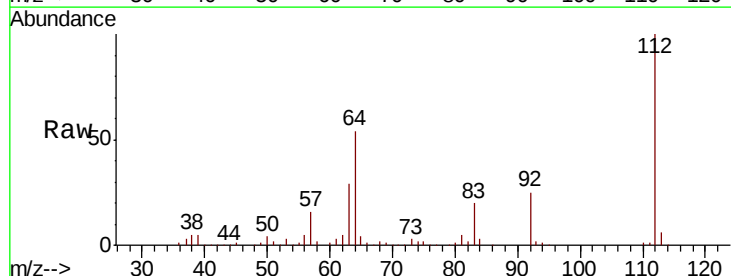

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

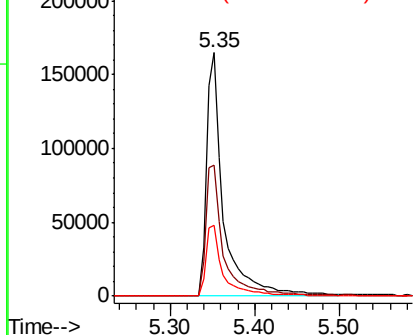

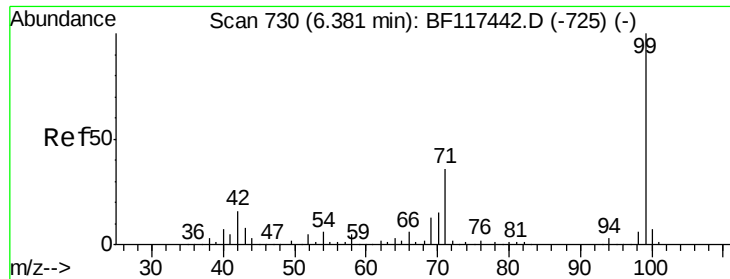

#7

Phenol-d6

Concen: 90.157 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.00 min

Lab File: BF117557.D

Acq: 28 Oct 2019 13:23

Instrument :

BNA_F

ClientSampleId :

180-34-(0-2.1)


Tot Ion: 99 Resp: 334637

Ion Ratio Lower Upper




99 100

42 15.0 12.8 19.2

71 35.1 28.6 43.0

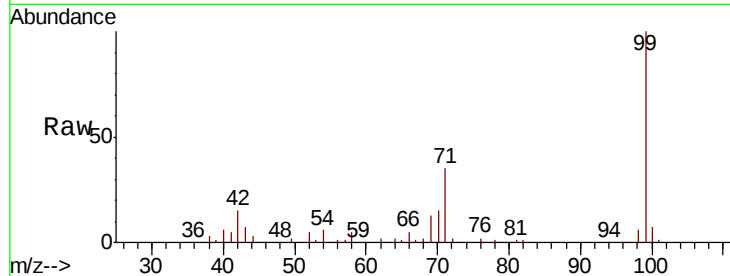

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

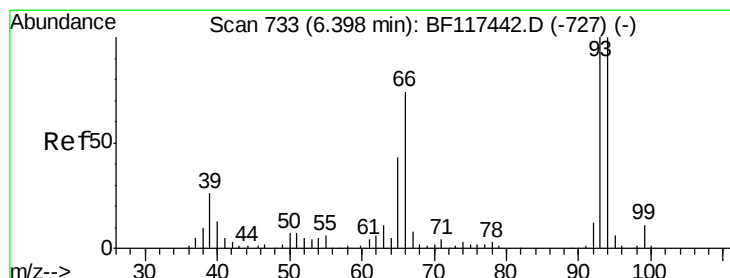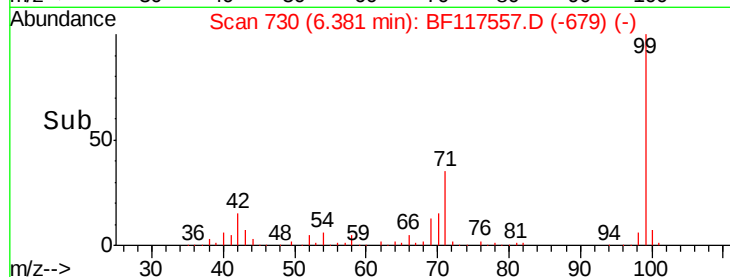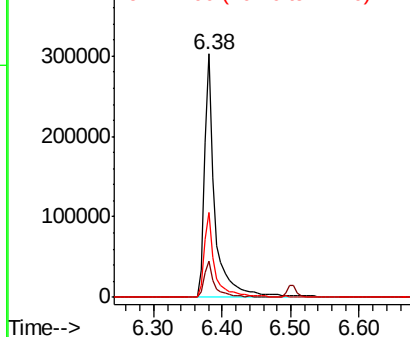

#10

Phenol

Concen: 2.174 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.01 min

Lab File: BF117557.D

Acq: 28 Oct 2019 13:23


Tgt Ion: 94 Resp: 8237

Ion Ratio Lower Upper



94 100


65 42.4 23.4 63.4

66 89.1 54.7 94.7

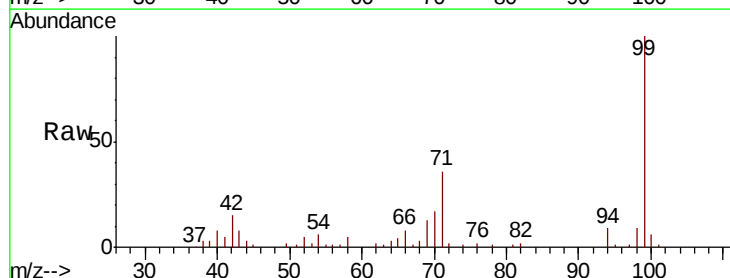

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



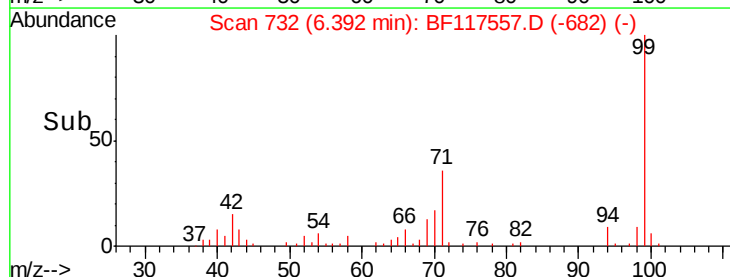
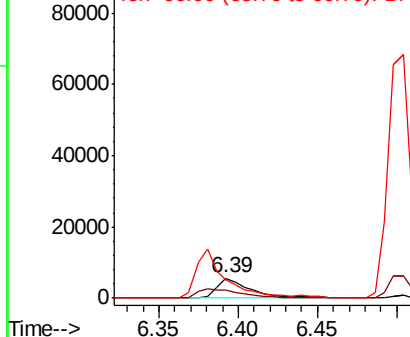


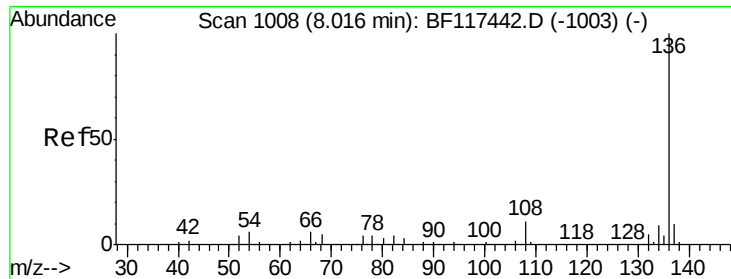

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.01 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23




Instrument :
BNA_F
ClientSampleId :
180-34-(0-2.1)


Tot Ion:136	Resp:	167425
Ion	Ratio	Lower Upper
136	100	
137	11.0	8.2 12.4
54	5.7	4.5 6.7
68	5.2	4.3 6.5

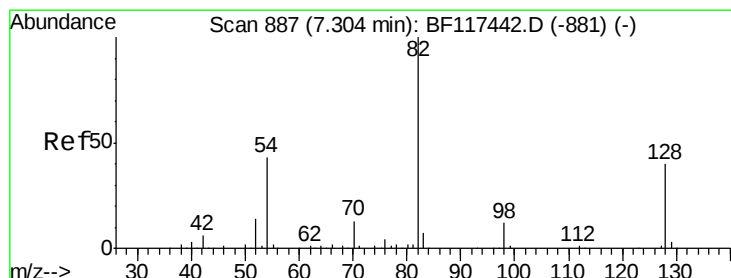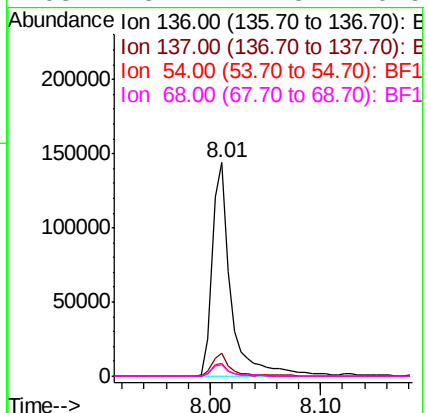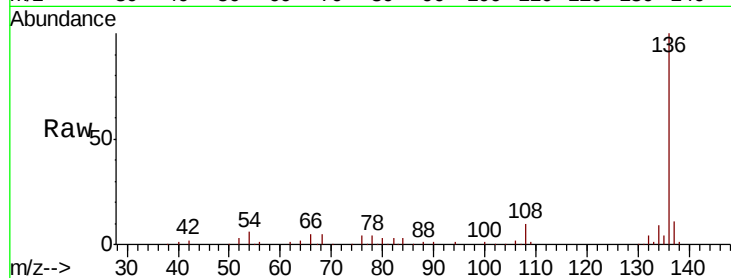

#23
Nitrobenzene-d5
Concen: 59.558 ng
RT: 7.29 min Scan# 885
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23

Tgt Ion: 82	Resp:	201984
Ion	Ratio	Lower Upper
82	100	
128	42.6	32.2 48.2
54	42.1	34.2 51.2

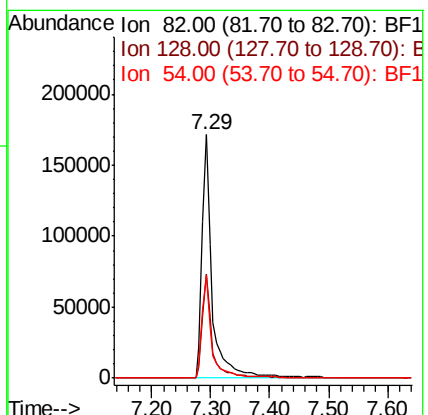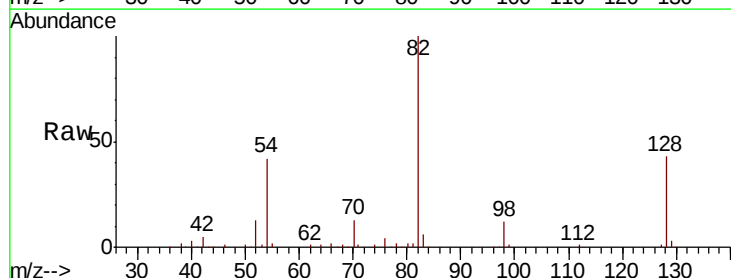







#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.76 min Scan# 1304
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23

Instrument :
BNA_F
ClientSampleId :
180-34-(0-2.1)

Tot Ion:164 Resp: 85631
Ion Ratio Lower Upper
164 100
162 99.4 81.8 122.6
160 41.2 34.4 51.6

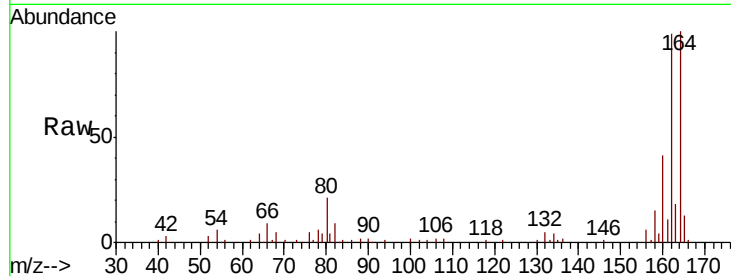


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

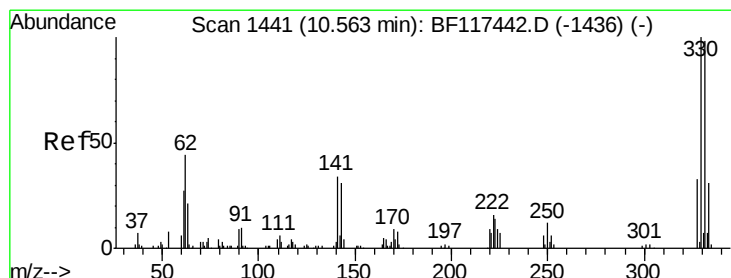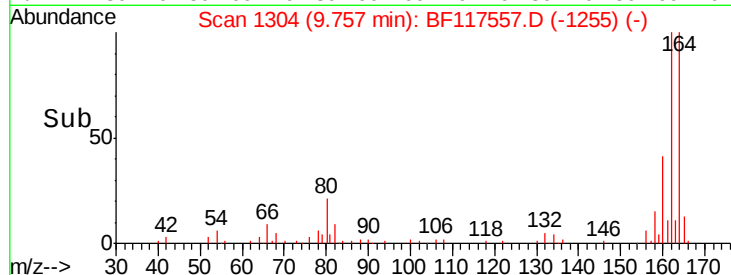
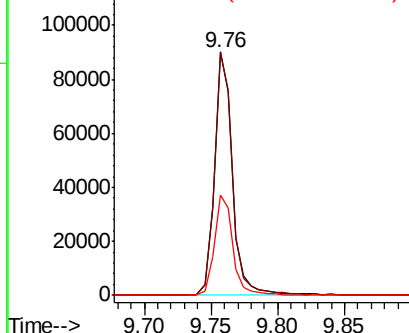


#42
2,4,6-Tribromophenol
Concen: 83.105 ng
RT: 10.56 min Scan# 1440
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23

Tgt Ion:330 Resp: 61575
Ion Ratio Lower Upper
330 100
332 94.8 78.5 117.7
141 43.7 37.0 55.6

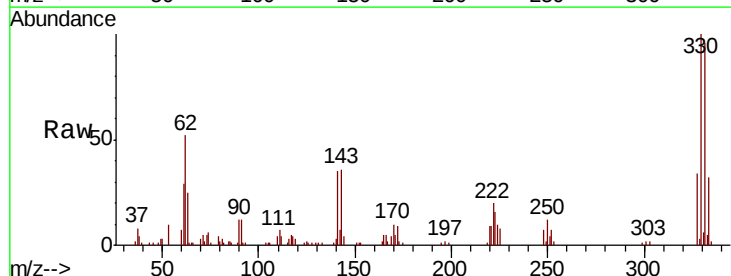

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




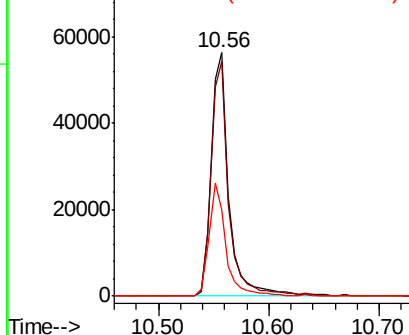




#45
2-Fluorobiphenyl
Concen: 50.110 ng
RT: 9.08 min Scan# 1189
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23




Instrument :
BNA_F
ClientSampleId :
180-34-(0-2.1)


Tot Ion:172 Resp: 304543
Ion Ratio Lower Upper
172 100
171 34.6 27.5 41.3
170 22.7 18.6 27.8

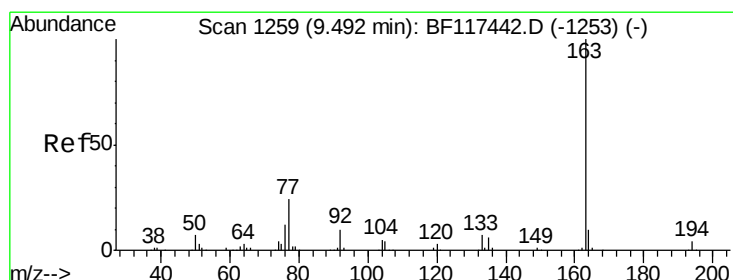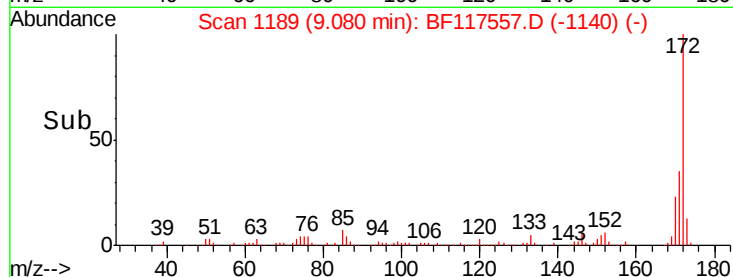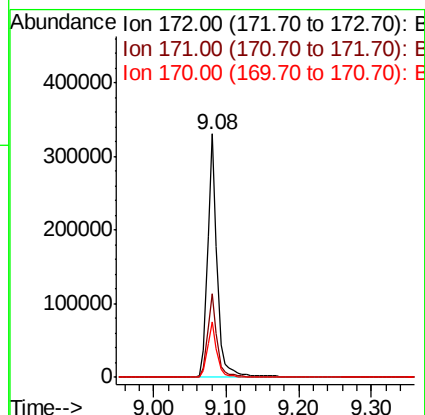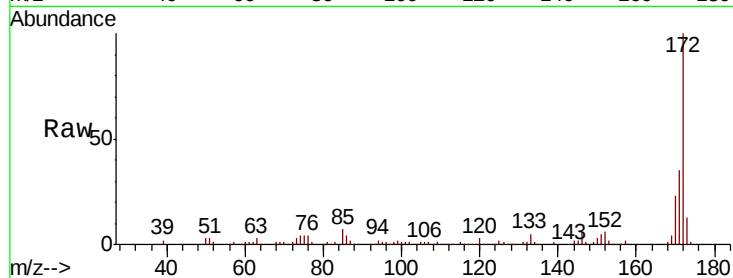

#50
Dimethylphthalate
Concen: 7.056 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.01 min
Lab File: BF117557.D
Acq: 28 Oct 2019 13:23

Tgt Ion:163 Resp: 43075
Ion Ratio Lower Upper
163 100
194 4.3 2.9 4.3#
164 9.9 8.2 12.2

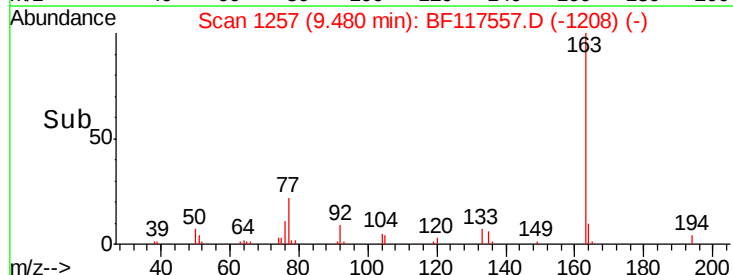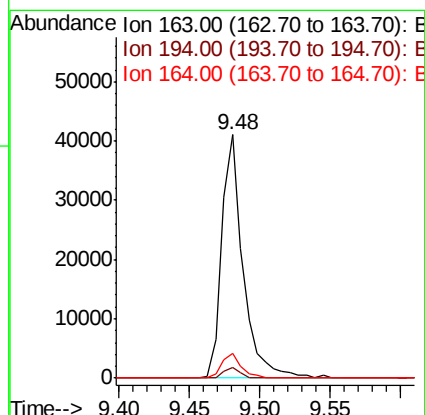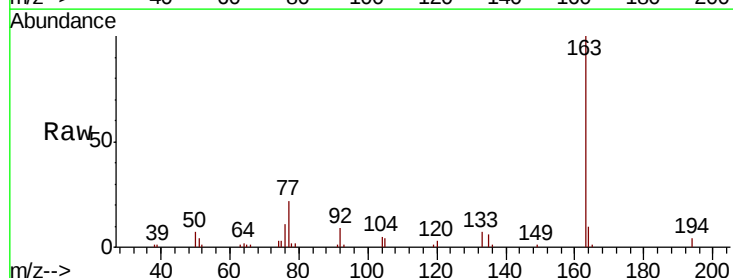



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.24 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF117557.D

Acq: 28 Oct 2019 13:23

Instrument :

BNA_F

ClientSampleId :

180-34-(0-2.1)


Tot Ion:188 Resp: 139353

Ion Ratio Lower Upper

188 100

94 9.9 8.0 12.0




80 12.0 9.5 14.3

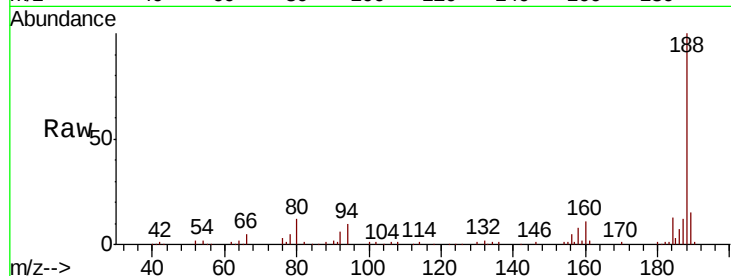

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

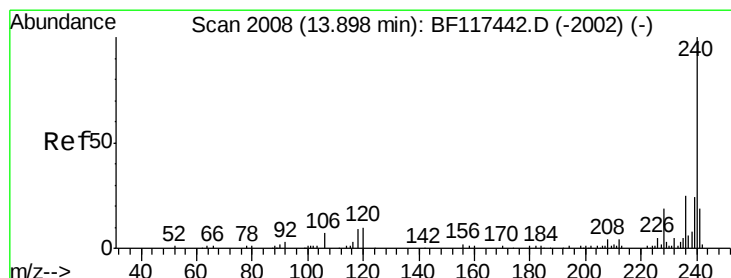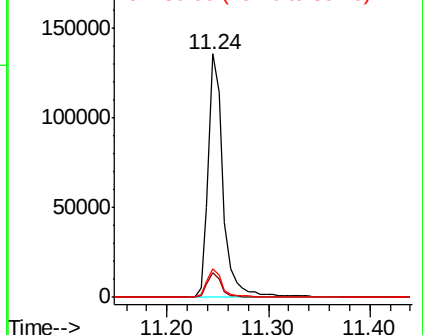

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.89 min Scan# 2007

Delta R.T. -0.01 min

Lab File: BF117557.D

Acq: 28 Oct 2019 13:23


Tgt Ion:240 Resp: 88661

Ion Ratio Lower Upper

240 100

120 12.9 8.4 12.6#



236 25.1 20.0 30.0

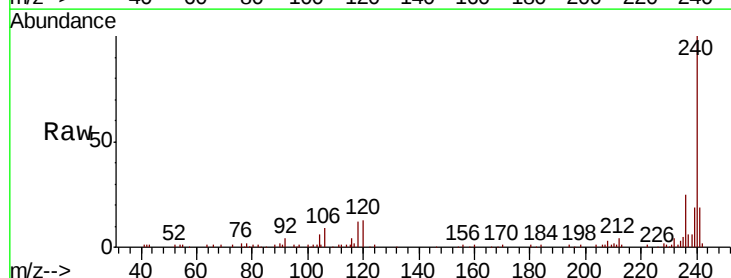


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



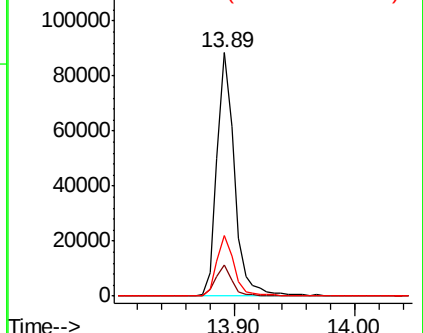





#79
 Terphenyl-d14
 Concen: 49.255 ng
 RT: 12.83 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BF117557.D
 Acq: 28 Oct 2019 13:23

Instrument :
 BNA_F
 ClientSampleId :
 180-34-(0-2.1)

Tot Ion	Ratio	Lower	Upper
244	100		
212	6.7	5.8	8.6
122	13.3	11.8	17.8

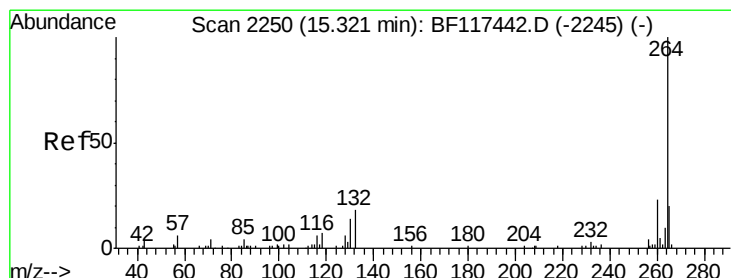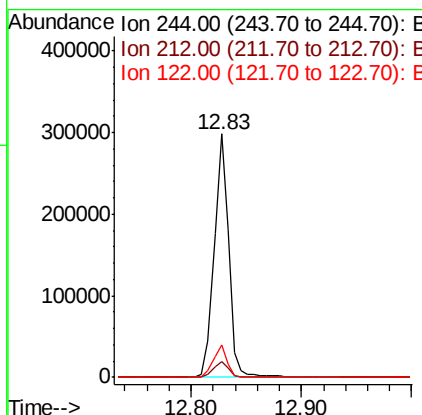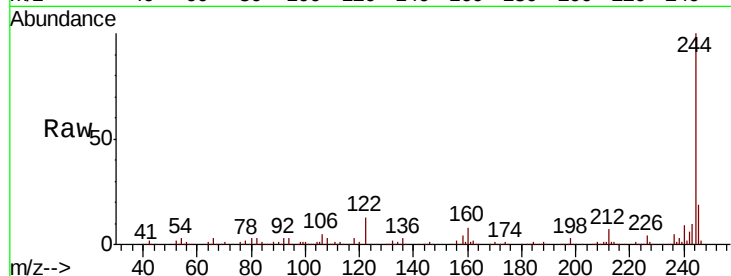

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.33 min Scan# 2251
 Delta R.T. 0.01 min
 Lab File: BF117557.D
 Acq: 28 Oct 2019 13:23

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.4	27.6
265	20.2	16.1	24.1

