
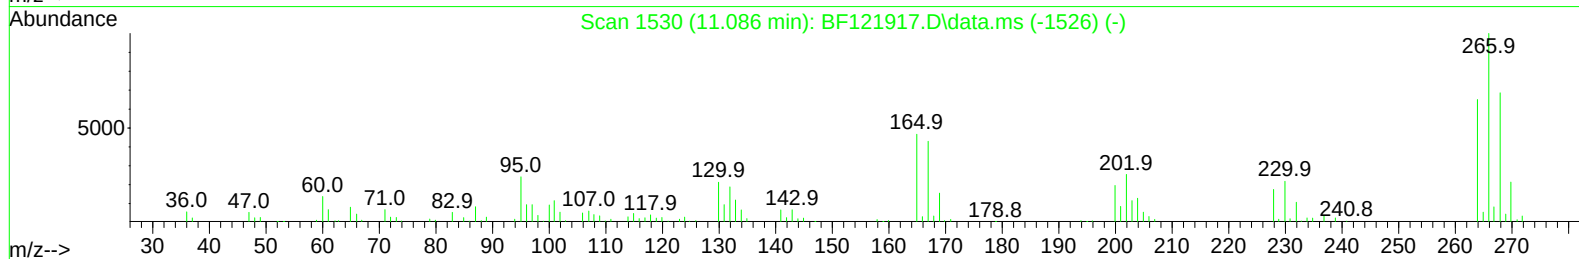
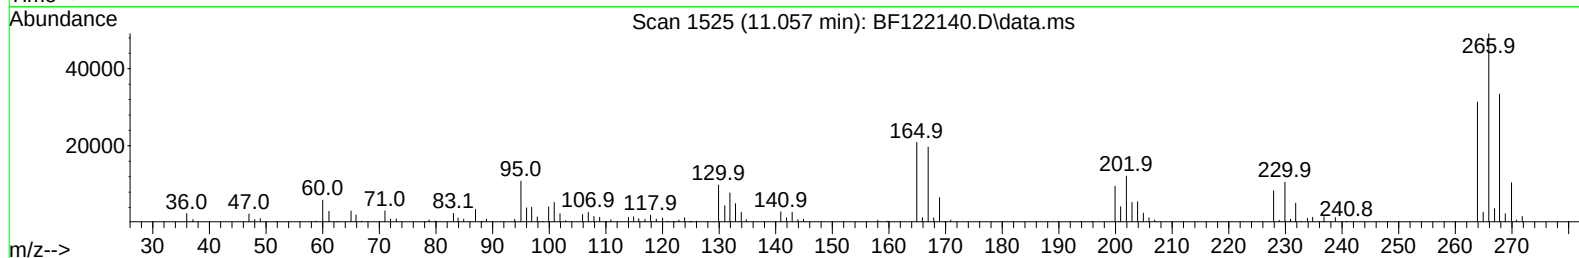


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102820\
Data File : BF122140.D
Acq On : 28 Oct 2020 9:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:53:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

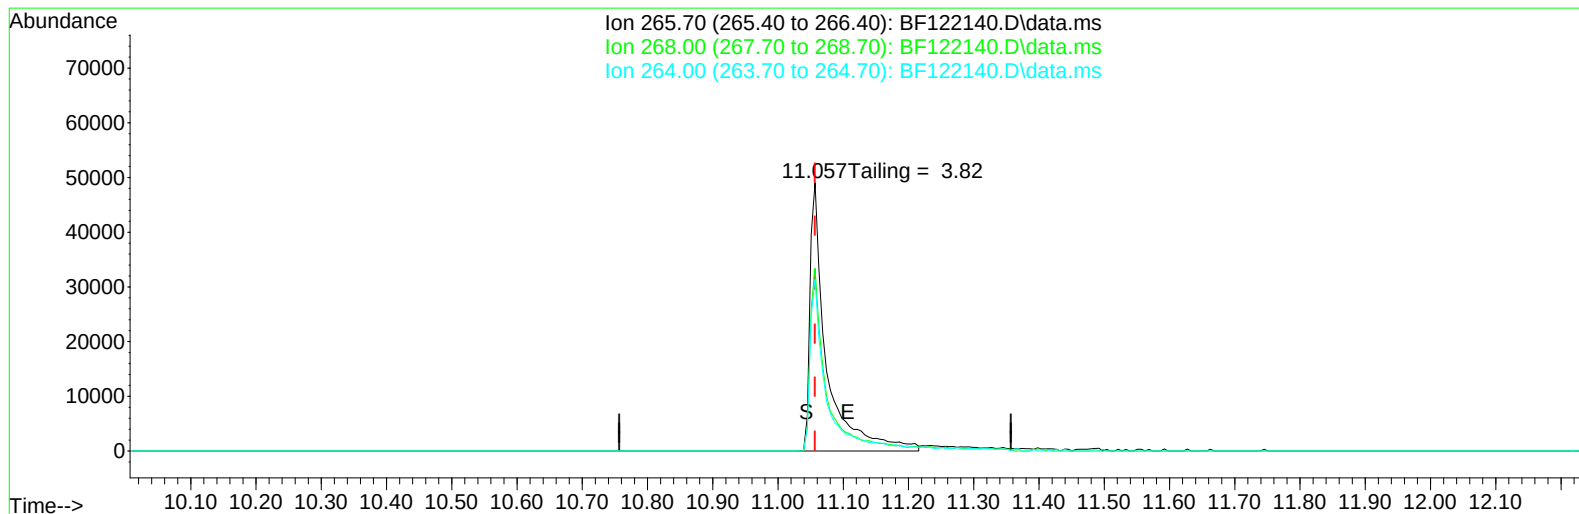

TIC: BF122140.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.000) 90439.65 ng

response 87758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	68.03
264.00	62.40	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102820\
Data File : BF122140.D
Acq On : 28 Oct 2020 9:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:53:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

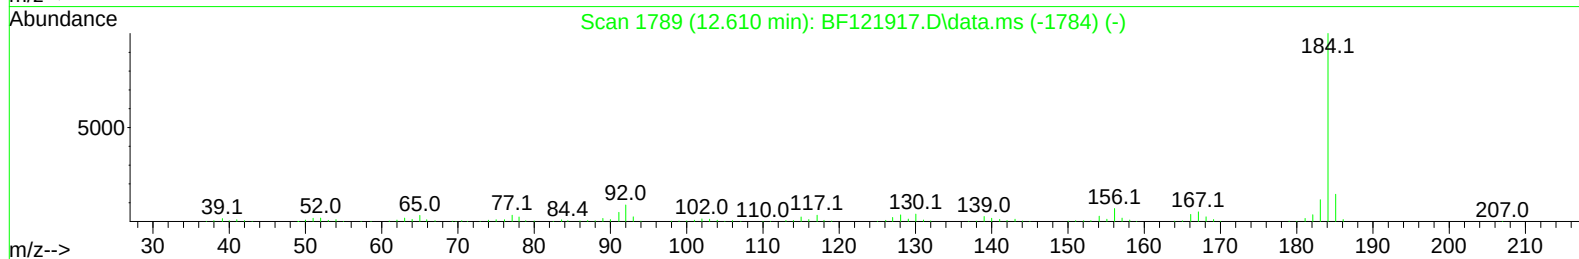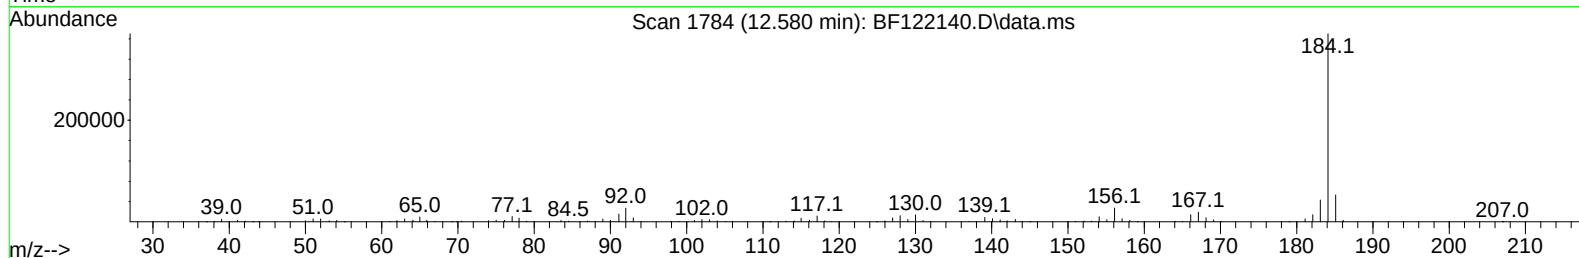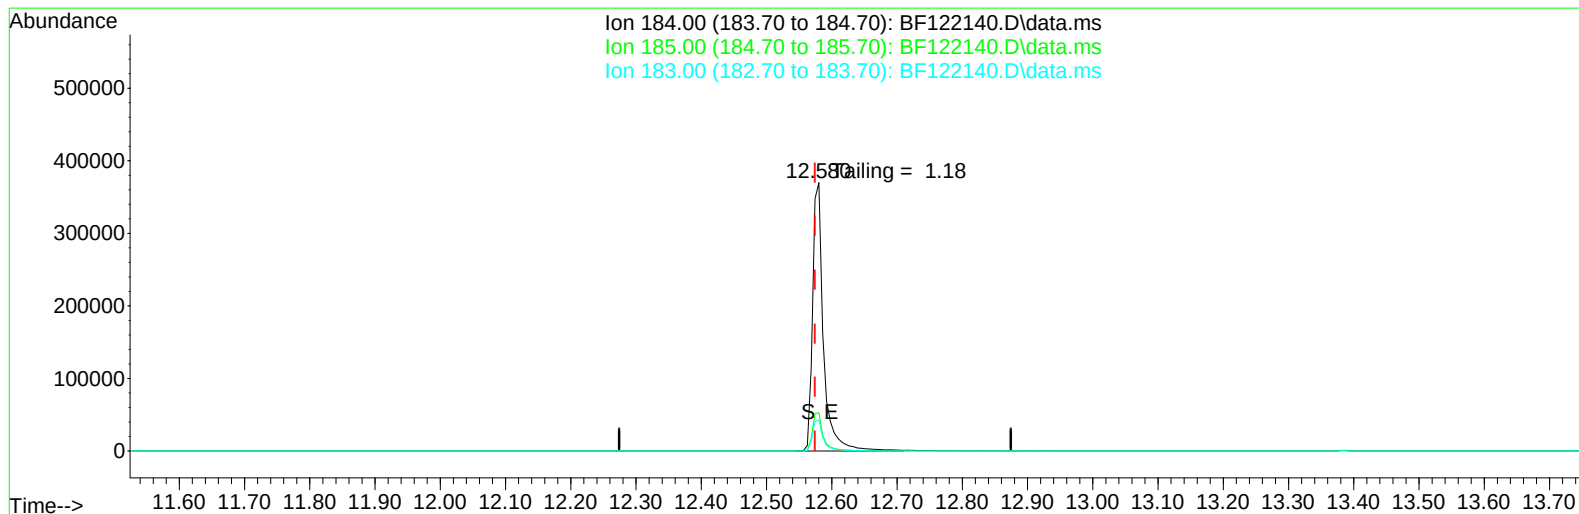

TIC: BF122140.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 0.00 ng

response 431422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.31
183.00	11.70	11.63
0.00	0.00	0.00