

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102820\
 Data File : BF122149.D
 Acq On : 28 Oct 2020 15:55
 Operator : JU/CG
 Sample : L4224-11 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-102720

Manual Integrations
 APPROVED

mohammad
 10/29/2020 10:44:57 AM

Quant Time: Oct 28 17:00:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 26 17:27:32 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.716	152	102469	20.00	ng	0.00
21) Naphthalene-d8	7.998	136	401800	20.00	ng	0.00
39) Acenaphthene-d10	9.745	164	198122	20.00	ng	0.00
64) Phenanthrene-d10	11.233	188	327413	20.00	ng	0.00
76) Chrysene-d12	13.880	240	227251	20.00	ng	0.00
86) Perylene-d12	15.316	264	238724	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	274739	39.57	ng	0.00
7) Phenol-d6	6.369	99	353667	39.57	ng	0.00
23) Nitrobenzene-d5	7.281	82	216891	27.68	ng	0.00
42) 2,4,6-Tribromophenol	10.545	330	80575	32.88	ng	0.00
45) 2-Fluorobiphenyl	9.069	172	391912	29.11	ng	0.00
79) Terphenyl-d14	12.816	244	292482	24.53	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	9.475	163	57741	3.99	ng	100
71) Phenanthrene	11.257	178	75306	4.19	ng	99
75) Fluoranthene	12.451	202	126361	6.56	ng	97
78) Pyrene	12.680	202	116414	6.72	ng	99
81) Benzo(a)anthracene	13.869	228	61748	4.15	ng	98
83) Chrysene	13.904	228	57514	3.93	ng	98
88) Benzo(b)fluoranthene	14.910	252	76330m	4.73	ng	
90) Benzo(a)pyrene	15.257	252	52740	3.78	ng	# 96
92) Benzo(g,h,i)perylene	17.157	276	32179	2.52	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102820\
Data File : BF122149.D
Acq On : 28 Oct 2020 15:55
Operator : JU/CG
Sample : L4224-11 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-102720

Manual Integrations
APPROVED

mohammad
10/29/2020 10:44:57 AM

Quant Time: Oct 28 17:00:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

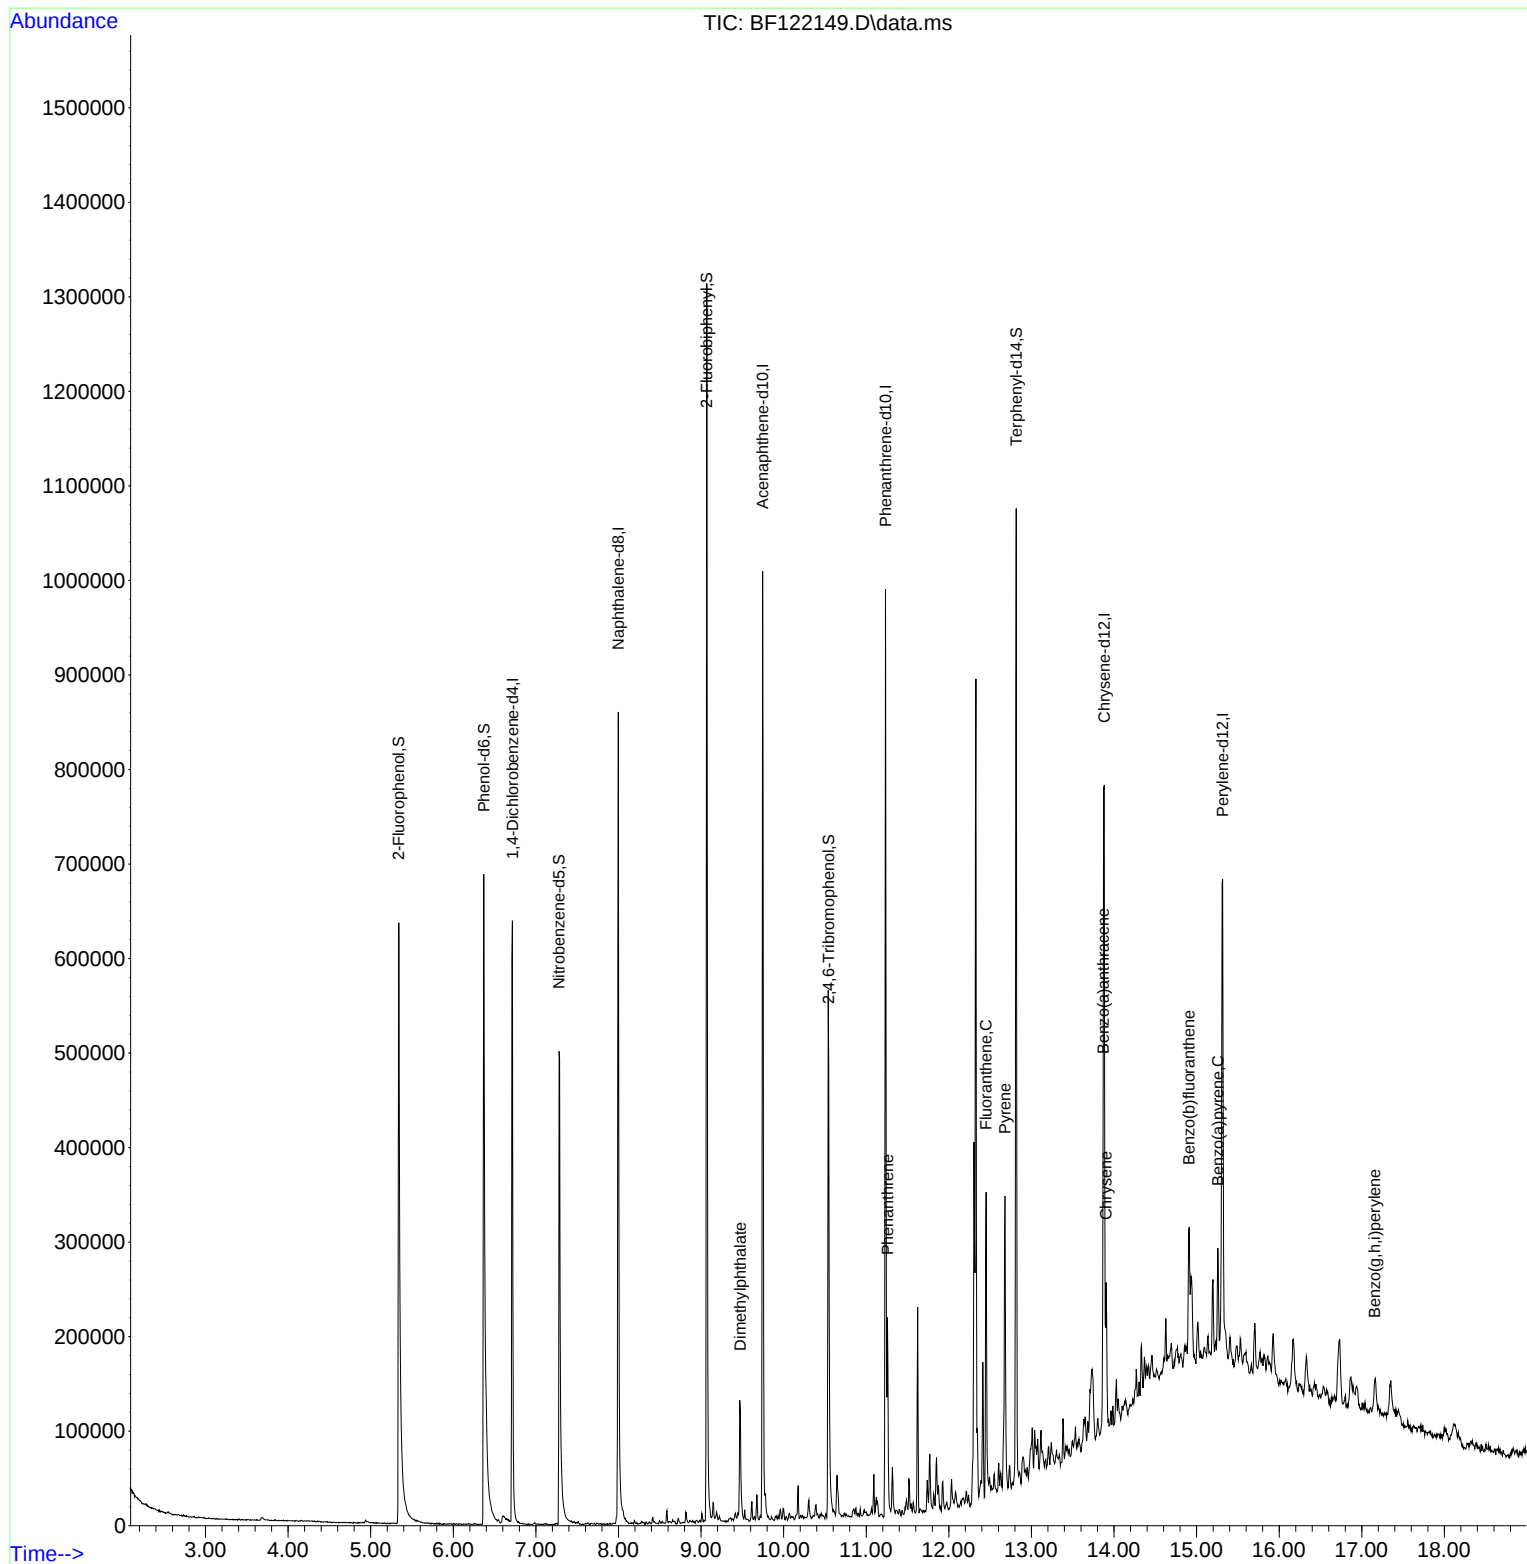







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.716 min Scan# 787
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:152 Resp: 102469
Ion Ratio Lower Upper
152 100
150 157.0 125.3 187.9
115 60.9 51.9 77.9

Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Manual Integrations
APPROVED

mohammad
10/29/2020 10:44:57 AM

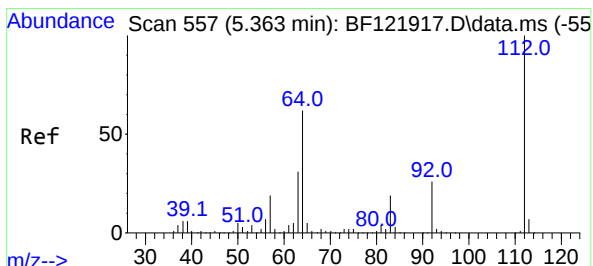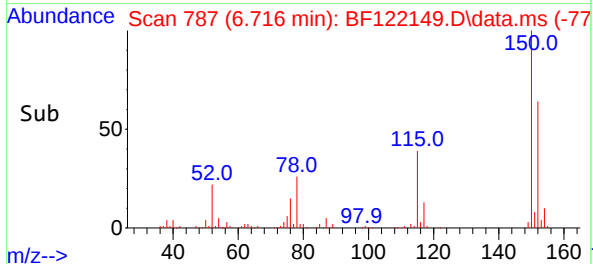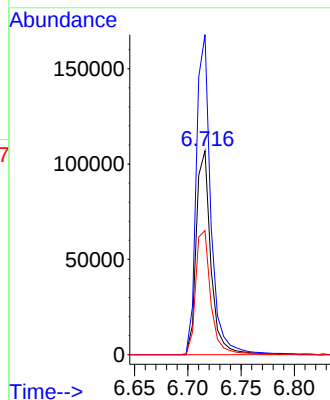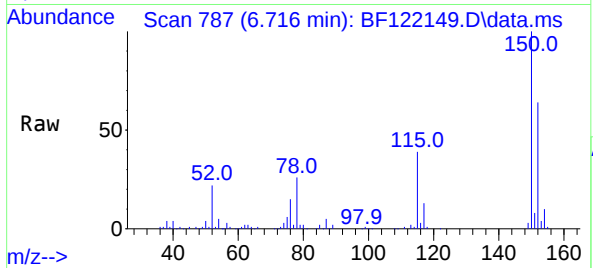

#5
2-Fluorophenol
Concen: 39.57 ng
RT: 5.340 min Scan# 553
Delta R.T. 0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:112 Resp: 274739
Ion Ratio Lower Upper
112 100
64 63.1 50.4 75.6
63 31.8 25.8 38.6

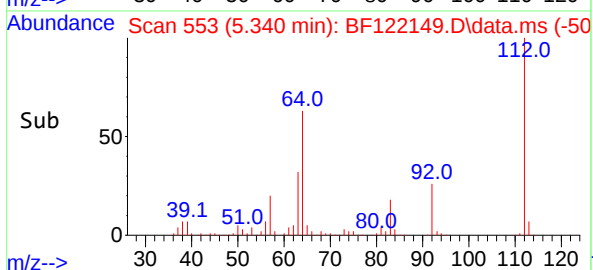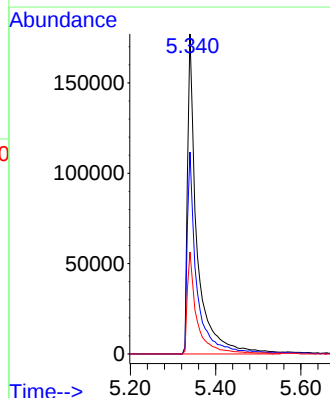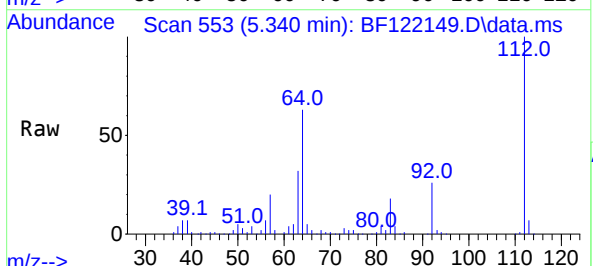







#7
Phenol-d6
Concen: 39.57 ng
RT: 6.369 min Scan# 728
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion: 99 Resp: 353667
Ion Ratio Lower Upper
99 100
42 19.7 15.9 23.9
71 34.1 27.1 40.7

Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Manual Integrations
APPROVED


mohammad
10/29/2020 10:44:57 AM

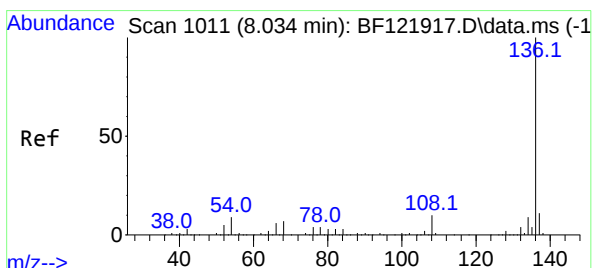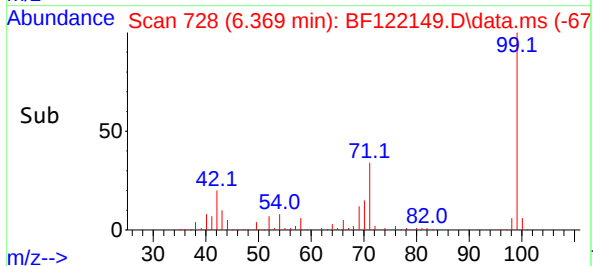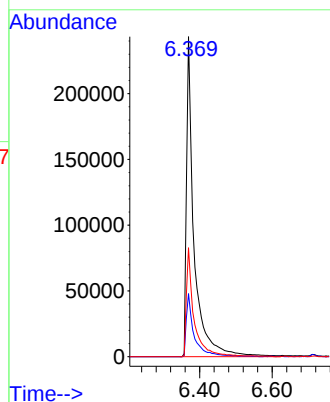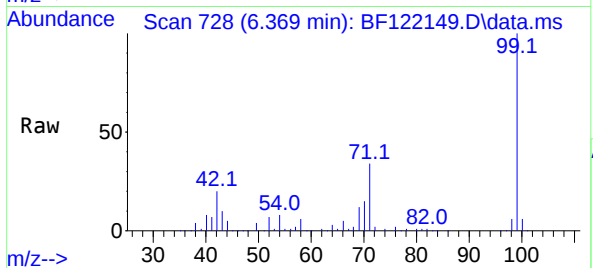

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.998 min Scan# 1005
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion: 136 Resp: 401800
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 9.0 7.1 10.7
68 6.3 5.0 7.4

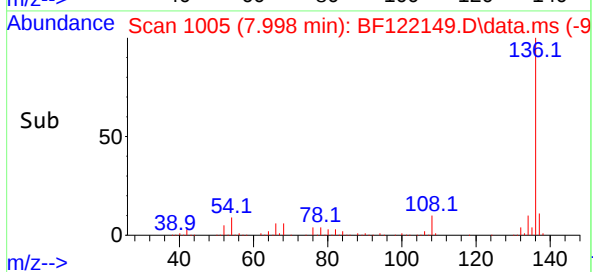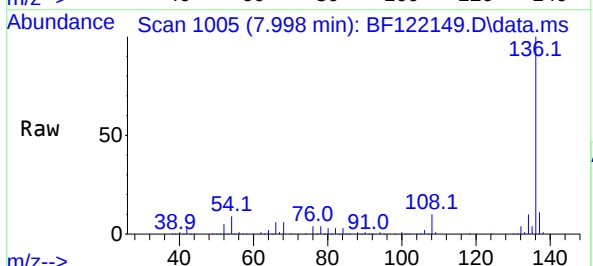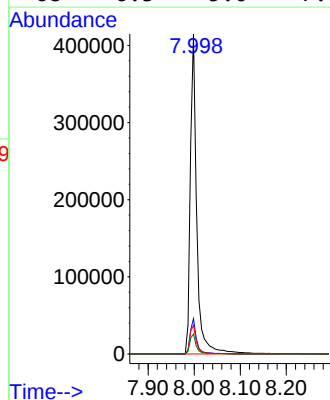

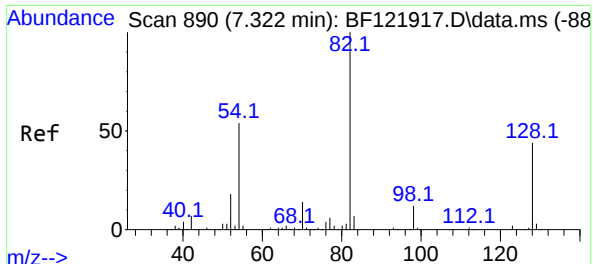

#23
Nitrobenzene-d5
Concen: 27.68 ng
RT: 7.281 min Scan# 883
Delta R.T. -0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55





Tgt Ion: 82 Resp: 216891

Ion	Ratio	Lower	Upper
82	100		
128	37.9	35.0	52.4
54	56.0	43.9	65.9

Instrument :
BNA_F
ClientSampleId :
OR-02-102720

Manual Integrations
APPROVED




mohammad
10/29/2020 10:44:57 AM

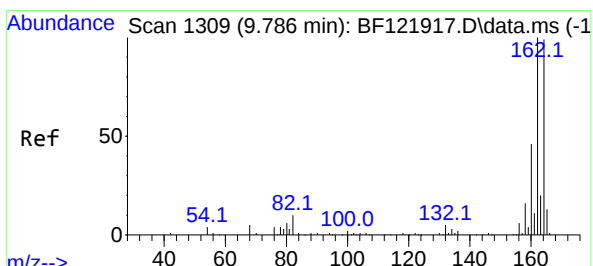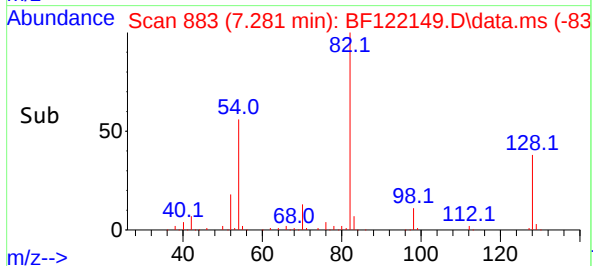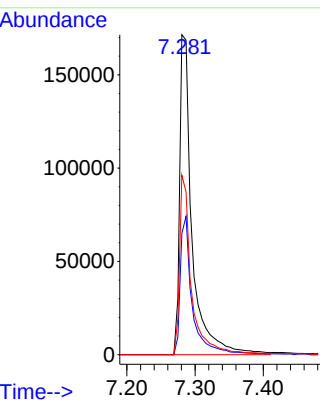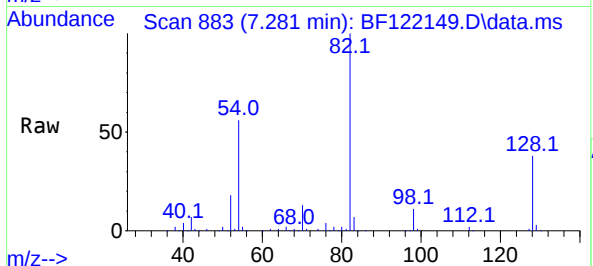

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.745 min Scan# 1302
Delta R.T. -0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion: 164 Resp: 198122


Ion	Ratio	Lower	Upper
164	100		
162	103.2	83.2	124.8
160	46.2	37.5	56.3

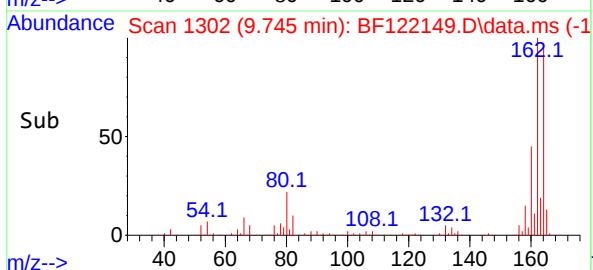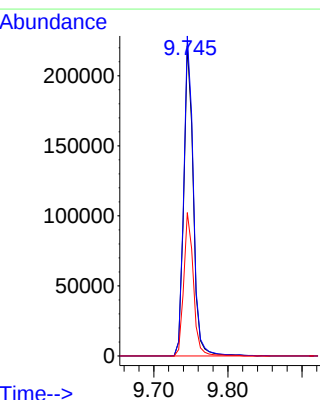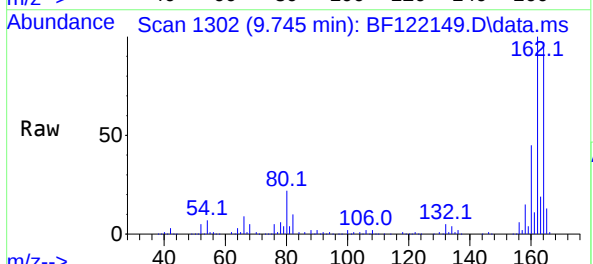



#42
2,4,6-Tribromophenol
Concen: 32.88 ng
RT: 10.545 min Scan# 1438
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55




Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Tgt Ion: 330 Resp: 80575
Ion Ratio Lower Upper
330 100
332 97.4 77.3 115.9
141 32.9 22.3 33.5

Manual Integrations
APPROVED



mohammad
10/29/2020 10:44:57 AM

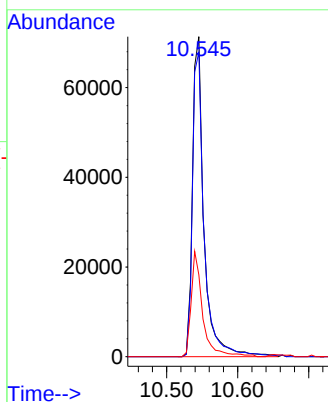

#45
2-Fluorobiphenyl
Concen: 29.11 ng
RT: 9.069 min Scan# 1187
Delta R.T. -0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55



Tgt Ion: 172 Resp: 391912
Ion Ratio Lower Upper
172 100
171 35.1 29.1 43.7
170 23.1 19.8 29.6

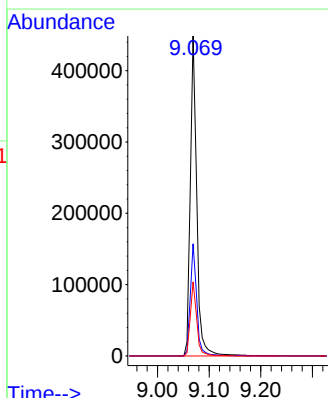







#50
Dimethylphthalate
Concen: 3.99 ng
RT: 9.475 min Scan# 1256
Delta R.T. -0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:163	Resp:	57741
Ion Ratio	Lower	Upper
163	100	
194	4.1	3.3 4.9
164	10.2	8.2 12.4

Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Manual Integrations
APPROVED


mohammad
10/29/2020 10:44:57 AM

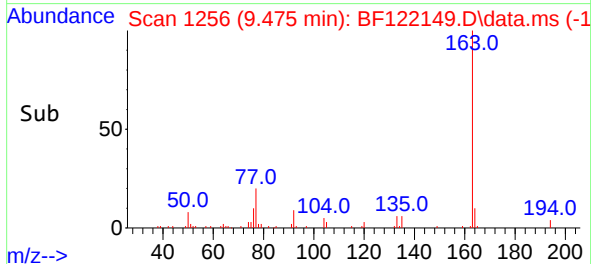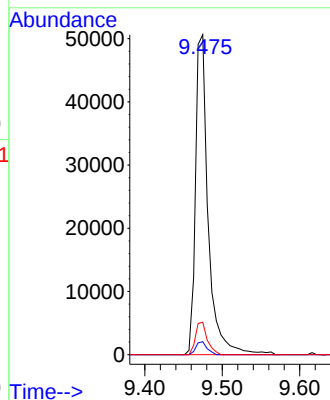

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.233 min Scan# 1555
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55


Tgt Ion:188	Resp:	327413
Ion Ratio	Lower	Upper
188	100	
94	10.2	8.3 12.5
80	10.6	9.1 13.7

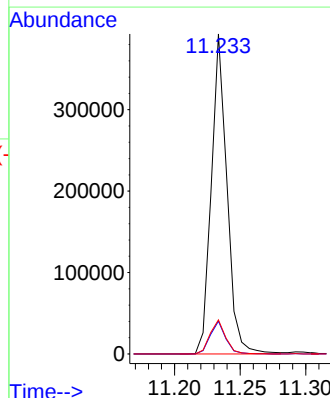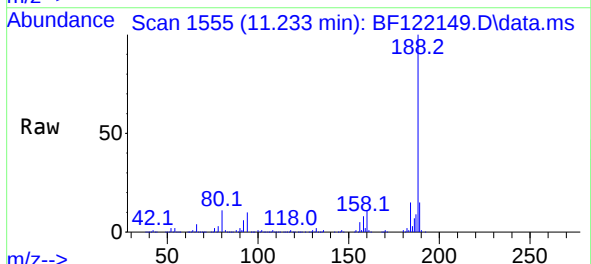



#71
Phenanthrene
Concen: 4.19 ng
RT: 11.257 min Scan# 1559
Delta R.T. -0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55




Instrument :
BNA_F
ClientSampleId :
OR-02-102720

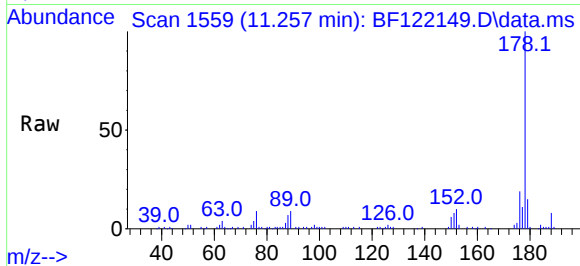


Tgt Ion:178 Resp: 75306
Ion Ratio Lower Upper
178 100
176 19.2 15.9 23.9
179 15.1 12.2 18.4

Manual Integrations
APPROVED



mohammad
10/29/2020 10:44:57 AM

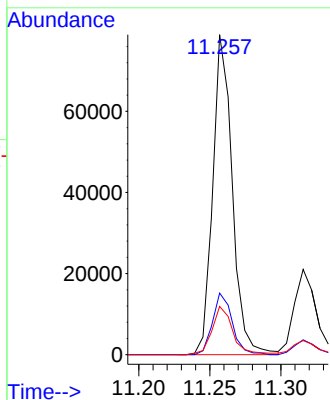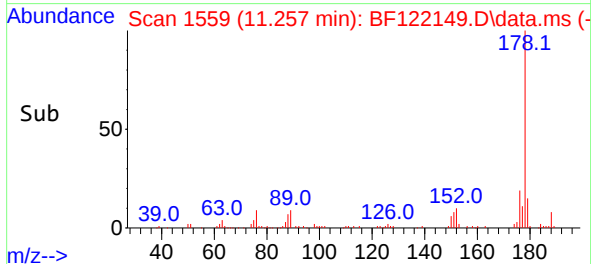


#75
Fluoranthene
Concen: 6.56 ng
RT: 12.451 min Scan# 1762
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

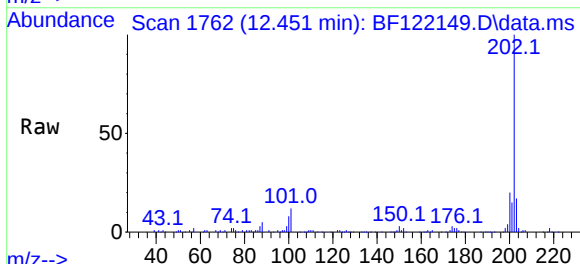


Tgt Ion:202 Resp: 126361
Ion Ratio Lower Upper
202 100
101 11.8 0.0 33.4
203 17.3 0.0 37.9

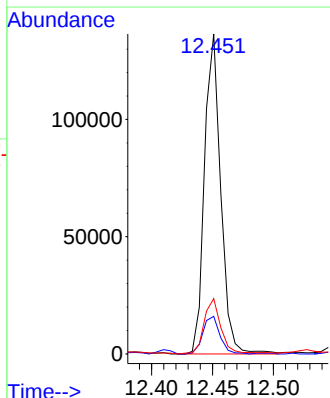



#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.880 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55






Tgt Ion:240 Resp: 227251
Ion Ratio Lower Upper
240 100
120 10.1 9.2 13.8
236 25.6 20.9 31.3


Instrument :
BNA_F
ClientSampleId :
OR-02-102720

Manual Integrations
APPROVED



mohammad
10/29/2020 10:44:57 AM

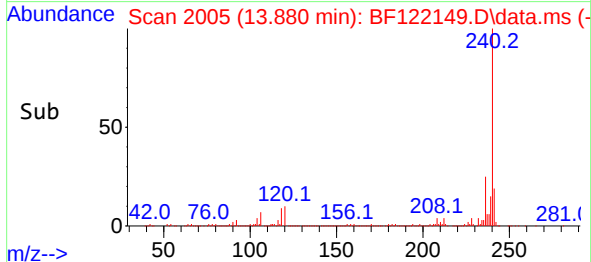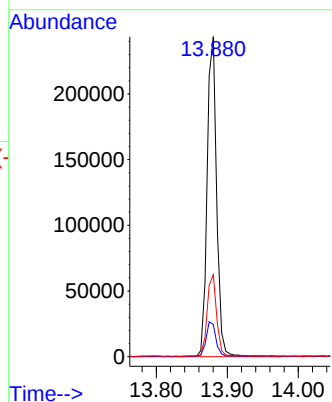


#78
Pyrene
Concen: 6.72 ng
RT: 12.680 min Scan# 1801
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

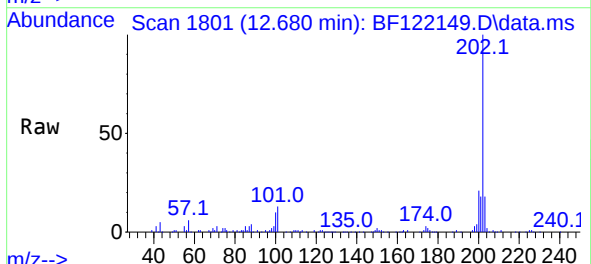


Tgt Ion:202 Resp: 116414
Ion Ratio Lower Upper
202 100
200 21.4 17.4 26.2
203 18.3 14.6 21.8

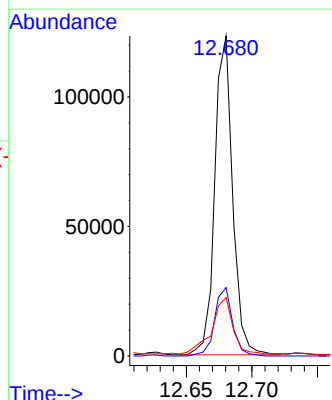



#79
Terphenyl-d14
Concen: 24.53 ng
RT: 12.816 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55




Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Tgt Ion:244 Resp: 292482
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.2
122 10.4 8.1 12.1

Manual Integrations
APPROVED



mohammad
10/29/2020 10:44:57 AM

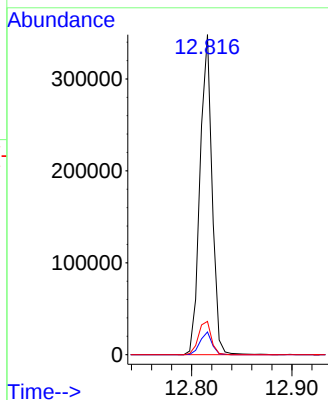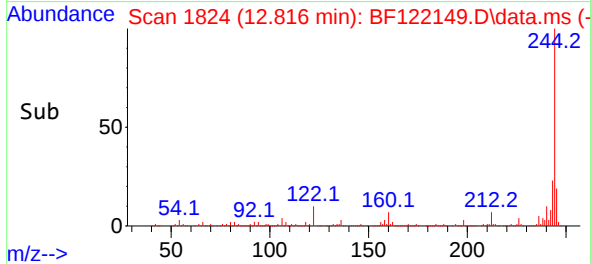


#81
Benzo(a)anthracene
Concen: 4.15 ng
RT: 13.869 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

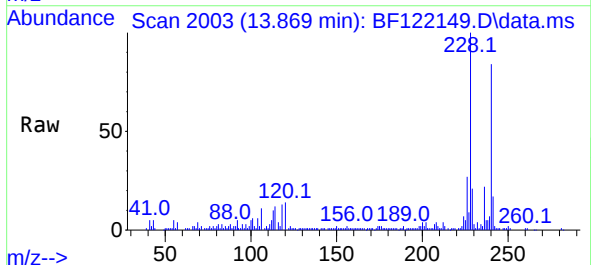

Tgt Ion:228 Resp: 61748
Ion Ratio Lower Upper
228 100
226 26.8 22.3 33.5
229 21.2 16.2 24.4

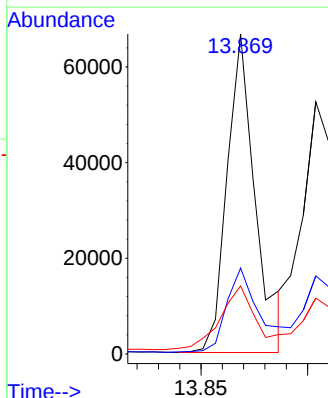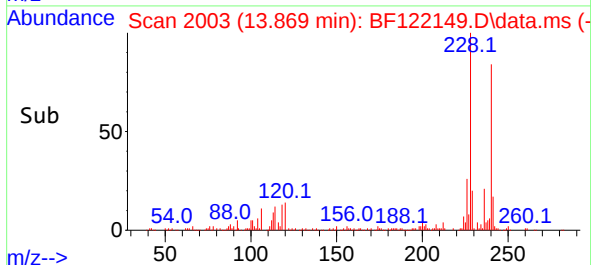







#83
Chrysene
Concen: 3.93 ng
RT: 13.904 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:	228	Resp:	57514
Ion	Ratio	Lower	Upper
228	100		
226	31.0	24.6	37.0
229	22.1	15.9	23.9

Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Manual Integrations
APPROVED


mohammad
10/29/2020 10:44:57 AM

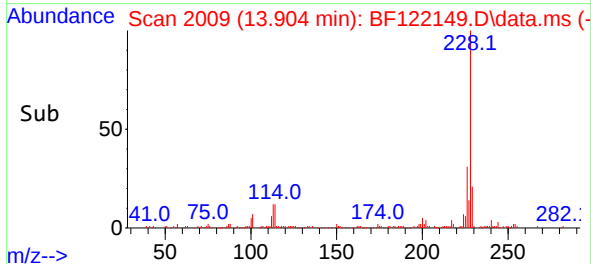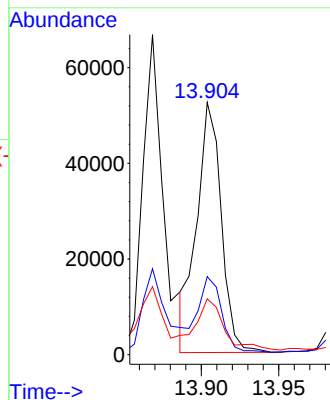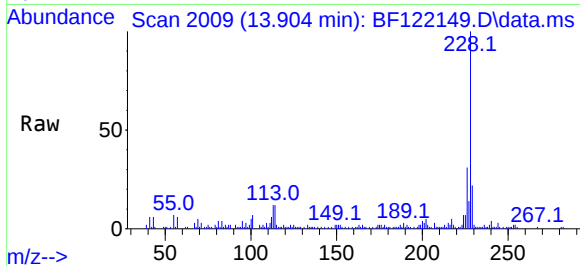

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.316 min Scan# 2249
Delta R.T. 0.012 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:	264	Resp:	238724
Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.7	28.1
265	22.0	17.3	25.9

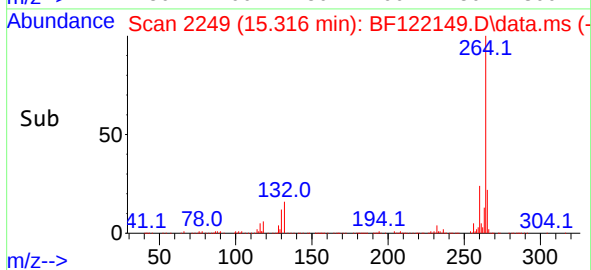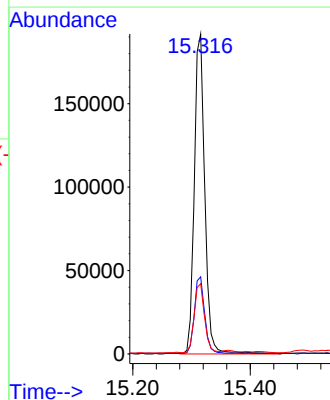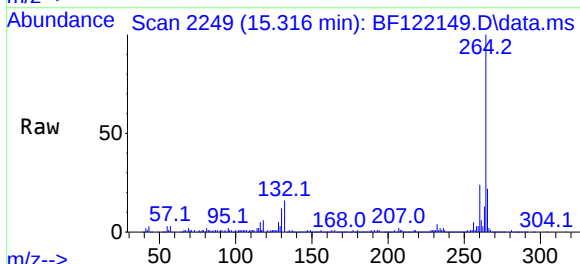







#88
Benzo(b)fluoranthene
Concen: 4.73 ng m
RT: 14.910 min Scan# 2180
Delta R.T. 0.012 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:252 Resp: 76330
Ion Ratio Lower Upper
252 100
253 24.2 18.2 27.2
125 11.4 8.0 12.0

Instrument :
BNA_F
ClientSampleId :
OR-02-102720




Manual Integrations
APPROVED


mohammad
10/29/2020 10:44:57 AM

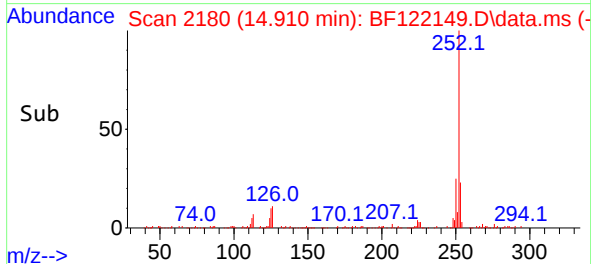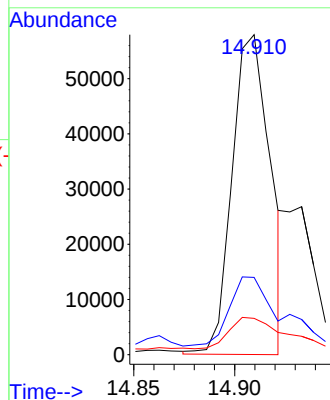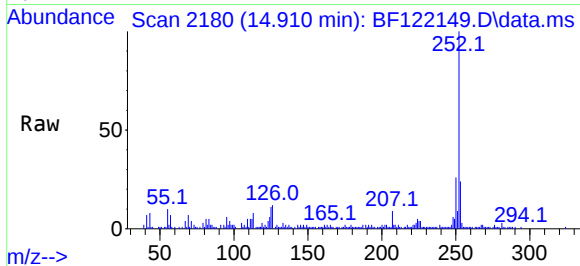


#90
Benzo(a)pyrene
Concen: 3.78 ng
RT: 15.257 min Scan# 2239
Delta R.T. 0.006 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55

Tgt Ion:252 Resp: 52740
Ion Ratio Lower Upper
252 100
253 23.1 17.3 25.9
125 13.0 8.6 13.0#

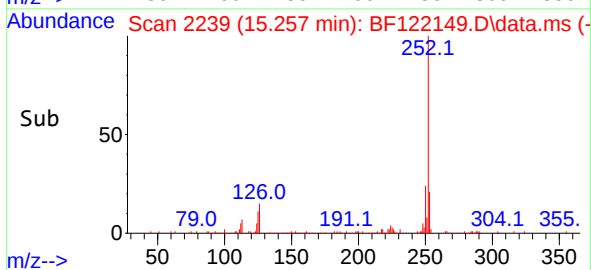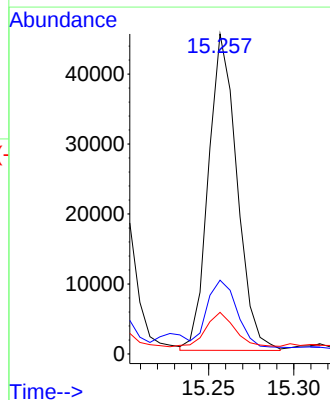
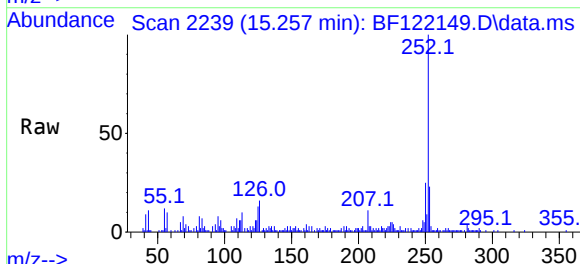




#92
Benzo(g,h,i)perylene
Concen: 2.52 ng
RT: 17.157 min Scan# 2562
Delta R.T. 0.024 min
Lab File: BF122149.D
Acq: 28 Oct 2020 15:55



Tgt Ion:	276	Resp:	32179
Ion	Ratio	Lower	Upper
276	100		
277	27.8	19.4	29.2
138	23.3	17.8	26.6

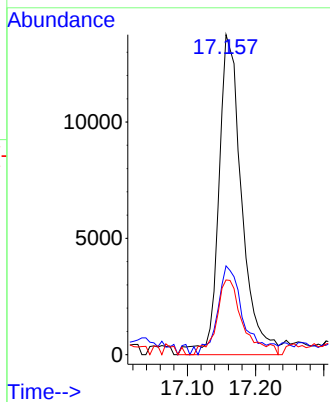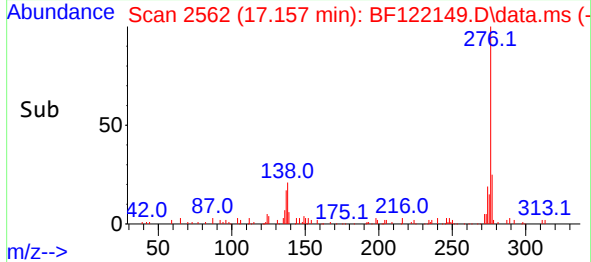

Instrument :
BNA_F
ClientSampleId :
OR-02-102720

Manual Integrations
APPROVED

mohammad
10/29/2020 10:44:57 AM