
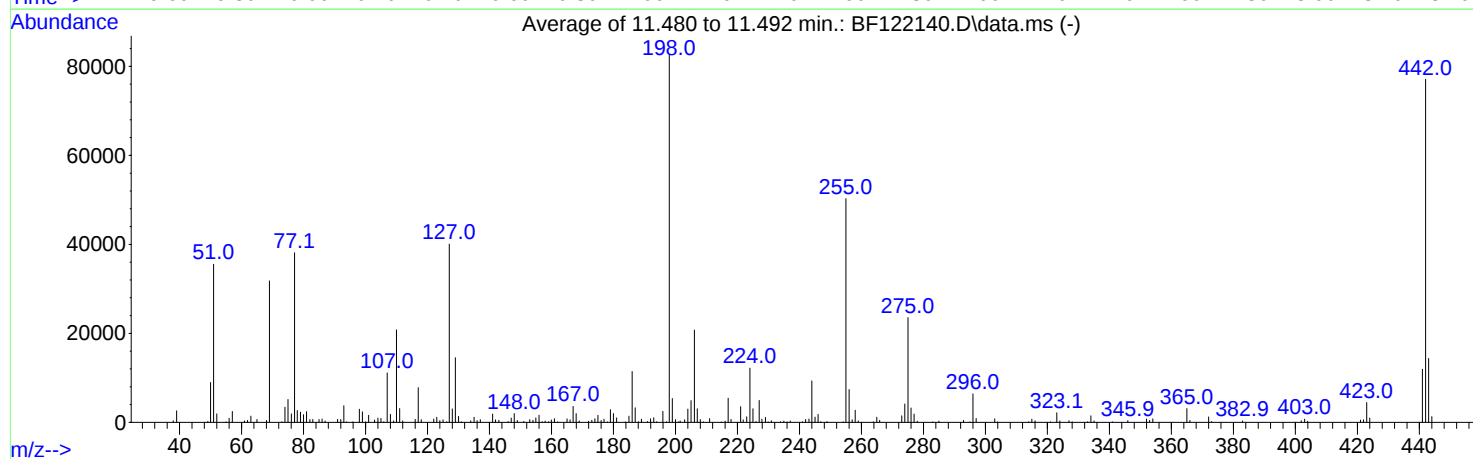


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102820\
 Data File : BF122140.D
 Acq On : 28 Oct 2020 9:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 26 17:27:32 2020

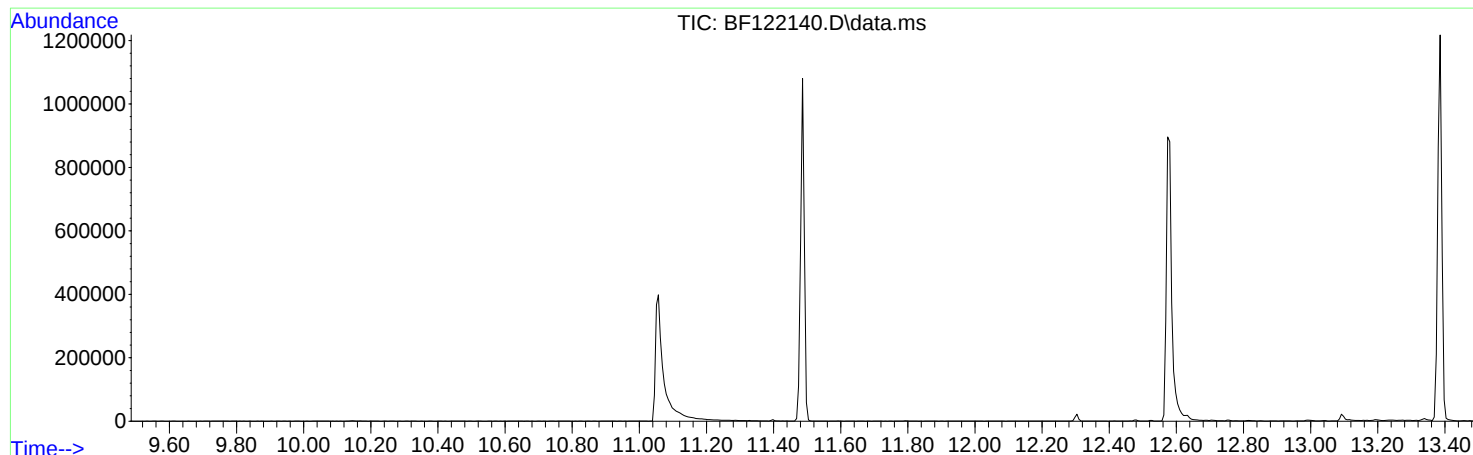

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	35517	PASS
68	69	0.00	2	1.4	447	PASS
69	198	0.00	100	38.5	31803	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	40059	PASS
197	198	0.00	2	0.2	142	PASS
198	198	100	100	100.0	82672	PASS
199	198	5	9	6.5	5371	PASS
275	198	10	60	28.5	23569	PASS
365	198	1	100	3.7	3096	PASS
441	198	0.01	100	14.4	11937	PASS
442	198	50	100	93.2	77083	PASS
443	442	15	24	18.6	14346	PASS