
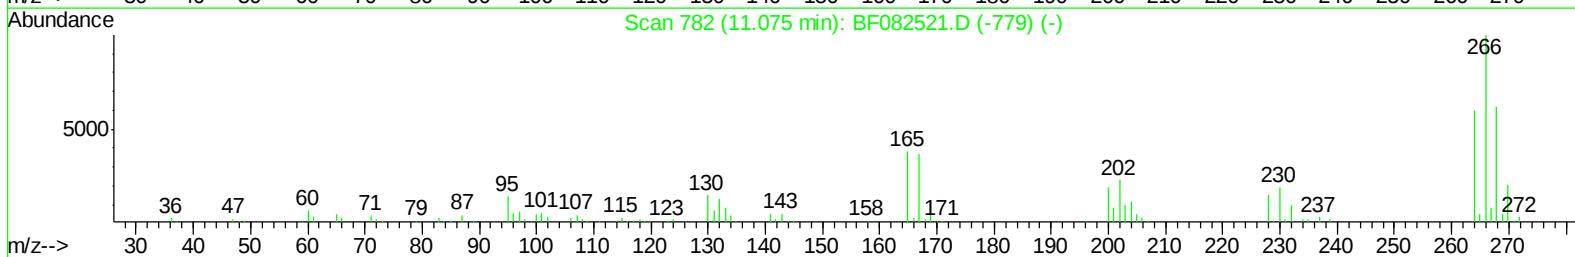
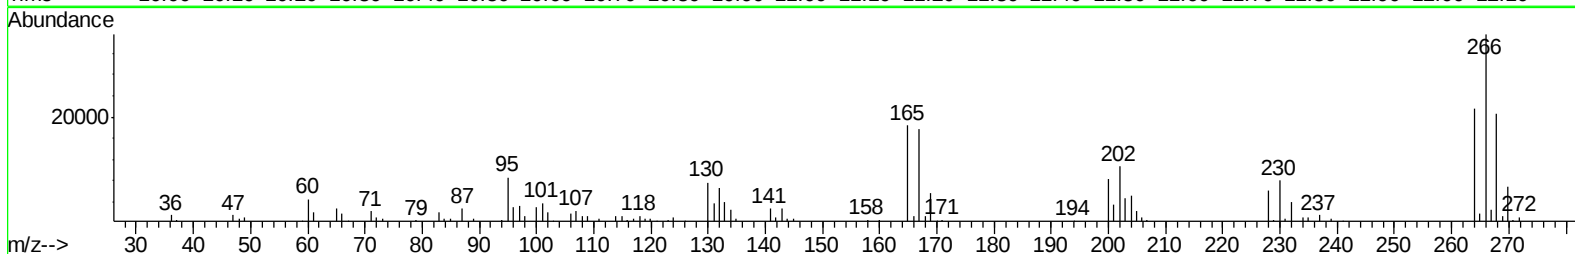


Data Path : Z:\HPCHEM1\BNA_F\Data\BF102915\
Data File : BF082574.D
Acq On : 29 Oct 2015 11:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 07:22:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 29 19:06:23 2015
Response via : Initial Calibration

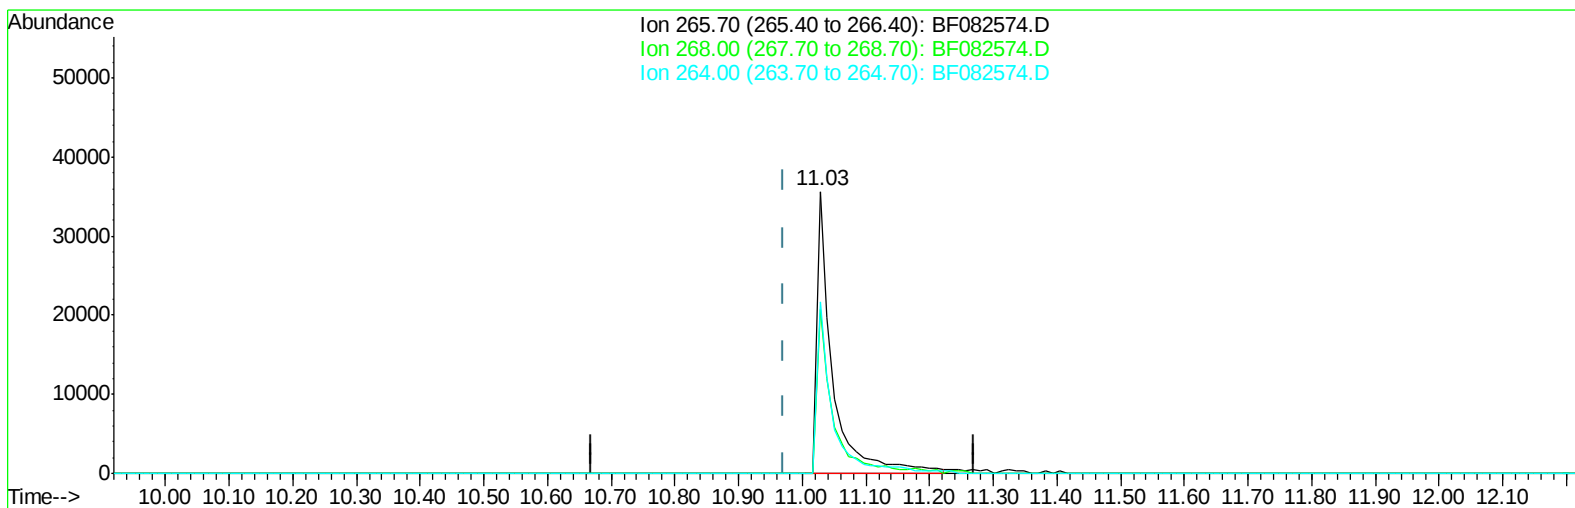

TIC: BF082574.D

(69) Pentachlorophenol (C)




11.028min (+0.057) 0.00ng

response 61569

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	57.99
264.00	60.00	60.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF102915\
Data File : BF082574.D
Acq On : 29 Oct 2015 11:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 07:22:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 29 19:06:23 2015
Response via : Initial Calibration

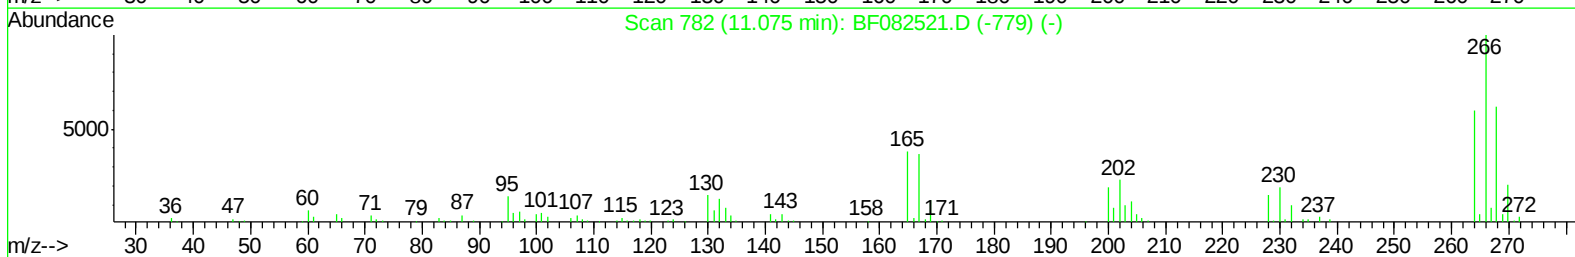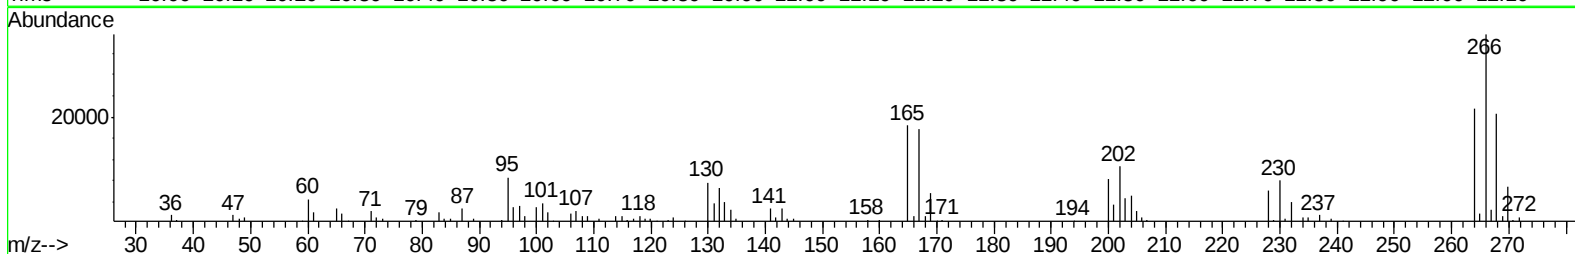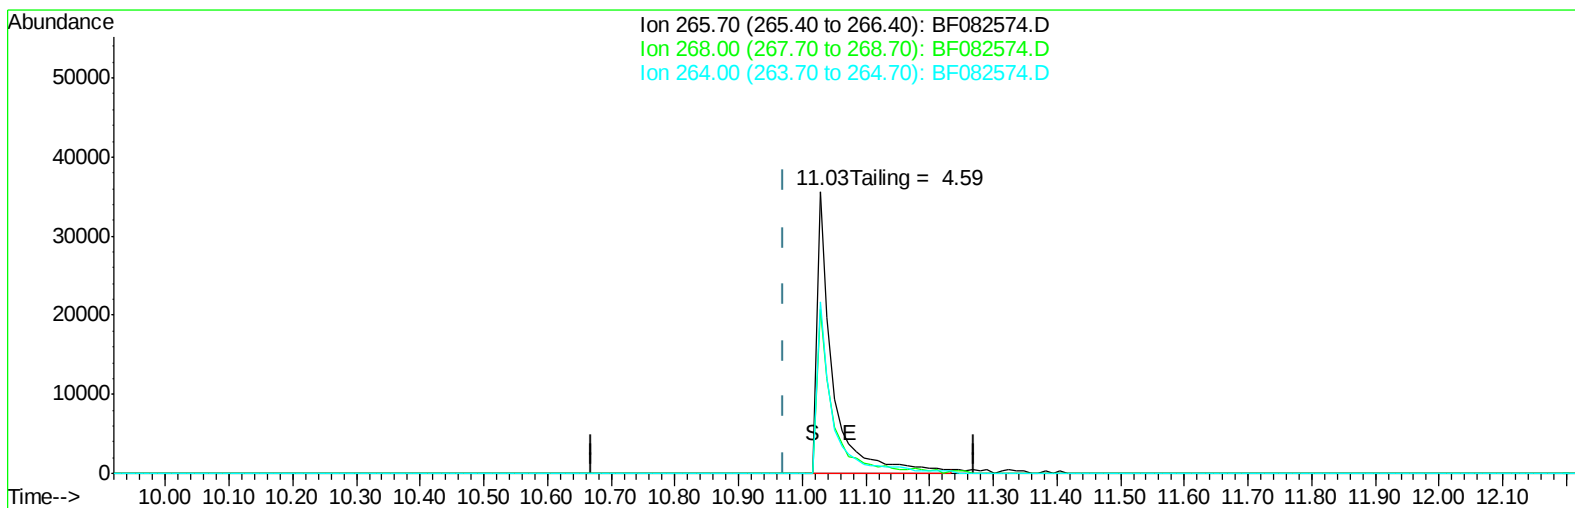

TIC: BF082574.D

(69) Pentachlorophenol (C)




11.028min (+0.057) 0.00ng

response 61569

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	57.99
264.00	60.00	60.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF102915\
Data File : BF082574.D
Acq On : 29 Oct 2015 11:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 07:22:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 29 19:06:23 2015
Response via : Initial Calibration

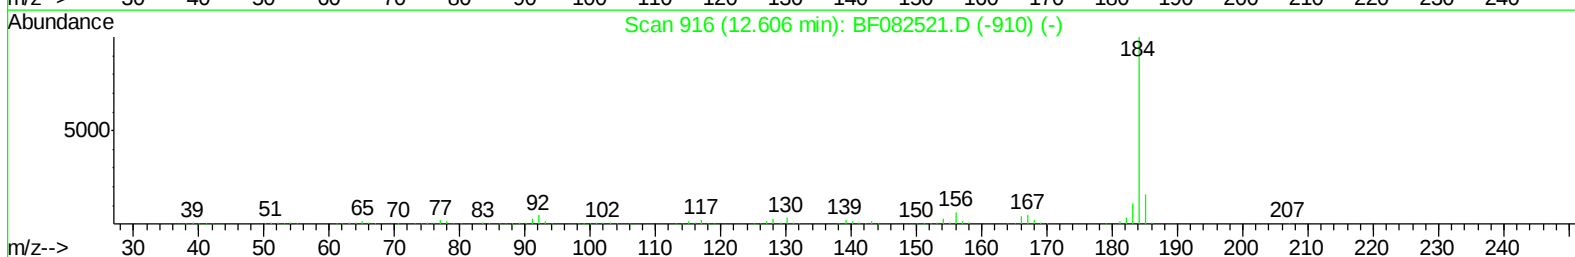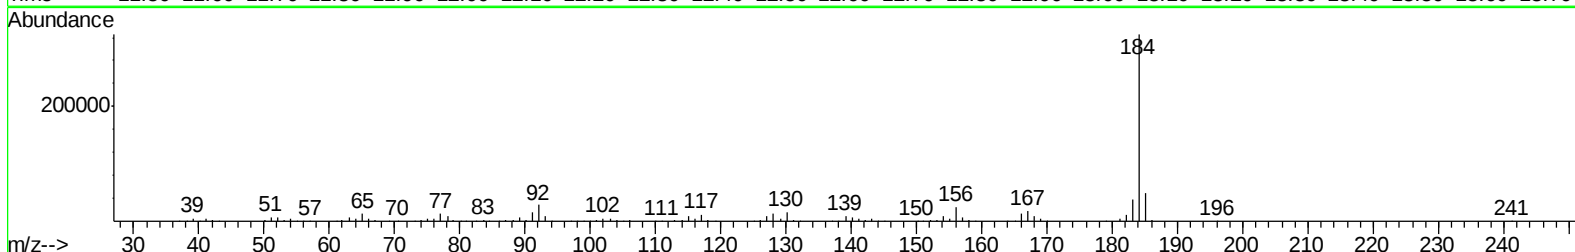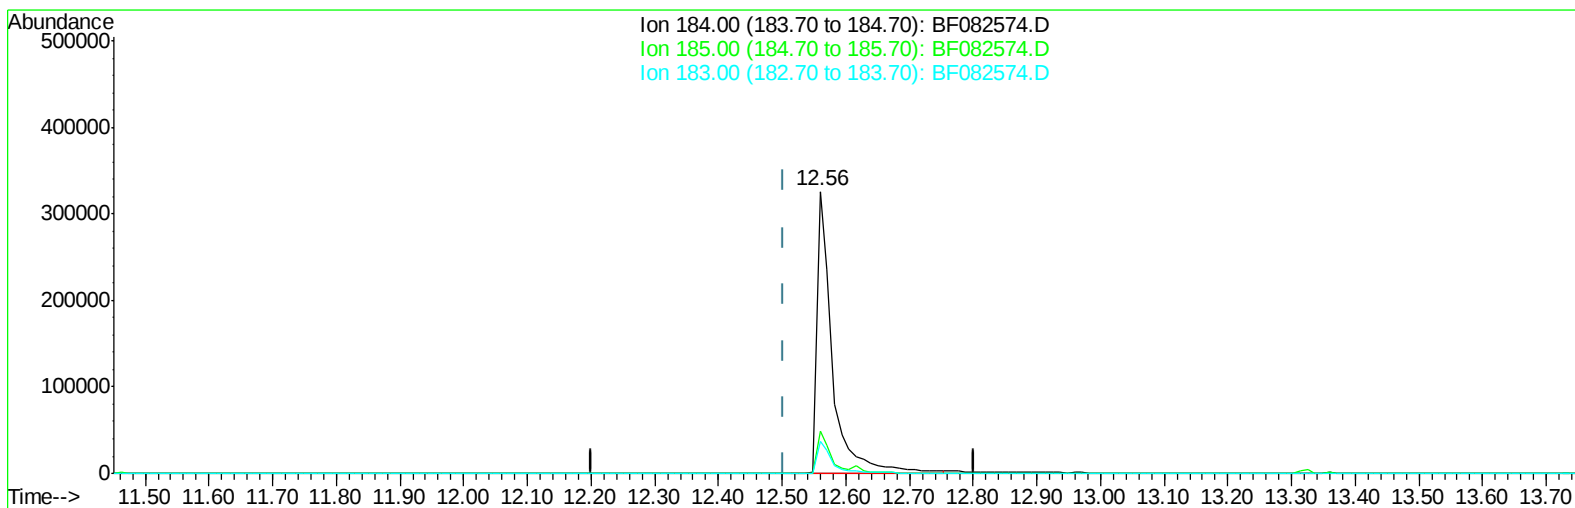

TIC: BF082574.D

(76) Benzidine




12.559min (+0.057) 0.00ng

response 559078

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.87
183.00	11.10	11.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF102915\
Data File : BF082574.D
Acq On : 29 Oct 2015 11:25
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 07:22:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 29 19:06:23 2015
Response via : Initial Calibration

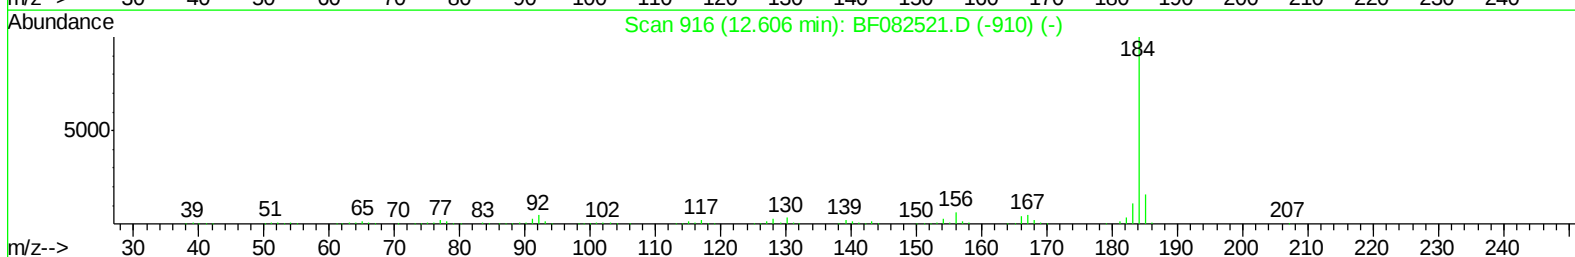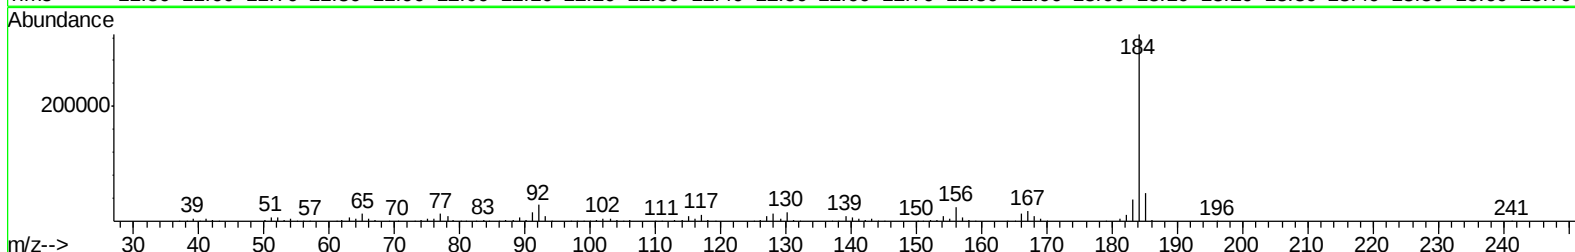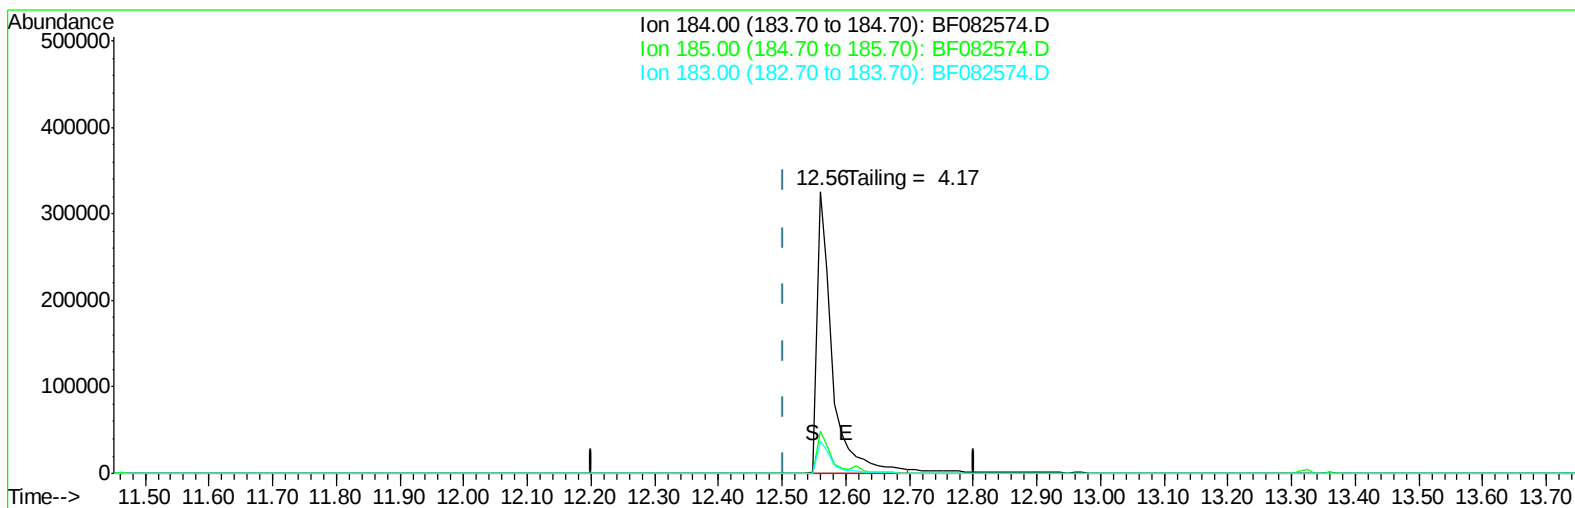

TIC: BF082574.D

(76) Benzidine

12.559min (+0.057) 0.00ng

response 559078

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.87
183.00	11.10	11.54
0.00	0.00	0.00