


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102918\
Data File : BF110249.D
Acq On : 29 Oct 2018 9:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 29 17:29:00 2018

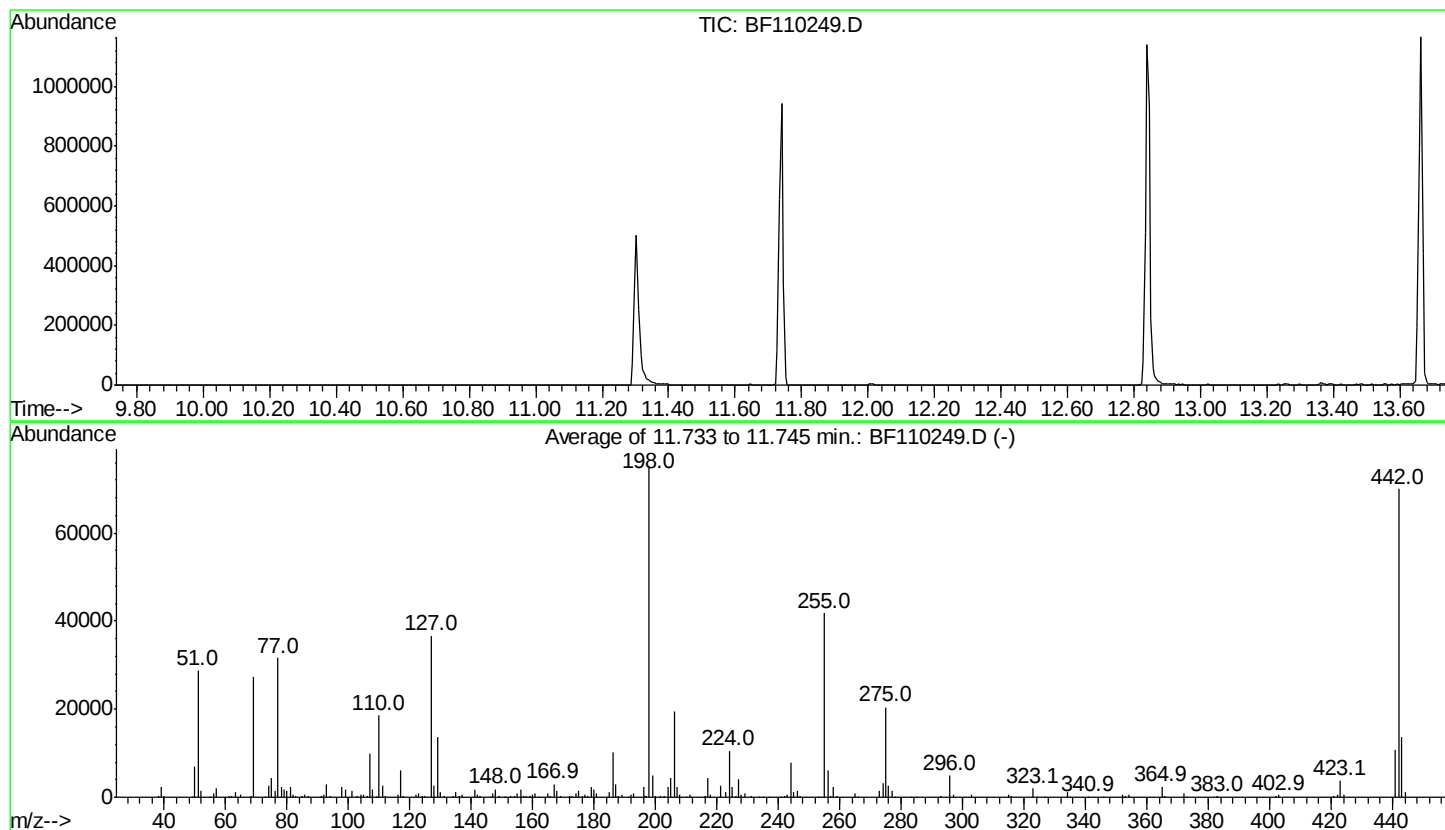

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	28755	PASS
68	69	0.00	2	1.5	420	PASS
69	198	0.00	100	36.4	27393	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	36728	PASS
197	198	0.00	2	0.6	435	PASS
198	198	100	100	100.0	75296	PASS
199	198	5	9	6.7	5026	PASS
275	198	10	60	27.1	20379	PASS
365	198	1	100	3.3	2472	PASS
441	198	0.01	100	14.2	10686	PASS
442	198	50	100	93.0	70040	PASS
443	442	15	24	19.6	13721	PASS