


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102918\
 Data File : BF110265.D
 Acq On : 29 Oct 2018 16:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 17:29:00 2018

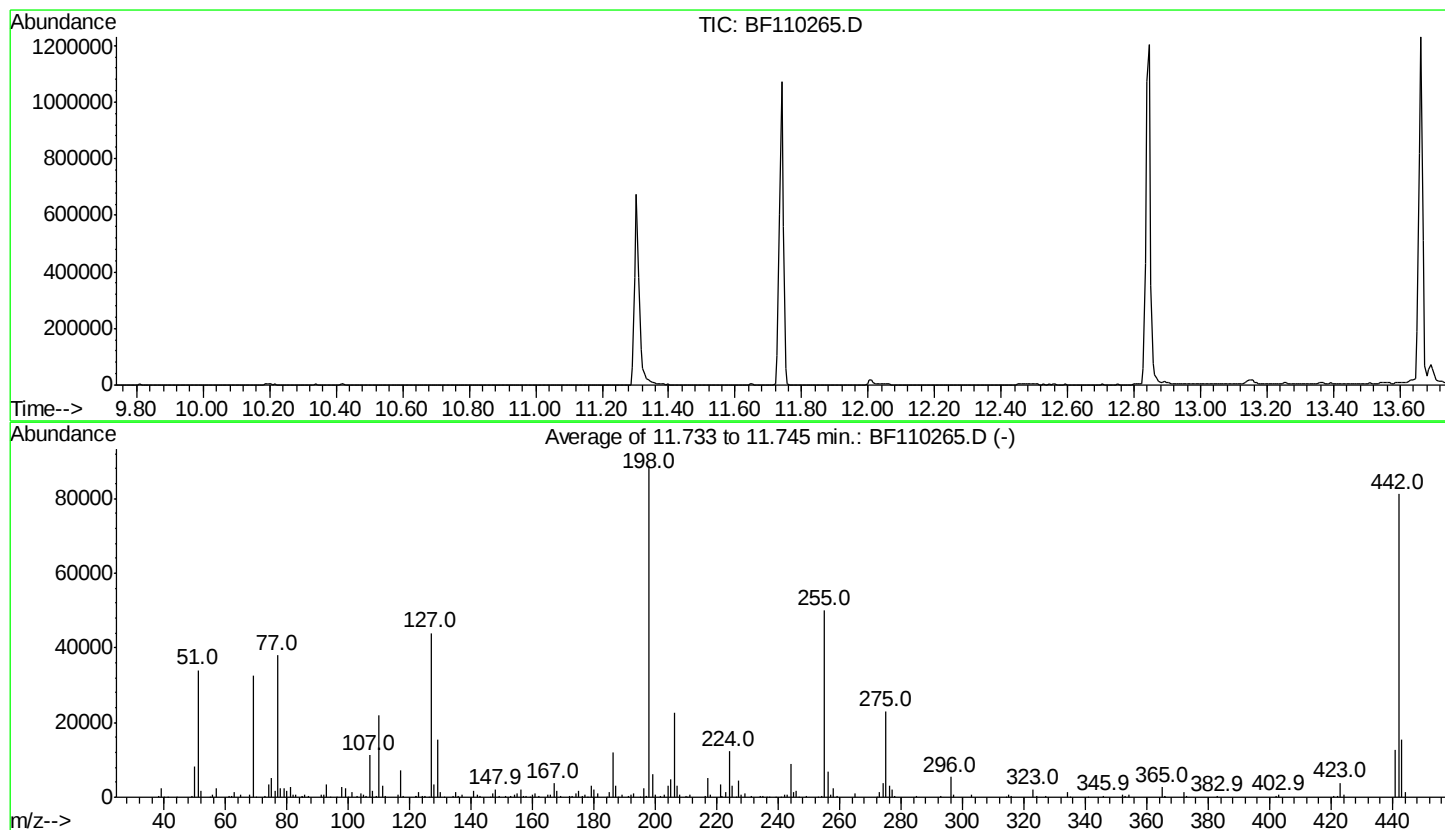

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	34064	PASS
68	69	0.00	2	1.7	562	PASS
69	198	0.00	100	36.7	32564	PASS
70	69	0.00	2	0.3	106	PASS
127	198	10	80	49.5	43973	PASS
197	198	0.00	2	0.2	217	PASS
198	198	100	100	100.0	88813	PASS
199	198	5	9	6.9	6115	PASS
275	198	10	60	25.8	22898	PASS
365	198	1	100	3.0	2656	PASS
441	198	0.01	100	14.4	12796	PASS
442	198	50	100	91.4	81205	PASS
443	442	15	24	18.9	15318	PASS