
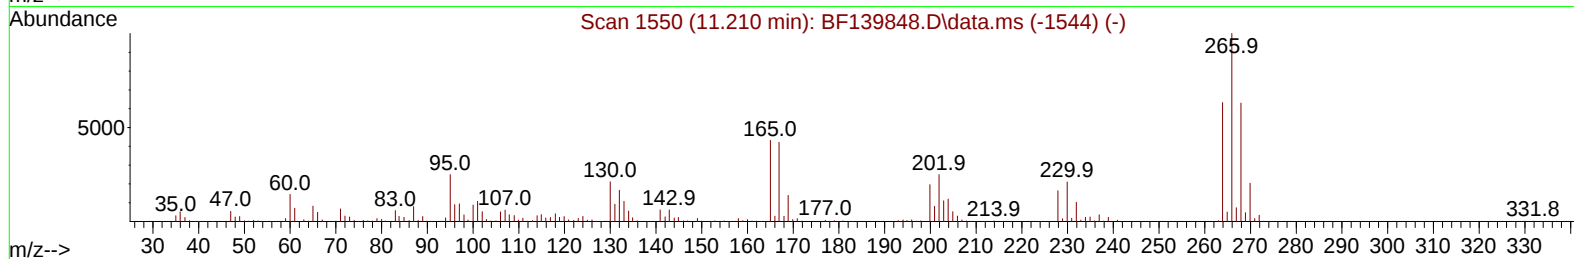
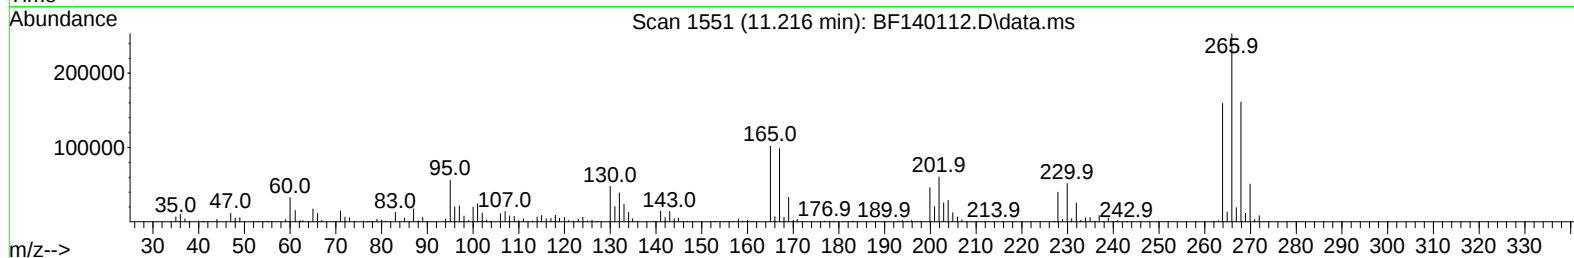


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140112.D
Acq On : 29 Oct 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 16:07:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

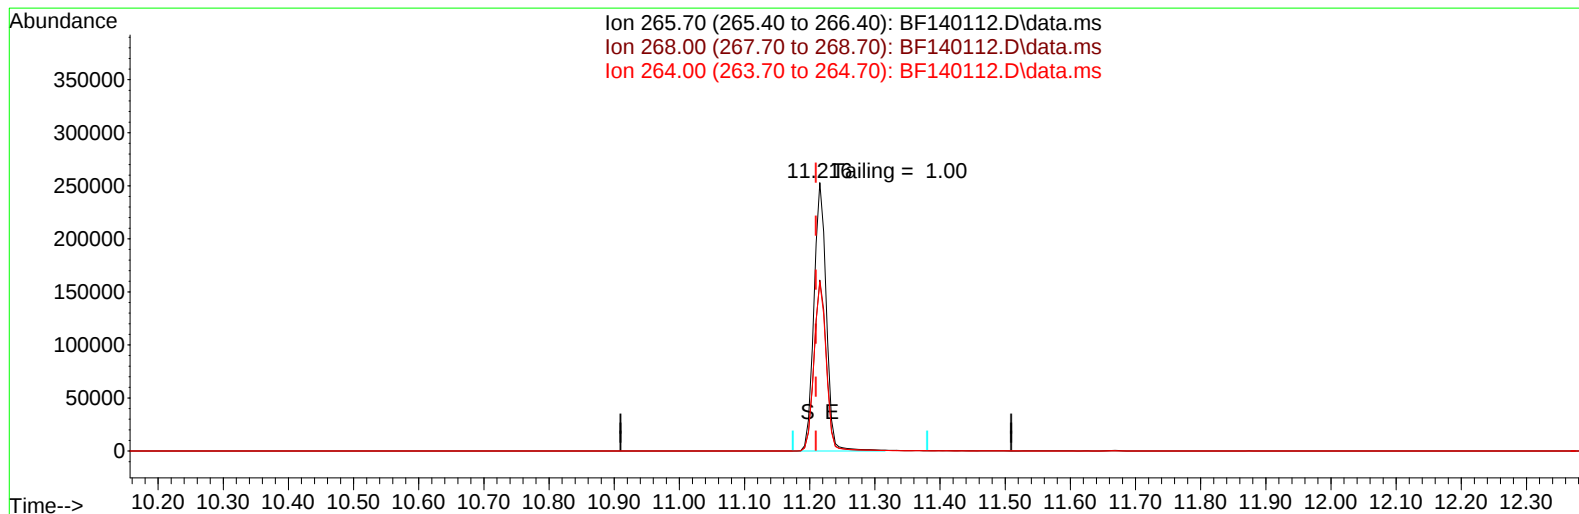

TIC: BF140112.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 107927.56 ng

response 336959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.70
264.00	63.20	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140112.D
Acq On : 29 Oct 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 16:07:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

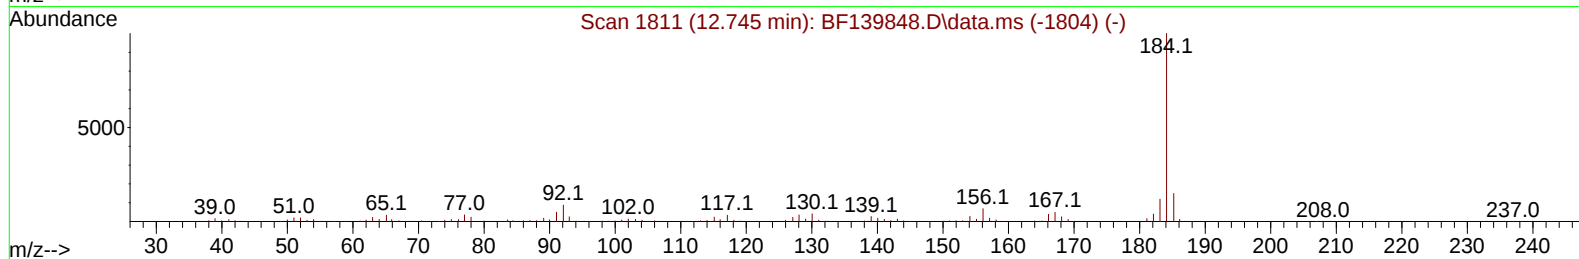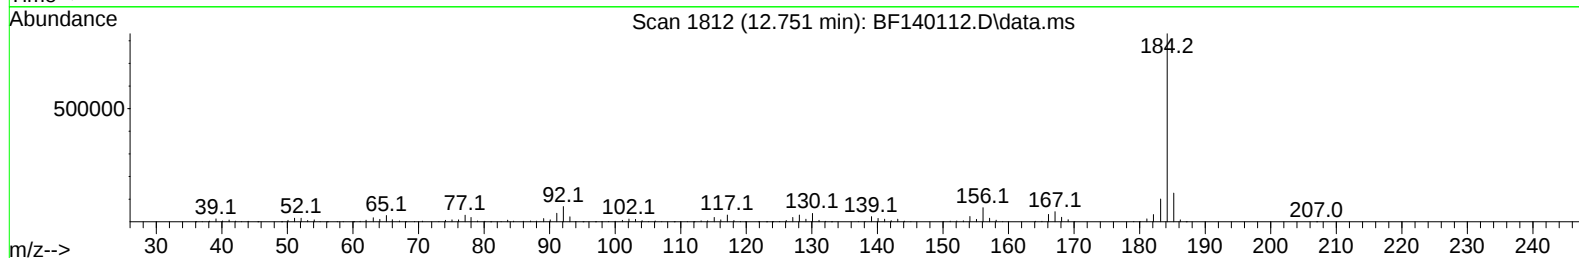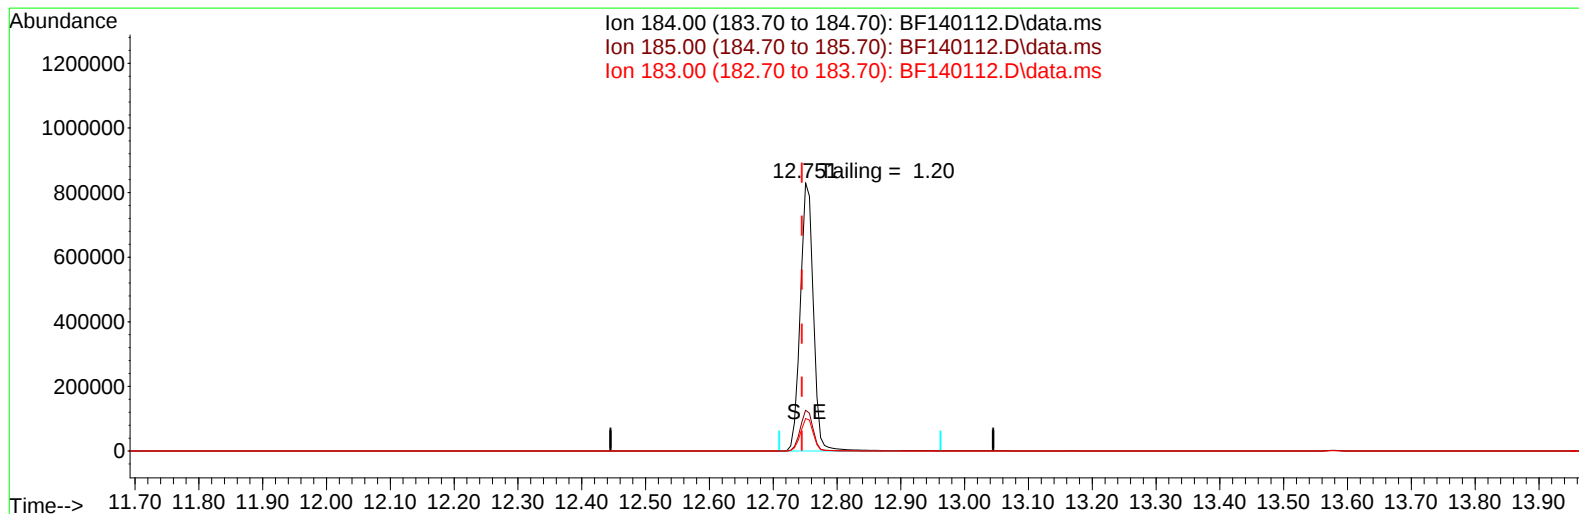

TIC: BF140112.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 174264.48 ng

response 1186317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.23
183.00	11.80	12.10
0.00	0.00	0.00