

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
 Data File : BF140144.D
 Acq On : 30 Oct 2024 06:24
 Operator : RC/JU
 Sample : P4594-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Quant Time: Oct 30 06:49:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 15:07:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	128166	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	503091	20.000	ng	0.00
39) Acenaphthene-d10	9.922	164	268045	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	412129	20.000	ng	0.00
76) Chrysene-d12	14.051	240	261160	20.000	ng	0.00
86) Perylene-d12	15.539	264	194687	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	886486	108.280	ng	0.02
7) Phenol-d6	6.510	99	1054579	99.456	ng	0.00
23) Nitrobenzene-d5	7.445	82	843783	92.956	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	278801	111.200	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1488821	91.797	ng	0.00
79) Terphenyl-d14	12.998	244	1338489	83.514	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140144.D
Acq On : 30 Oct 2024 06:24
Operator : RC/JU
Sample : P4594-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-5

Quant Time: Oct 30 06:49:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration




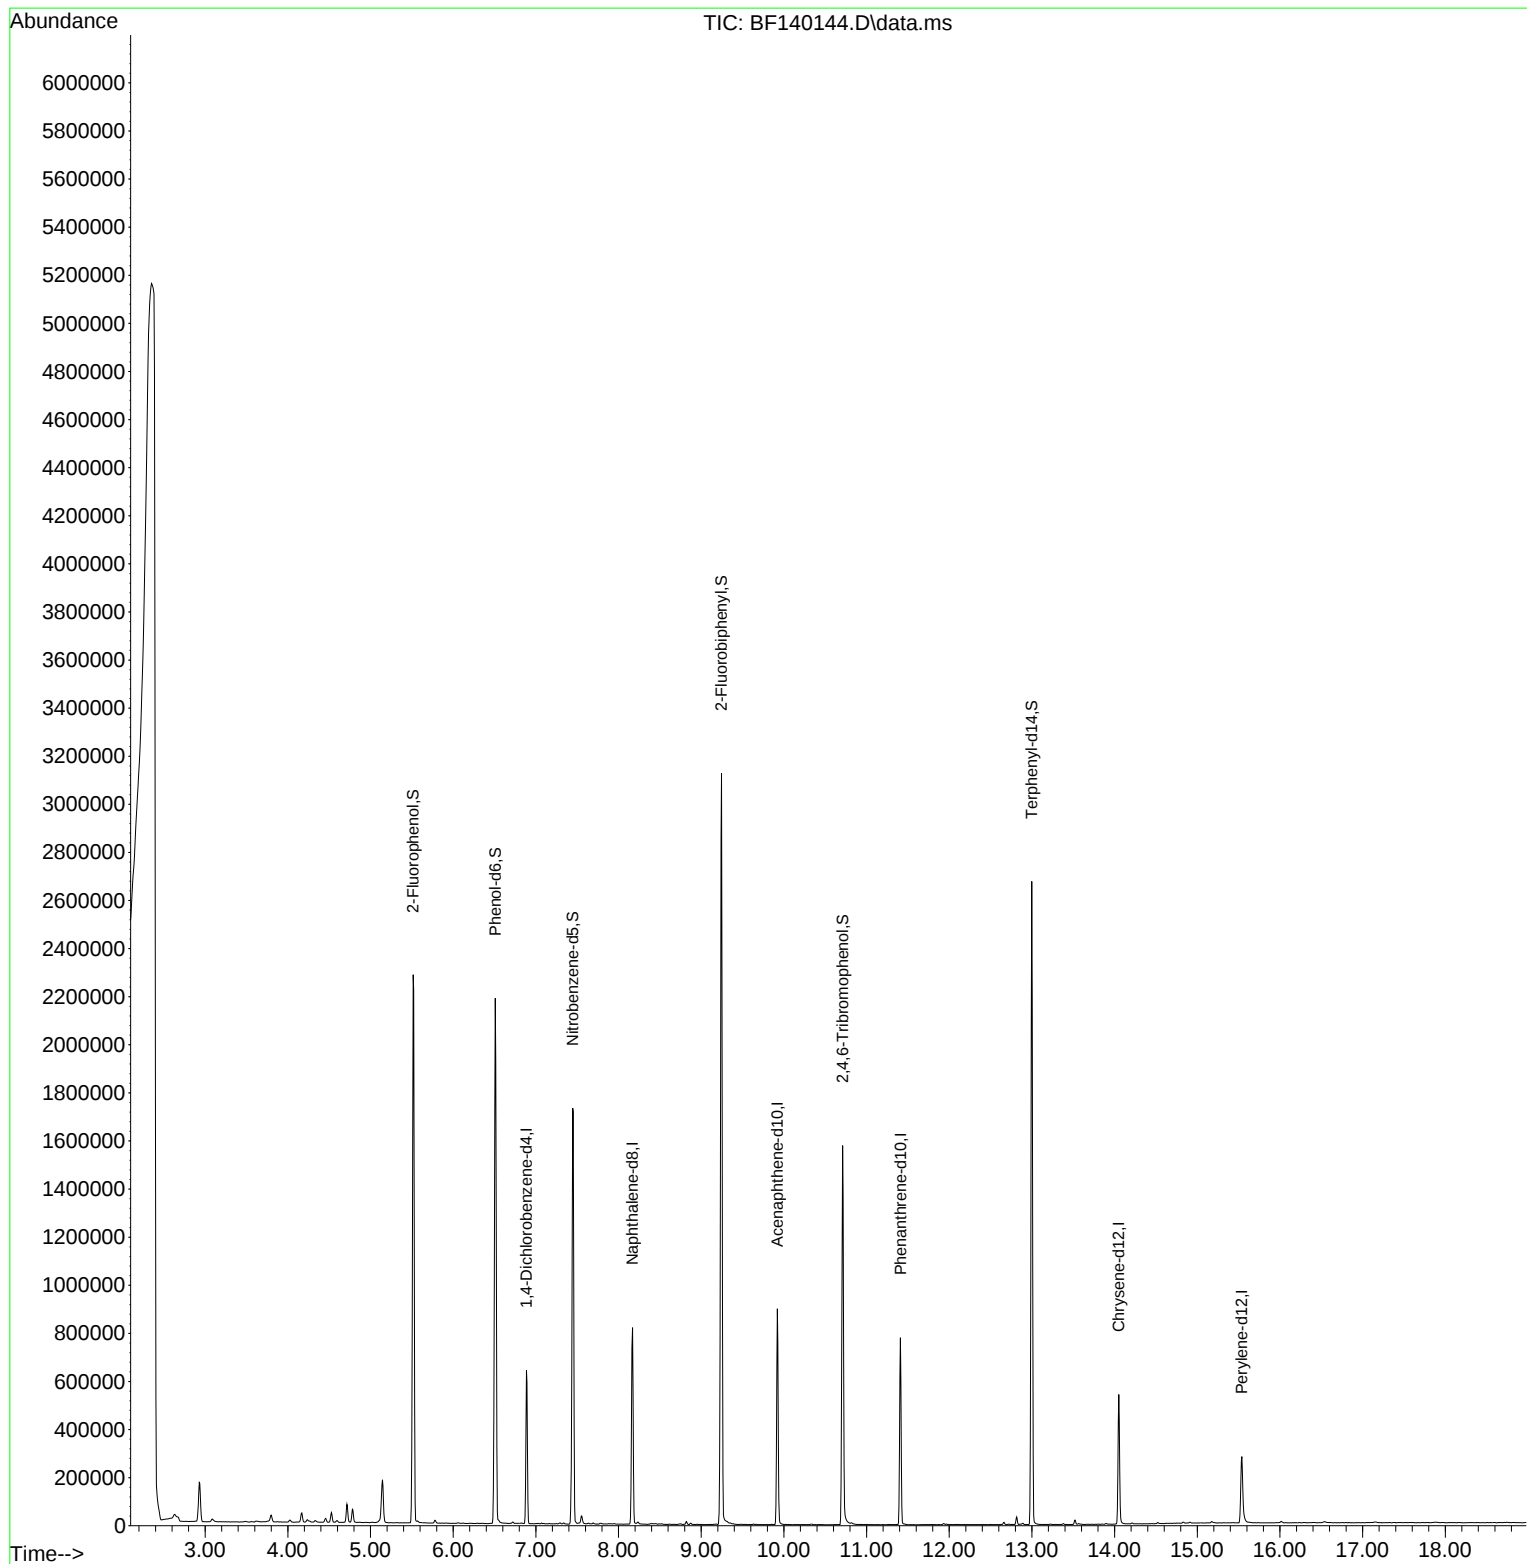


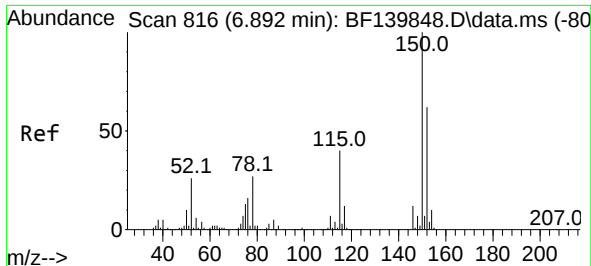

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.005 min
Lab File: BF140144.D
Acq: 30 Oct 2024 06:24




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion:152 Resp: 128166
Ion Ratio Lower Upper
152 100
150 155.5 130.2 195.2
115 64.4 51.4 77.2

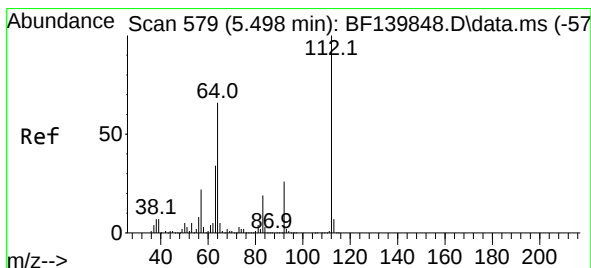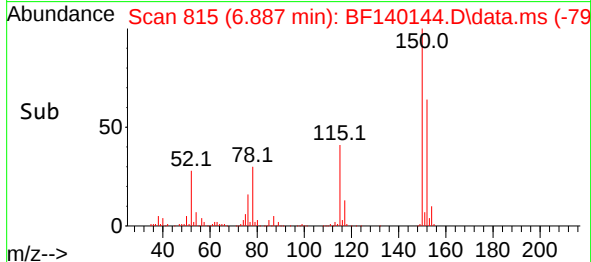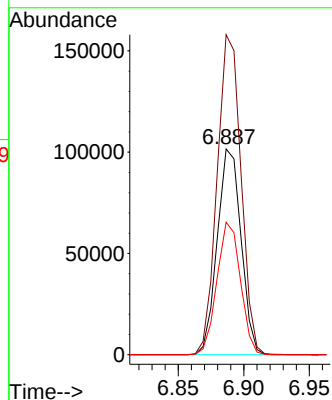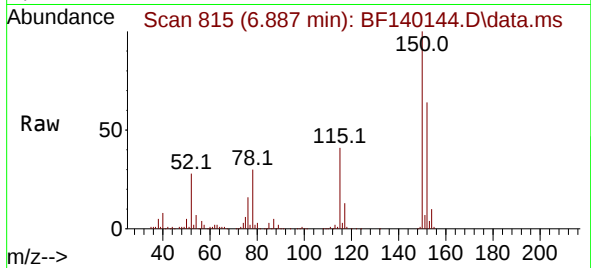

#5
2-Fluorophenol
Concen: 108.280 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.018 min
Lab File: BF140144.D
Acq: 30 Oct 2024 06:24

Tgt Ion:112 Resp: 886486
Ion Ratio Lower Upper
112 100
64 67.2 53.0 79.6
63 35.6 27.0 40.4

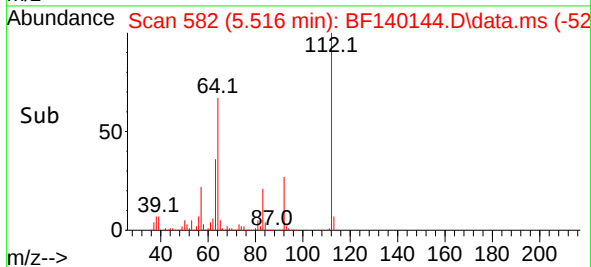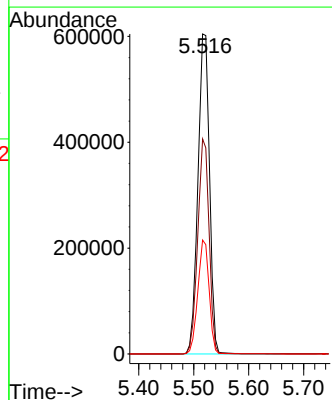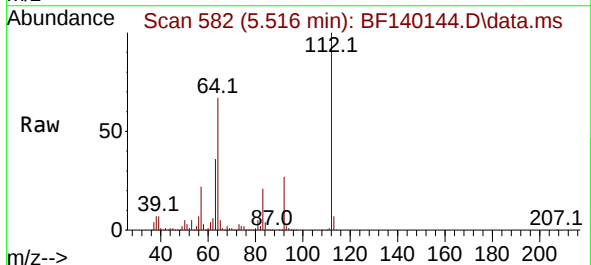




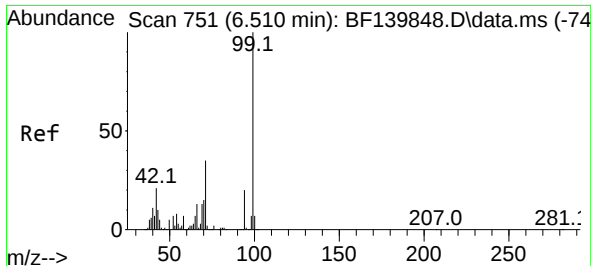


#7
Phenol-d6
Concen: 99.456 ng
RT: 6.510 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF140144.D
Acq: 30 Oct 2024 06:24

Instrument :
BNA_F
ClientSampleId :
TP-5

Tgt Ion: 99 Resp: 1054579




Ion	Ratio	Lower	Upper
99	100		
42	20.9	16.7	25.1
71	37.1	27.7	41.5

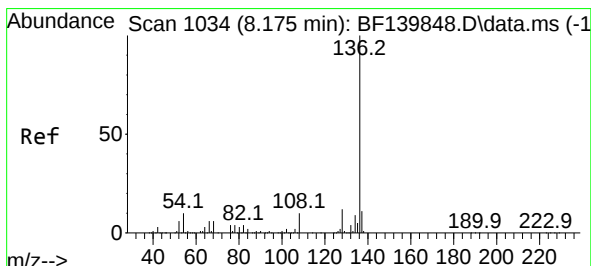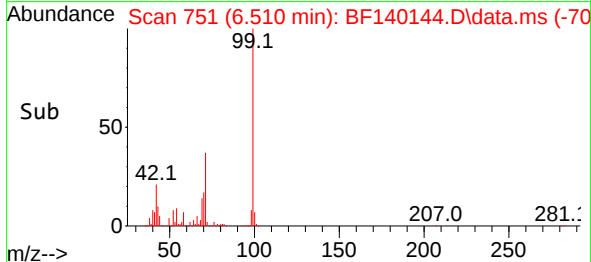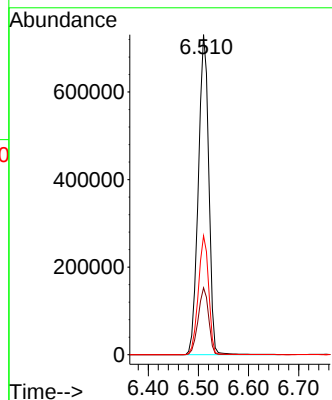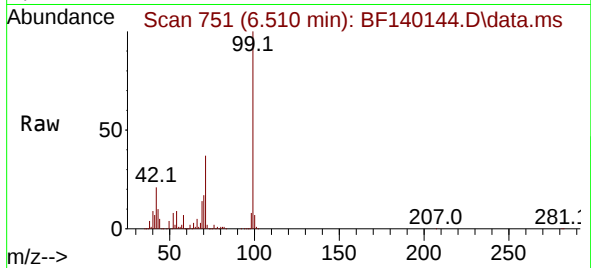


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1033
Delta R.T. -0.006 min
Lab File: BF140144.D
Acq: 30 Oct 2024 06:24

Tgt Ion: 136 Resp: 503091

Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.6	12.8
54	10.2	8.4	12.6
68	6.0	5.1	7.7


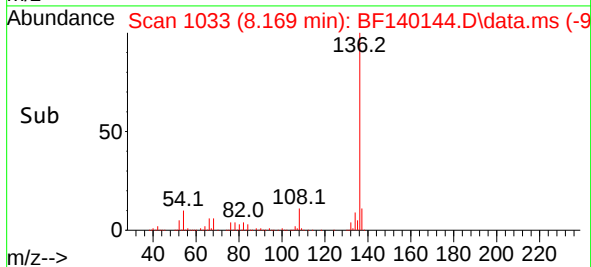
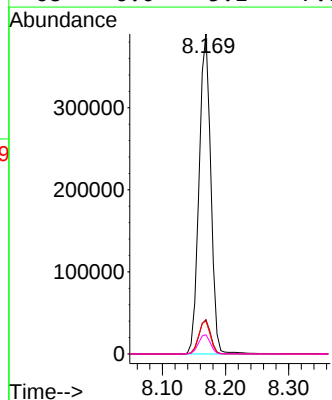
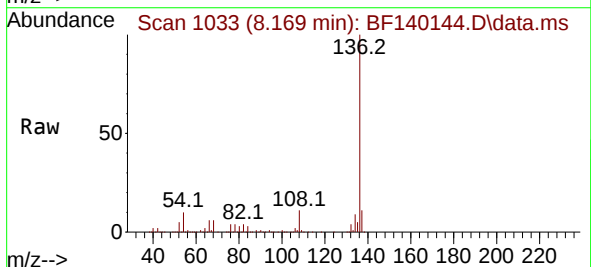


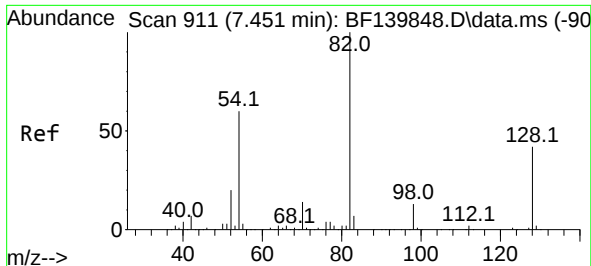

#23
Nitrobenzene-d5
Concen: 92.956 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF140144.D
Acq: 30 Oct 2024 06:24




Instrument :
BNA_F
ClientSampleId :
TP-5


Tgt Ion: 82 Resp: 843783
Ion Ratio Lower Upper
82 100
128 41.2 33.4 50.0
54 58.2 47.8 71.8

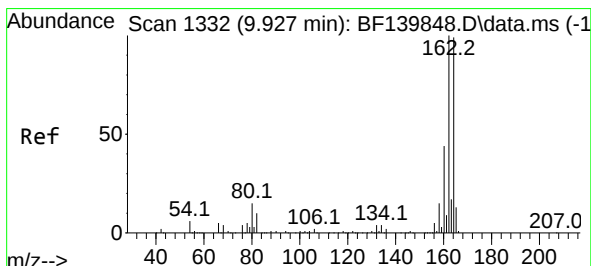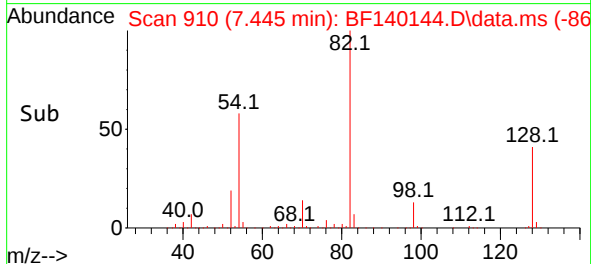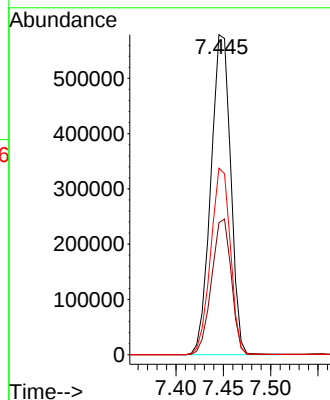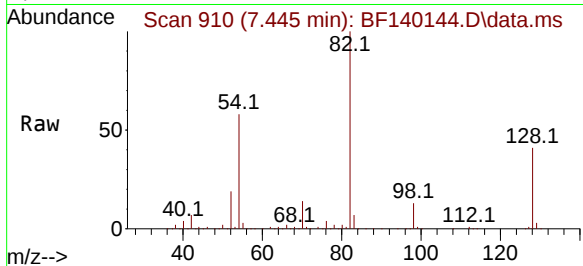

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1331
Delta R.T. -0.005 min
Lab File: BF140144.D
Acq: 30 Oct 2024 06:24

Tgt Ion:164 Resp: 268045
Ion Ratio Lower Upper
164 100
162 101.7 81.0 121.4
160 45.1 35.4 53.0

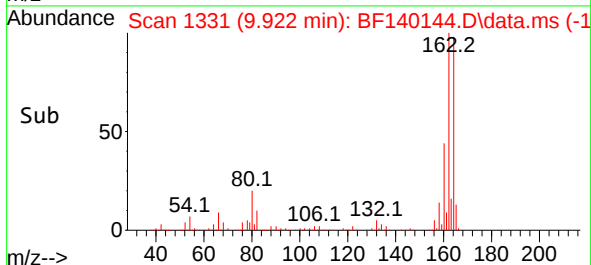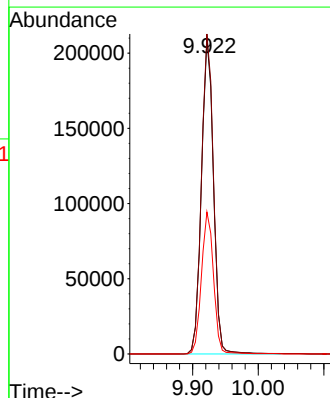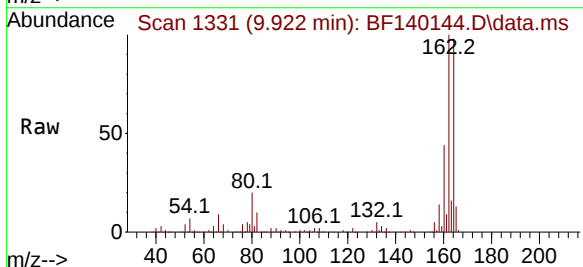

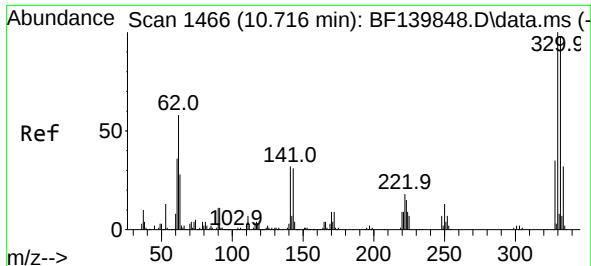

#42

2,4,6-Tribromophenol

Concen: 111.200 ng

RT: 10.710 min Scan# 1465

Delta R.T. -0.006 min

Lab File: BF140144.D

Acq: 30 Oct 2024 06:24

Instrument :

BNA_F

ClientSampleId :

TP-5





Tgt Ion:330 Resp: 278801

Ion Ratio Lower Upper

330 100

332 96.7 78.1 117.1

141 31.5 26.6 39.8

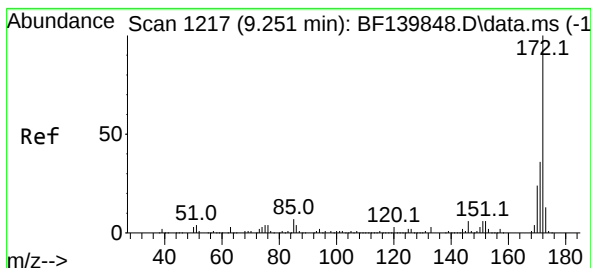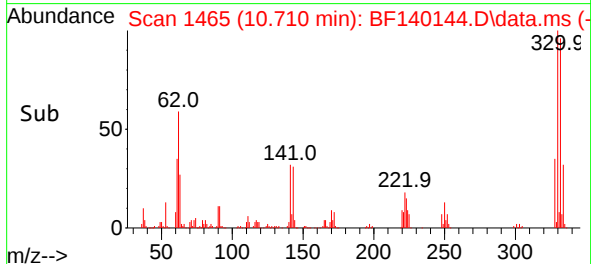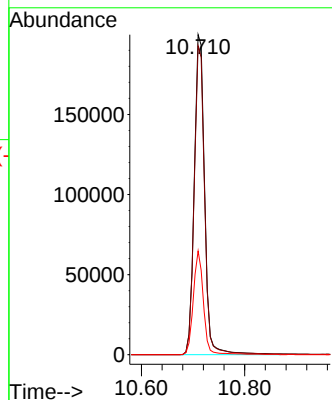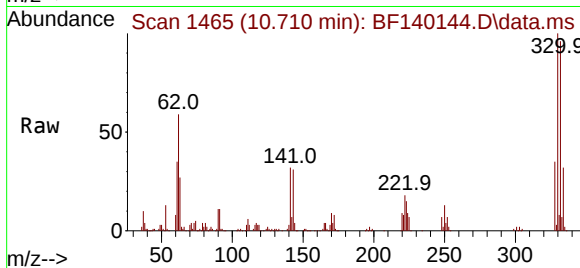

#45

2-Fluorobiphenyl

Concen: 91.797 ng

RT: 9.245 min Scan# 1216

Delta R.T. -0.006 min

Lab File: BF140144.D

Acq: 30 Oct 2024 06:24




Tgt Ion:172 Resp: 1488821


Ion Ratio Lower Upper

172 100

171 35.9 28.6 43.0

170 23.9 19.1 28.7

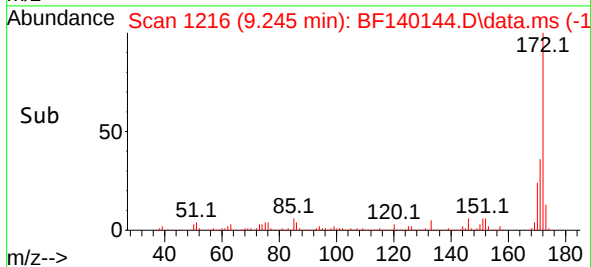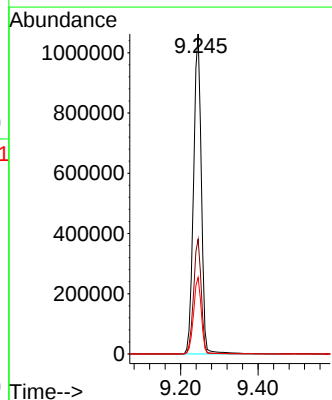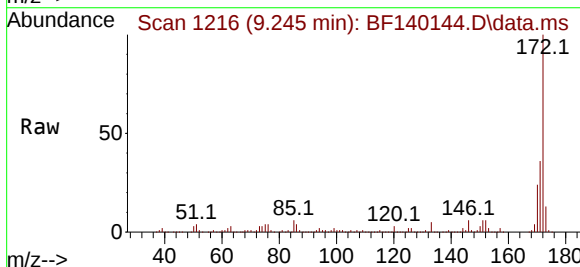

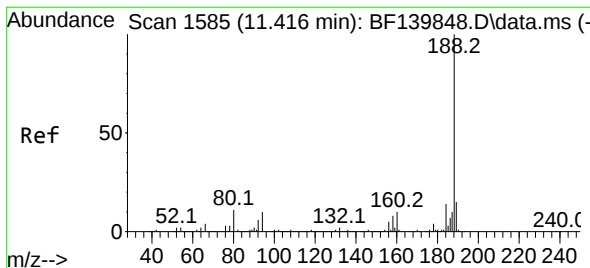

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.410 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF140144.D

Acq: 30 Oct 2024 06:24

Instrument :

BNA_F

ClientSampleId :

TP-5





Tgt Ion:188 Resp: 412129

Ion Ratio Lower Upper

188 100

94 9.2 7.9 11.9

80 10.3 9.0 13.4

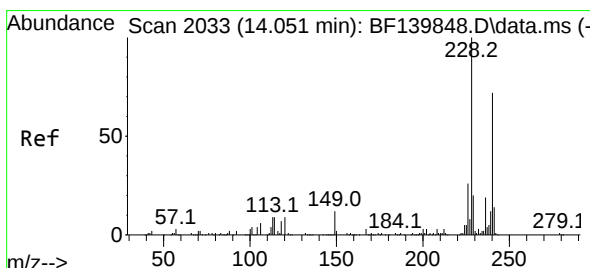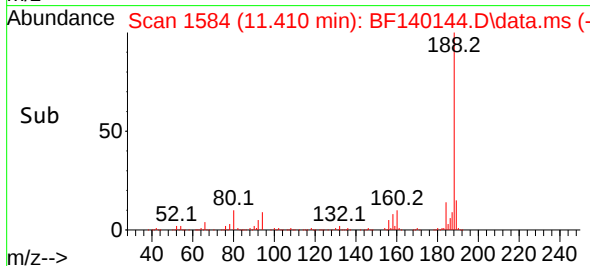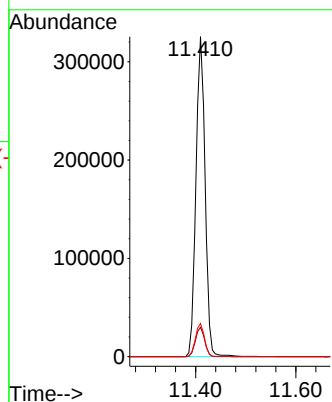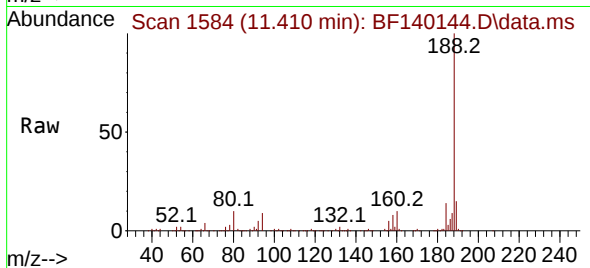

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.051 min Scan# 2033

Delta R.T. 0.000 min

Lab File: BF140144.D

Acq: 30 Oct 2024 06:24




Tgt Ion:240 Resp: 261160


Ion Ratio Lower Upper

240 100

120 11.1 9.4 14.2

236 26.1 20.9 31.3


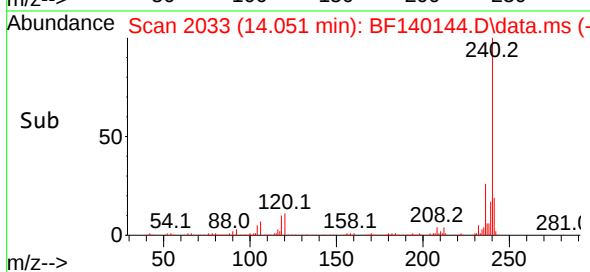
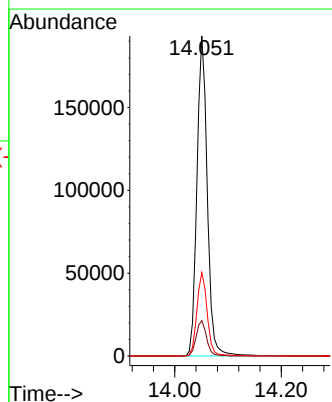
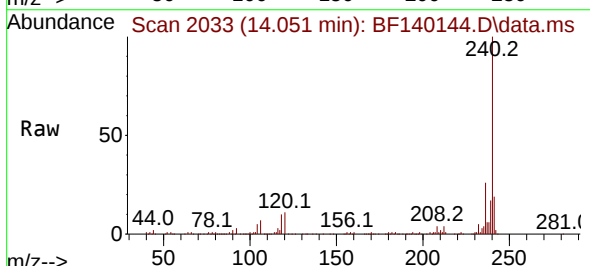


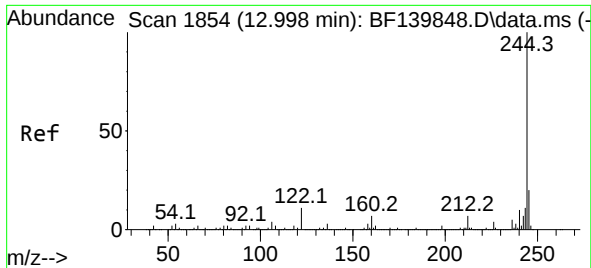

#79
 Terphenyl-d14
 Concen: 83.514 ng
 RT: 12.998 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF140144.D
 Acq: 30 Oct 2024 06:24

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Tgt Ion:244 Resp: 1338489
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.7 8.5
 122 10.0 8.6 13.0

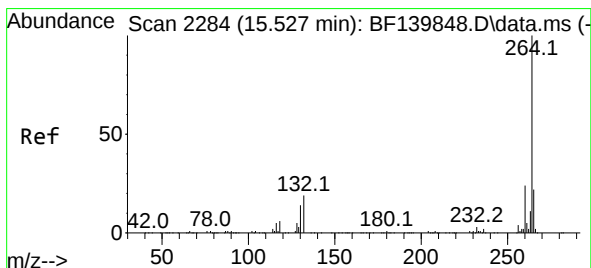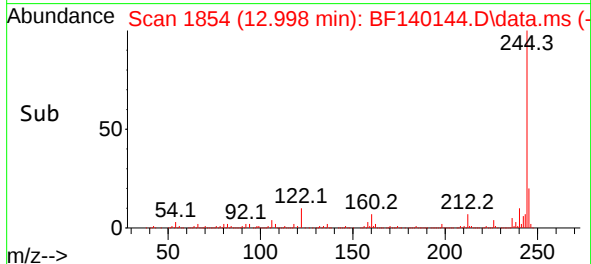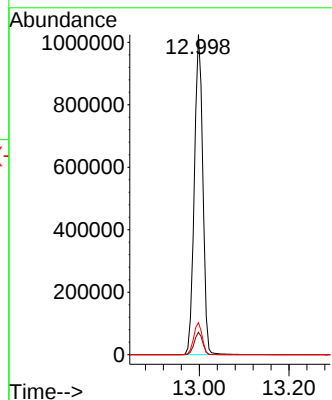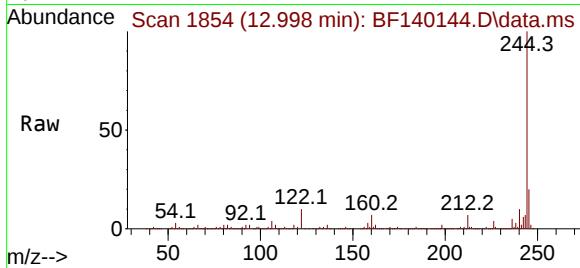

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.539 min Scan# 2286
 Delta R.T. 0.012 min
 Lab File: BF140144.D
 Acq: 30 Oct 2024 06:24

Tgt Ion:264 Resp: 194687
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.4 29.2
 265 21.3 17.4 26.0

