

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
 Data File : BF140134.D
 Acq On : 30 Oct 2024 02:04
 Operator : RC/JU
 Sample : PB164500BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB164500BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.246	20	26	34	rVB	81464	137671	3.52%	0.608%
2	5.516	575	582	587	rBV	2372445	3334980	85.20%	14.722%
3	6.510	744	751	756	rBV	2290118	3341232	85.36%	14.750%
4	6.887	810	815	820	rBV	622264	753518	19.25%	3.326%
5	7.445	903	910	916	rBV	1625735	2296872	58.68%	10.139%
6	8.169	1027	1033	1038	rBV	757451	985402	25.18%	4.350%
7	9.245	1209	1216	1221	rBV	2843587	3914141	100.00%	17.279%
8	9.922	1325	1331	1344	rBV	842972	1066221	27.24%	4.707%
9	10.710	1459	1465	1494	rBV	1187285	1594204	40.73%	7.038%
10	11.410	1579	1584	1595	rBV	717492	900639	23.01%	3.976%
11	12.998	1848	1854	1859	rBV	2299201	2967408	75.81%	13.099%
12	14.051	2027	2033	2067	rBV	540373	794053	20.29%	3.505%
13	15.533	2279	2285	2308	rVB	328164	566575	14.48%	2.501%




Sum of corrected areas: 22652916

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140134.D
Acq On : 30 Oct 2024 02:04
Operator : RC/JU
Sample : PB164500BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

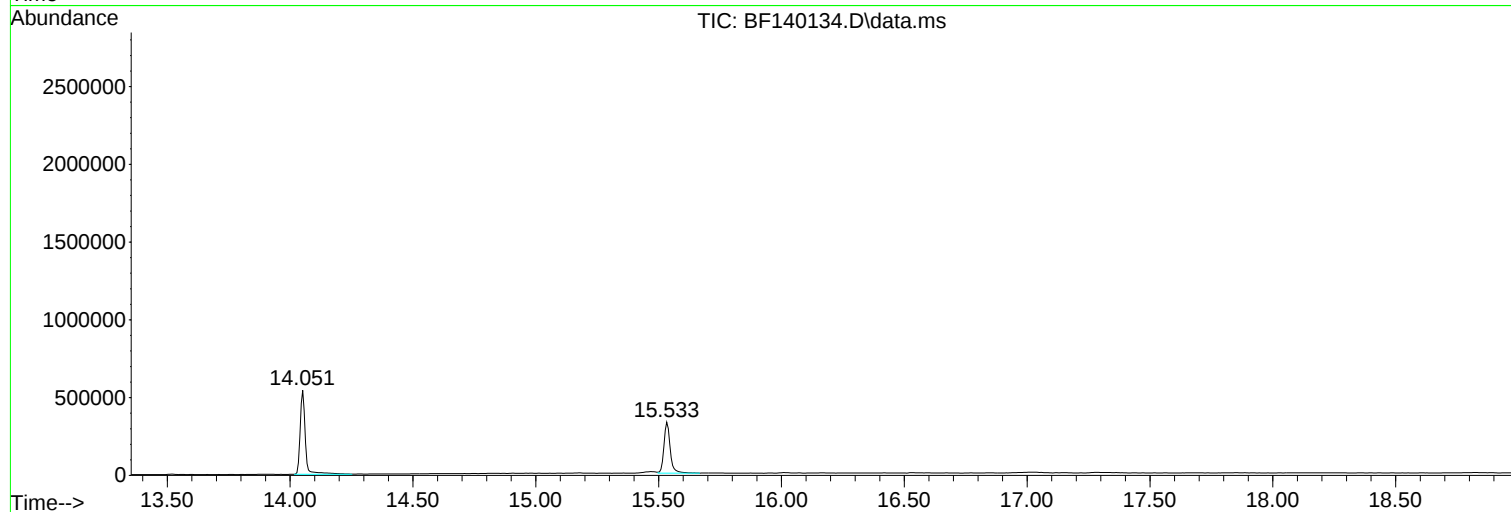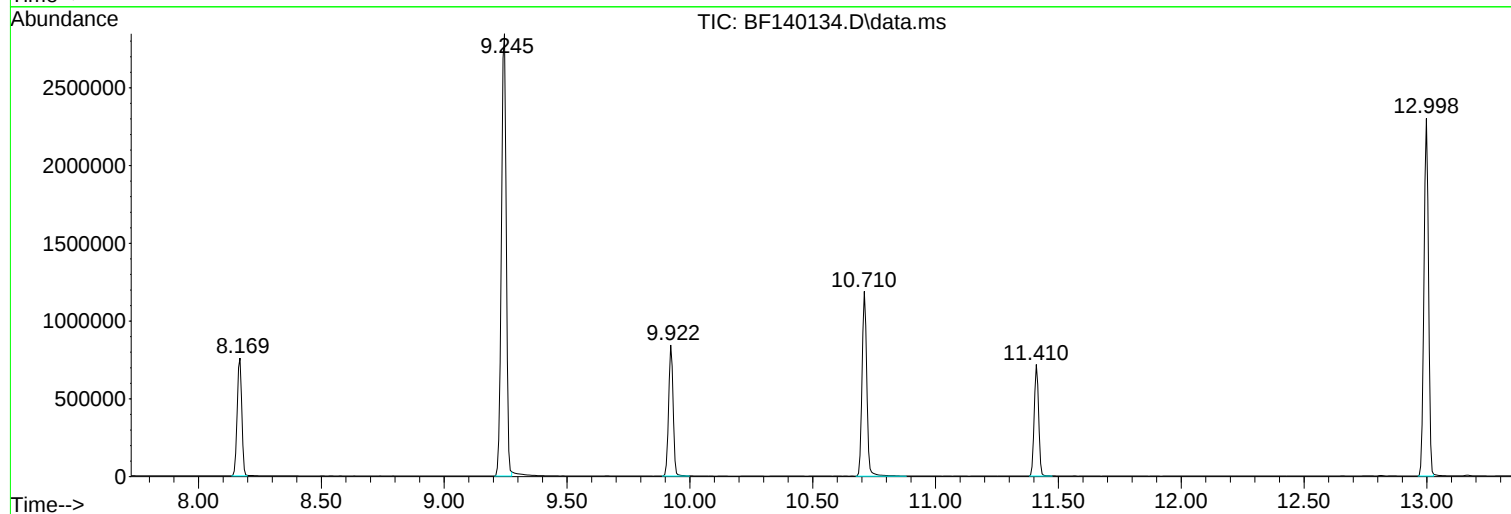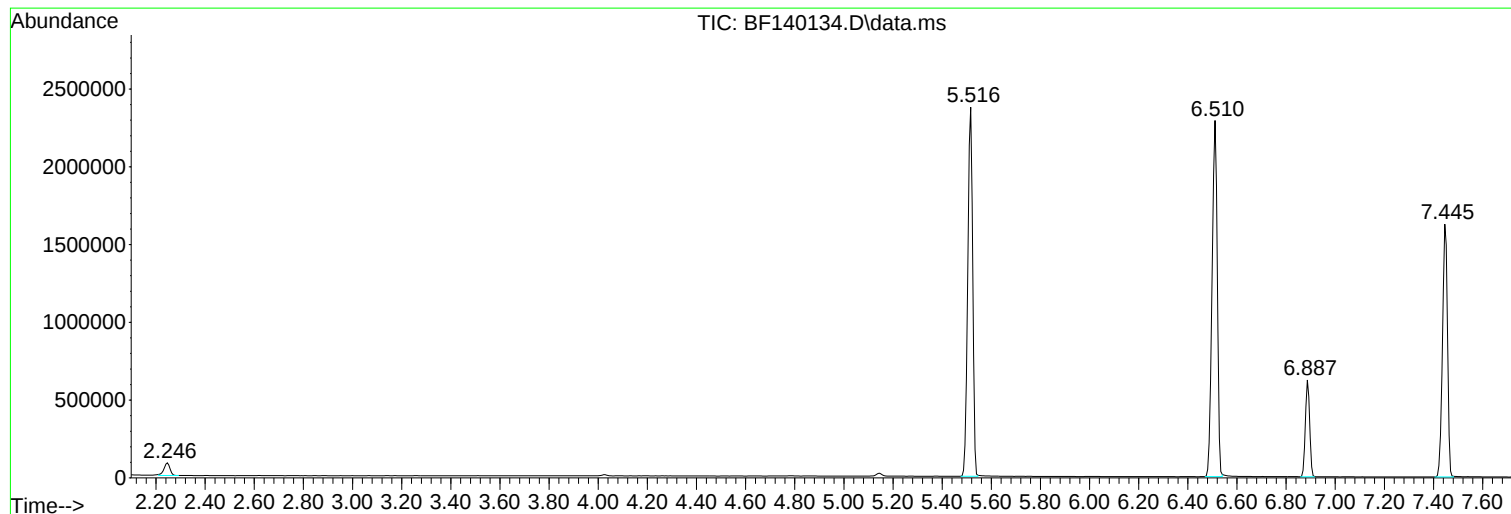

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140134.D
Acq On : 30 Oct 2024 02:04
Operator : RC/JU
Sample : PB164500BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164500BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.246	3.65 ng	137671	1,4-Dichlorobenzene-d4	6.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	17
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

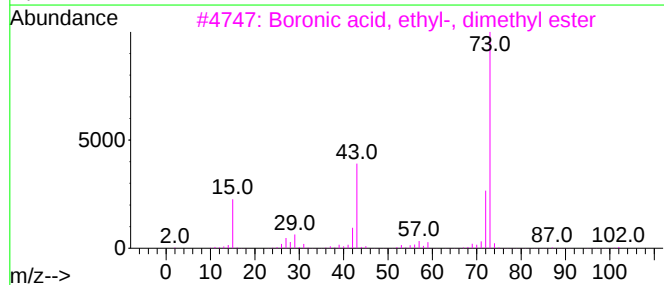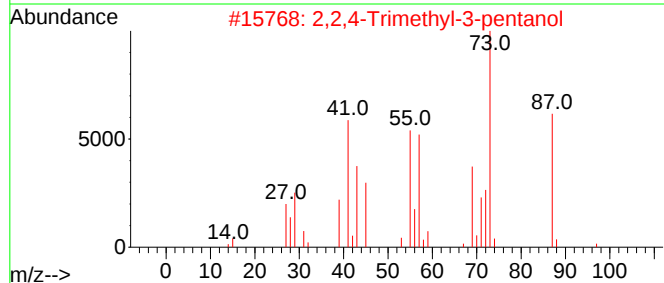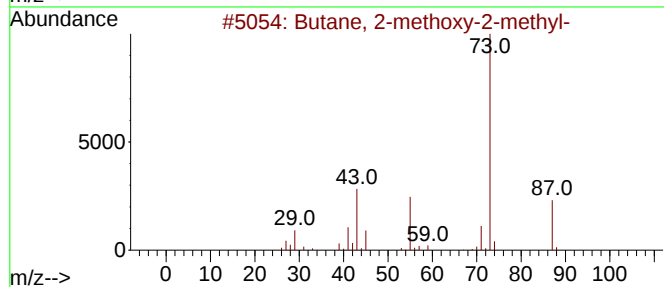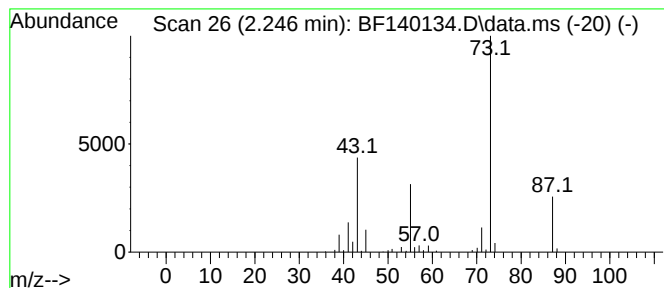

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140134.D
Acq On : 30 Oct 2024 02:04
Operator : RC/JU
Sample : PB164500BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.246	3.6	ng	137671	1	6.887	753518	20.0