
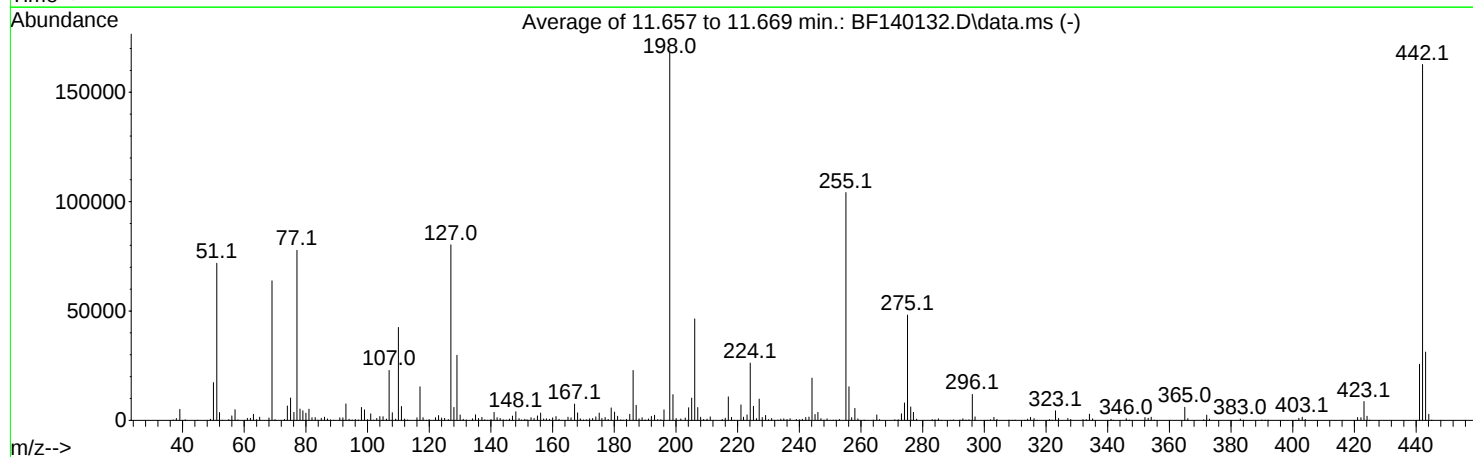


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140132.D
Acq On : 30 Oct 2024 00:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

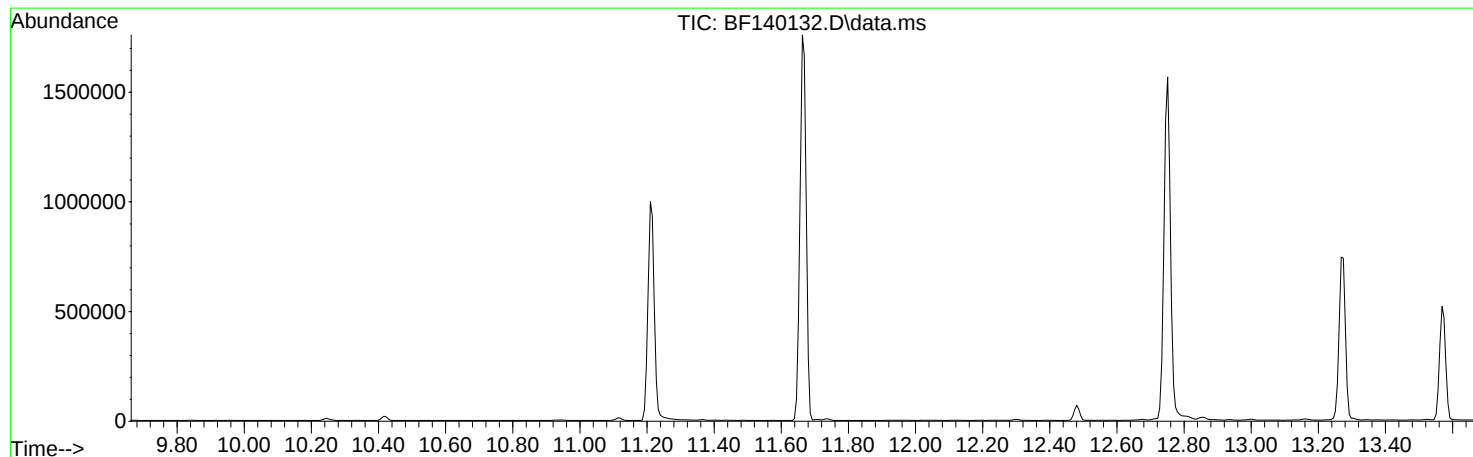




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	71835	PASS
68	69	0.00	2	1.8	1119	PASS
69	198	0.00	100	37.9	63813	PASS
70	69	0.00	2	0.6	351	PASS
127	198	10	80	47.7	80259	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	168181	PASS
199	198	5	9	7.0	11801	PASS
275	198	10	60	28.6	48115	PASS
365	198	1	100	3.6	6009	PASS
441	198	0.01	100	15.3	25685	PASS
442	442	50	100	100.0	162675	PASS
443	442	15	24	19.2	31224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140132.D
Acq On : 30 Oct 2024 00:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 30 01:34:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

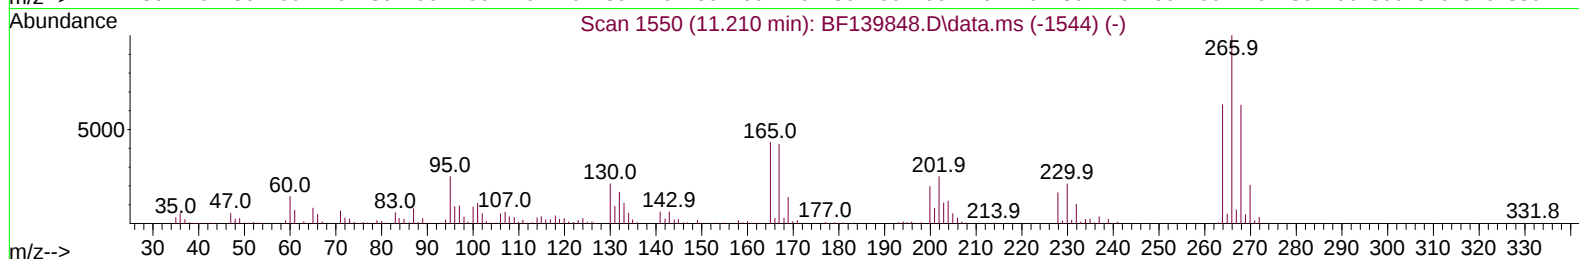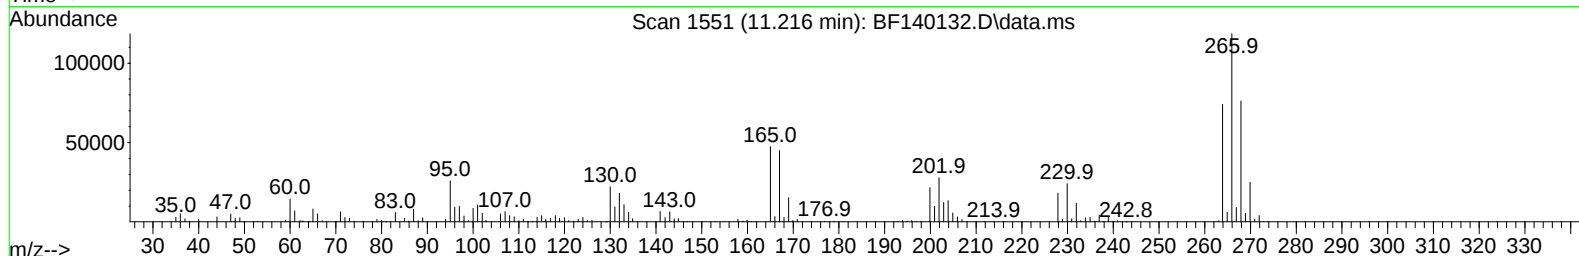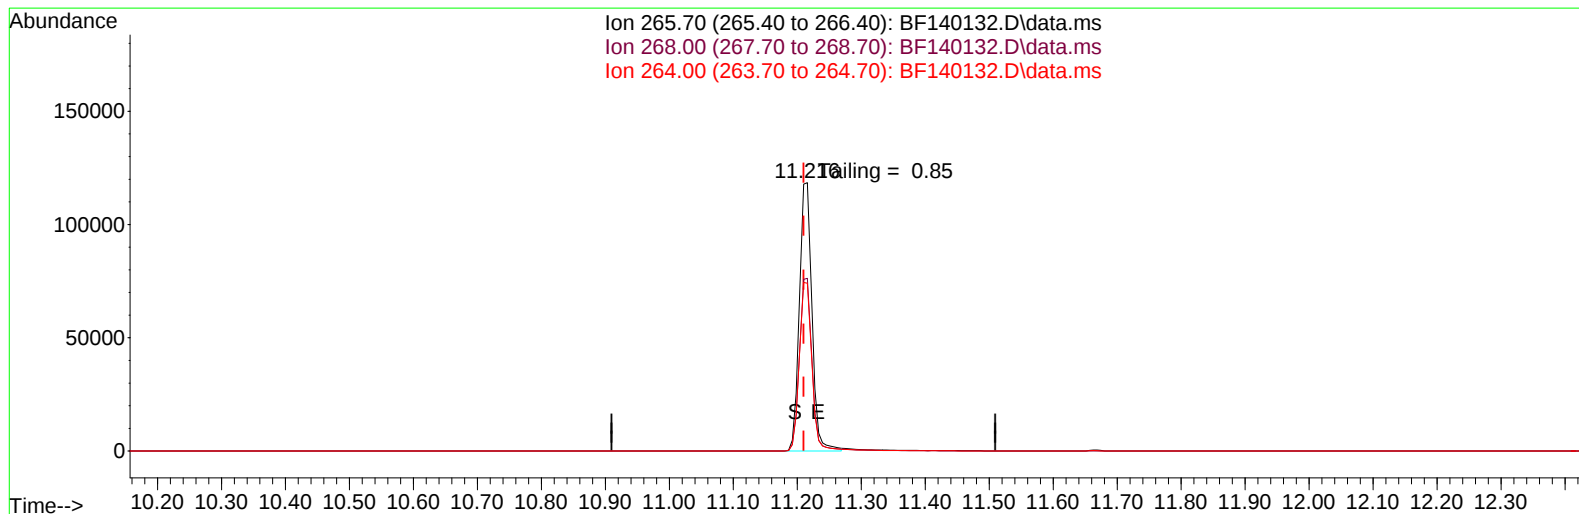

TIC: BF140132.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 102072.82 ng m




response 162211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.34
264.00	63.20	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140132.D
Acq On : 30 Oct 2024 00:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 30 01:34:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

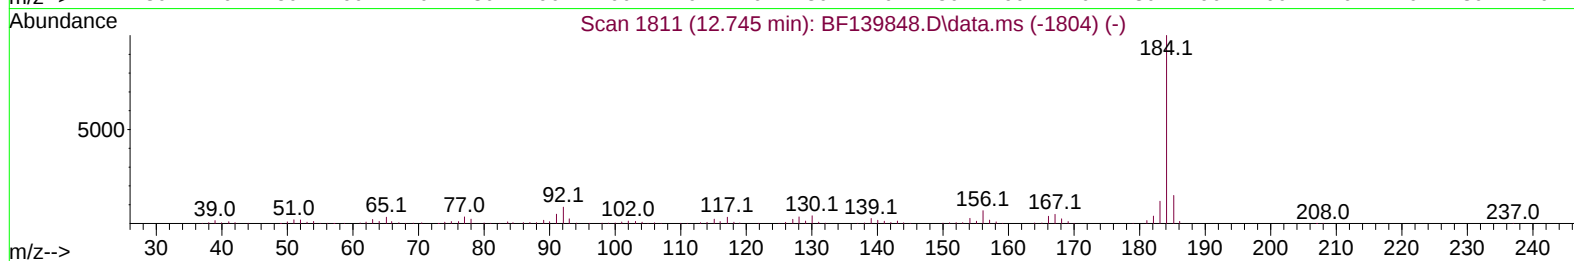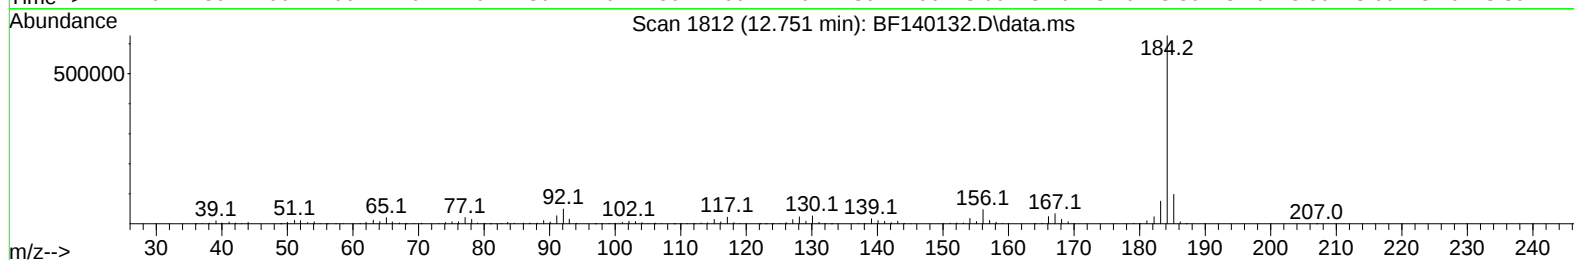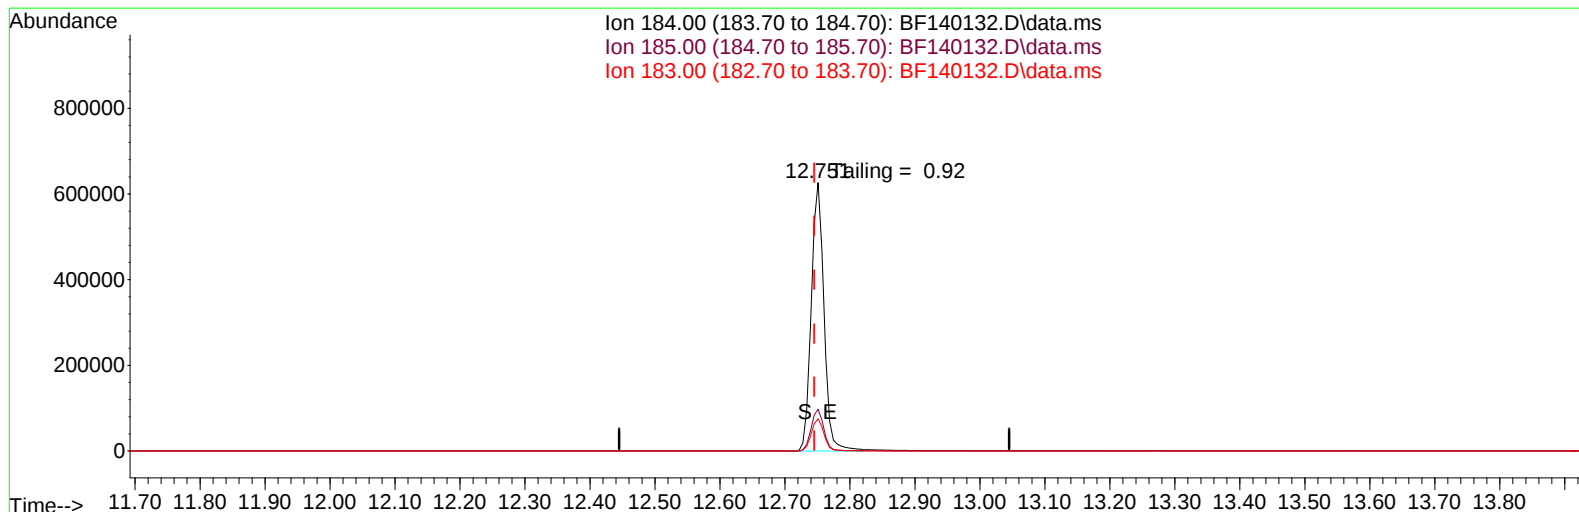

TIC: BF140132.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 127164.54 ng

response 861499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.59
183.00	11.80	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2024	BNA_F	<u>BF140112.D</u>
Compound Name	Response	Retention Time
DDT	128298	13.569
DDD	203048	13.274
DDE	543	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
203591	331889	61.34

Instrument :
BNA_F
ClientSampleId :
DFTPP