
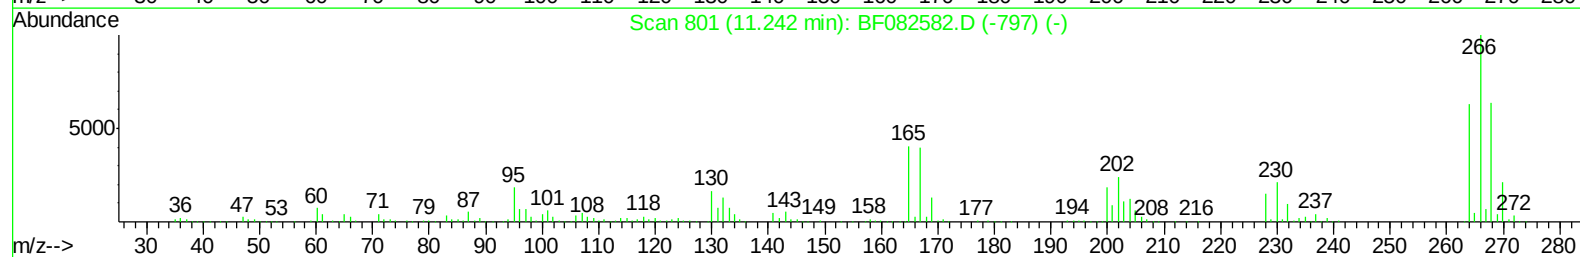
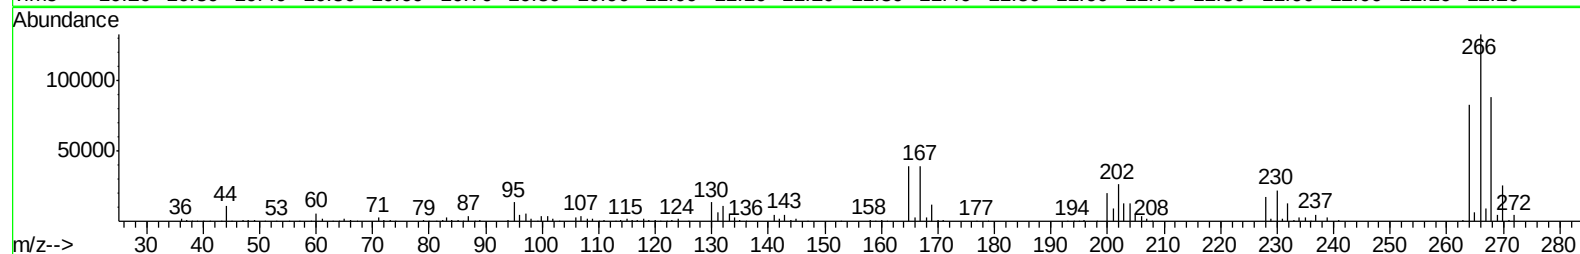


Data Path : Z:\HPCHEM1\BNA_F\Data\BF103015\
Data File : BF082578.D
Acq On : 30 Oct 2015 17:36
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 08:13:22 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

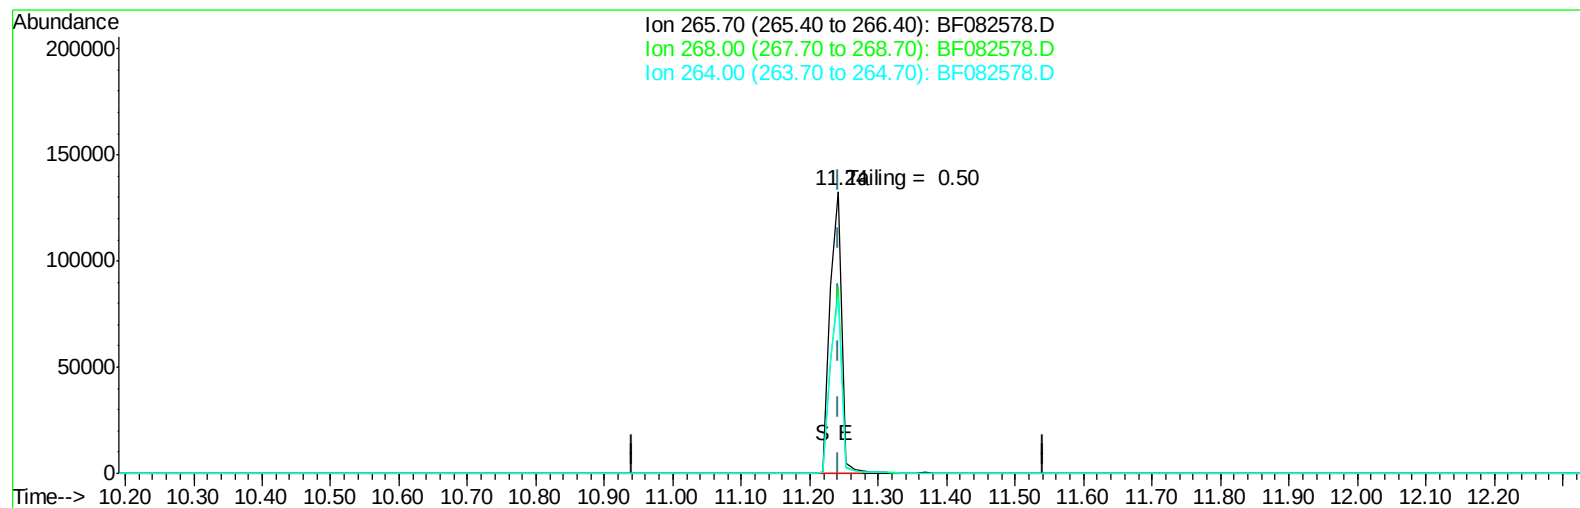

TIC: BF082578.D

(69) Pentachlorophenol (C)




11.242min (+0.000) 0.00ng

response 159094

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	66.35
264.00	63.20	62.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF103015\
Data File : BF082578.D
Acq On : 30 Oct 2015 17:36
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 08:13:22 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 31 00:17:39 2015
Response via : Initial Calibration

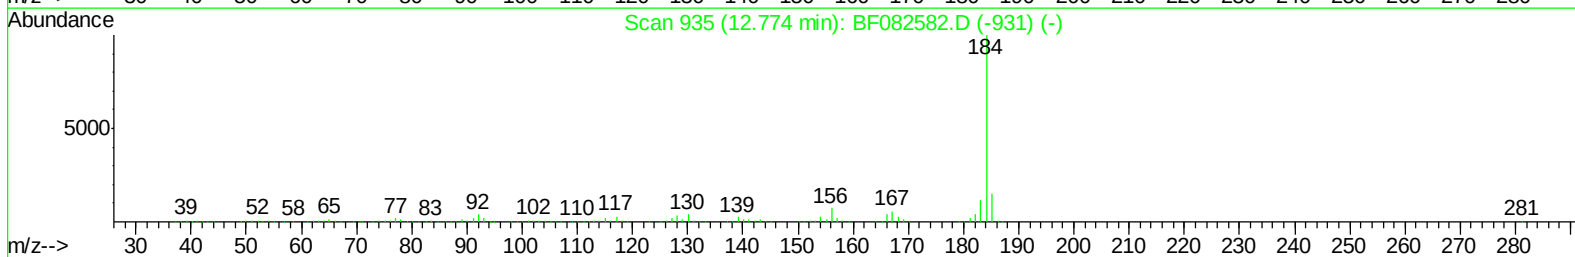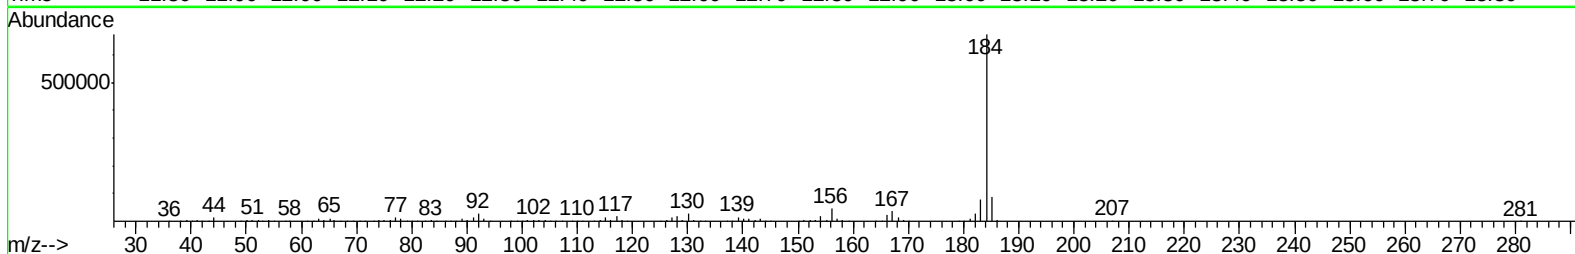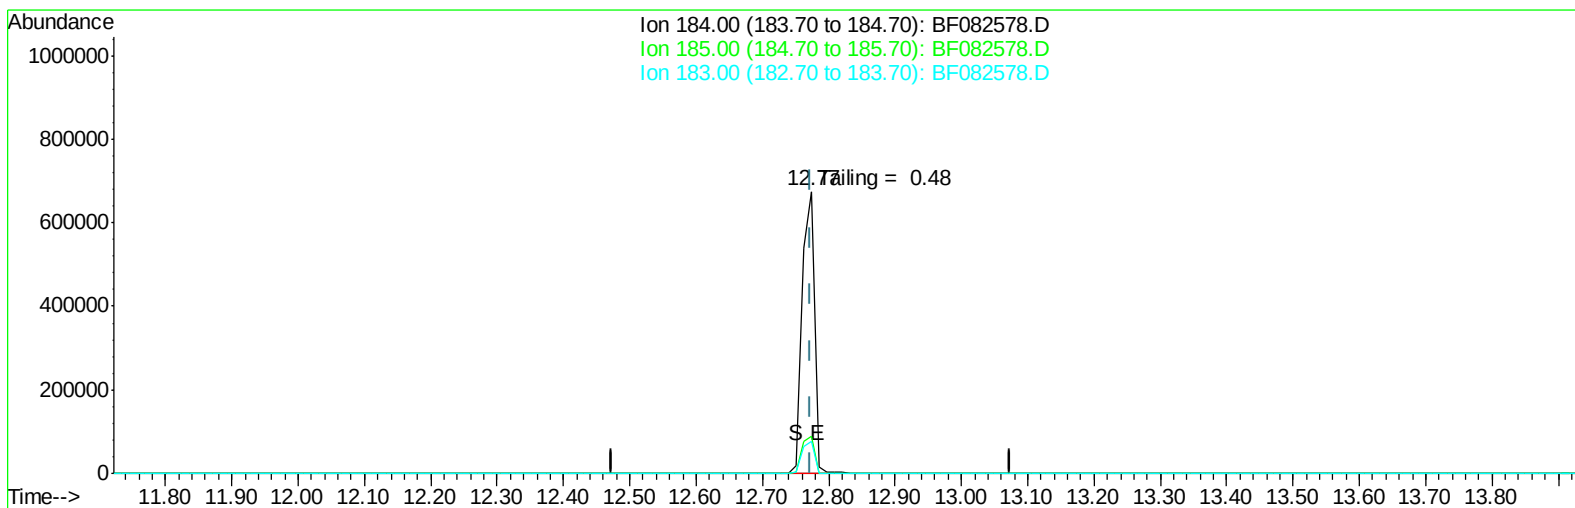

TIC: BF082578.D

(76) Benzidine

12.774min (+0.000) 83918.41ng m

response 859114

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.36
183.00	12.00	11.42
0.00	0.00	0.00