
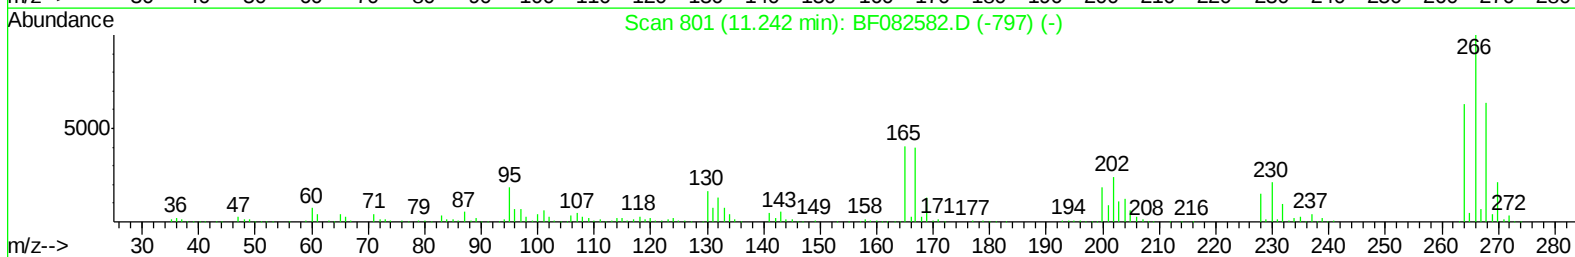
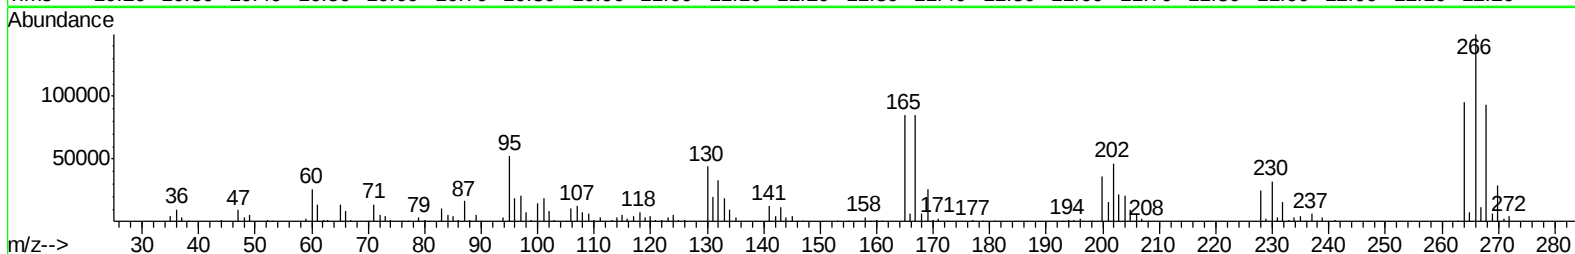


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF103015\  
Data File : BF082601.D  
Acq On : 31 Oct 2015 5:24  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:19:54 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF103015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 31 00:17:39 2015  
Response via : Initial Calibration

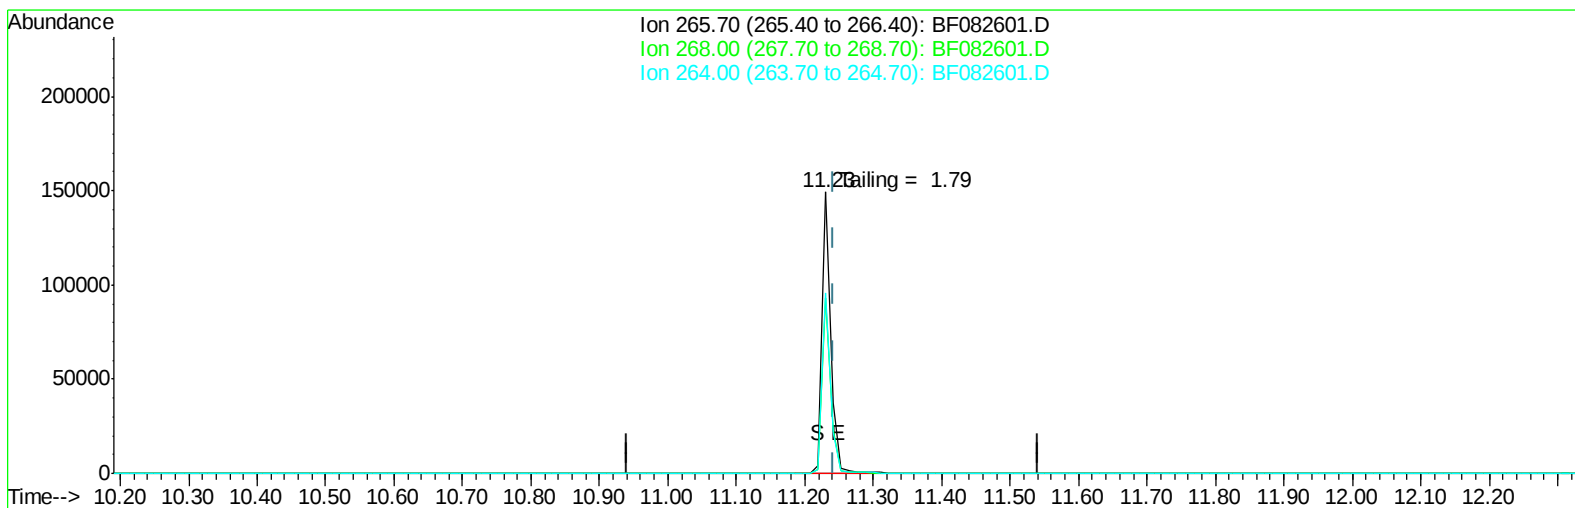

TIC: BF082601.D

(69) Pentachlorophenol (C)




11.231min (-0.011) 0.00ng

response 135618

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.80 | 62.41 |
| 264.00 | 63.20 | 63.93 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF103015\  
Data File : BF082601.D  
Acq On : 31 Oct 2015 5:24  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:19:54 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF103015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 31 00:17:39 2015  
Response via : Initial Calibration

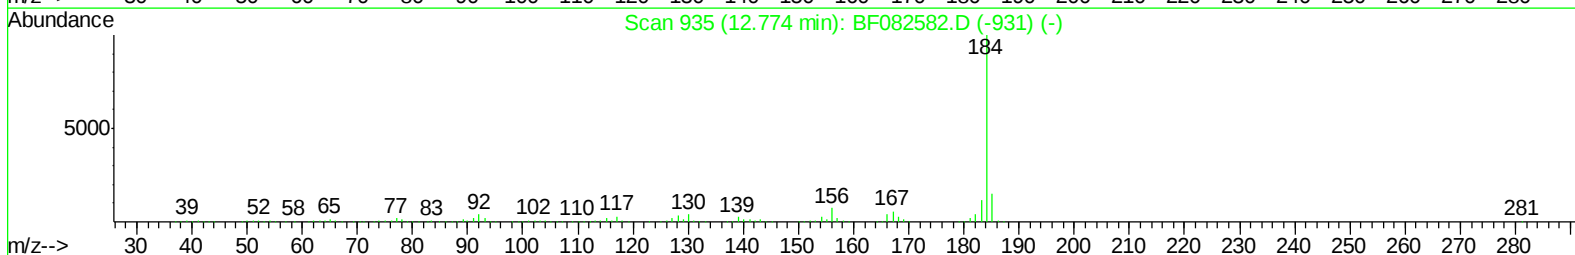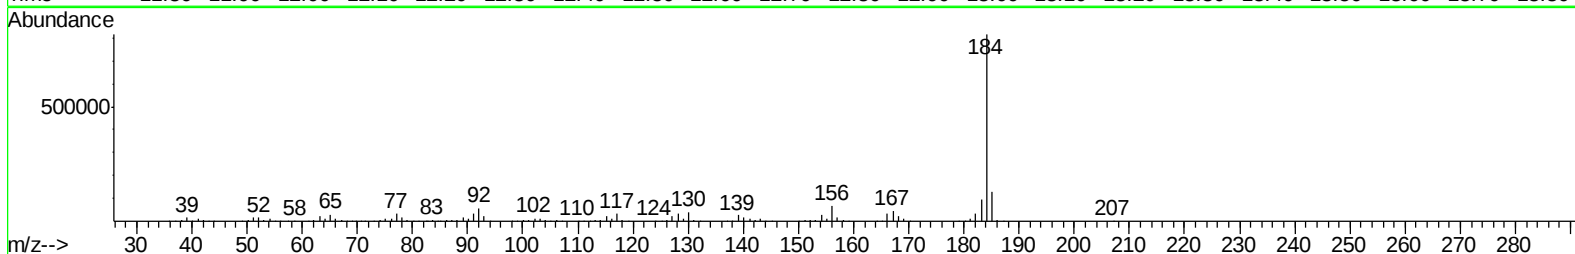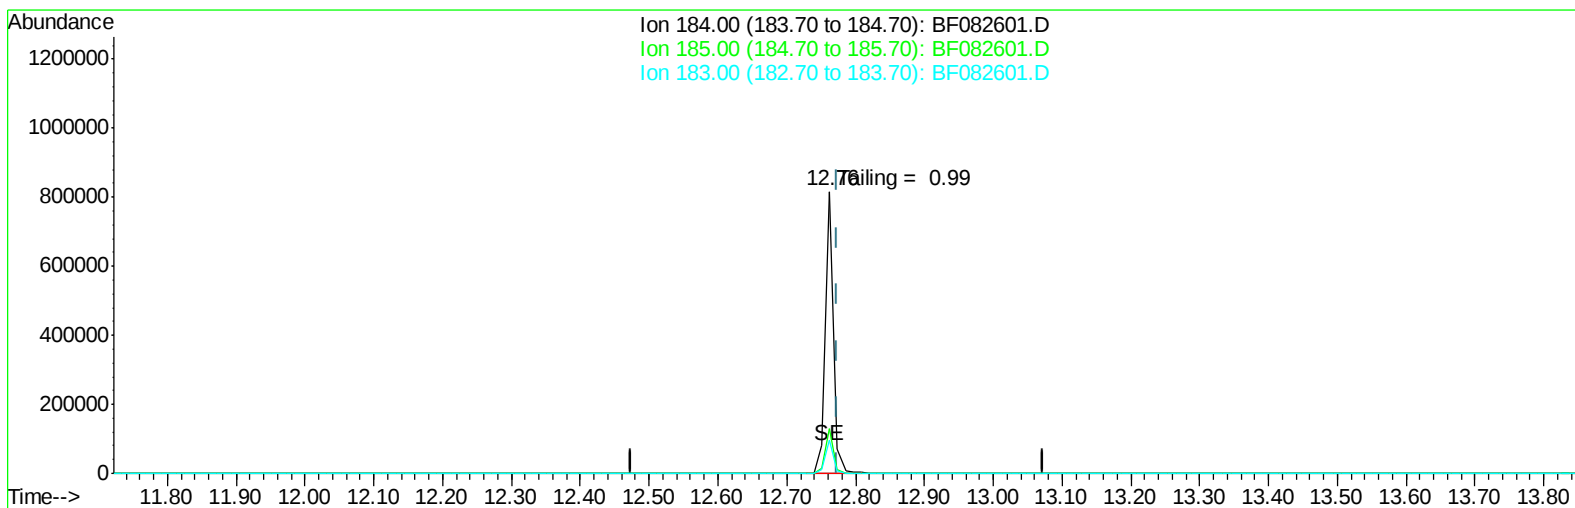

TIC: BF082601.D

(76) Benzidine

12.762min (-0.011) 0.00ng

response 674021

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.00 | 15.83 |
| 183.00 | 12.00 | 11.80 |
| 0.00   | 0.00  | 0.00  |